GG-D-00444b(DSA-DM)
19 January 1968.
Interim Revision of
Fed. Spec. GG-D-444a
19 April 1957

INTERIM FEDERAL SPECIFICATION

DISPENSER, COTTON PELLET, DENTAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-D-444a.

1. SCOPE

1.1 Scope. This specification covers a cotton pellet holder and dispenser suitable for use in dental offices.

2. APPLICABLE DOCUMENTS

2.1 The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
MMM-A-250	Adhesive, Water-Resistant, (For Sealing Fiberboard Boxes).
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper, (For Carton Sealing).

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-123 Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Copies of Military specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Dispensers shall be fabricated of either of the following materials as specified (see 6.1).

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:50Z
Check the source to verify that this is the current version before use.

3.1.1 Brass. Brass shall conform to requirements of class 8, alloy number 260 of GG-I-526.

3.1.2 Carbon steel. Carbon steel shall conform to class 1, type 1010 of GG-I-526.

3.2 Style, design, and dimensions. Cotton-pellet dispensers shall be designed for use on a bracket table and shall conform to figure 1 in style and dimensions. They shall be circular in form, with thirteen openings in the top for withdrawal of cotton pellets. The sides of the holder may taper as shown in figure 1 or may be straight.

3.3 Finish. The entire surface of the dispenser shall be plated as indicated in GG-I-526 for the respective class 1 or class 8 material. Exposed surfaces shall have a mirror finish.

3.4 Corrosion resistance. Corrosion tests (salt spray and boil tests) as specified in GG-I-526, shall apply.


3.5 Workmanship. The workmanship shall be first class throughout. The finished holders shall be free from defects which detract from their appearance or may impair their serviceability.


4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

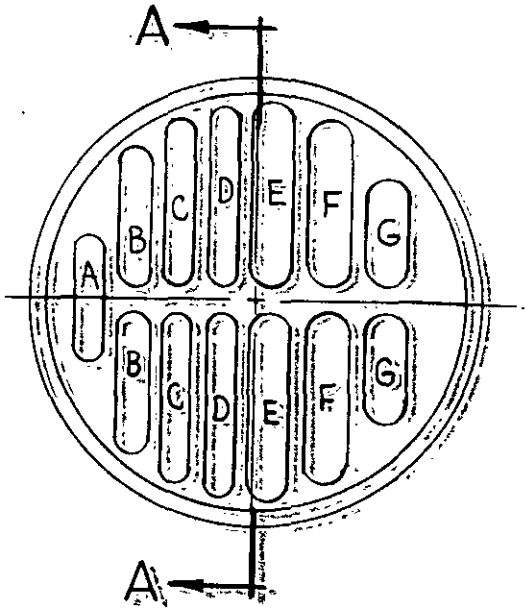

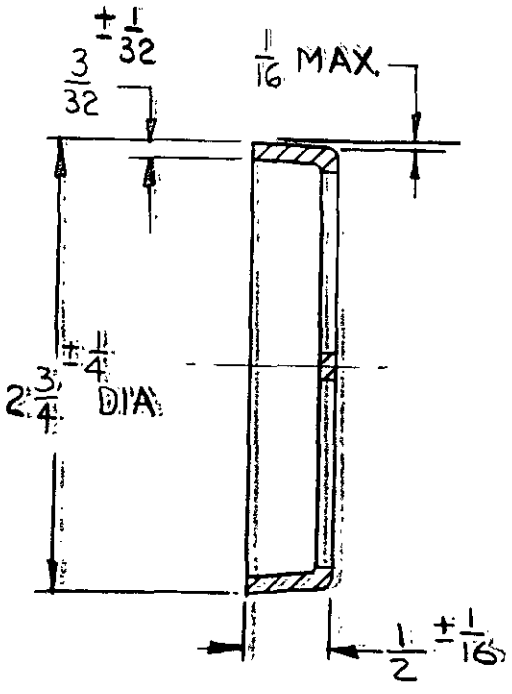

SECTION A-A

OPENINGS	SIZE
A	3/16 × 3/4
B	3/16 × 7/8
C	3/16 × 1 1/16
D	3/16 × 1 1/8
E	1/4 × 1 1/8
F	1/4 × 1
G	1/4 × 5/8

NOTE:
ALL DIMENSIONS ARE IN INCHES
TOLERANCE: WIDTH OF OPENING ±1/32
LENGTH OF OPENING ±1/16

FIGURE 1. DENTAL COTTON PELLET DISPENSER

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:50Z
Check the source to verify that this is the currentversion before use.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection level and acceptable quality level (AQL) shall be as indicated in table I.

Table I. Inspection and Acceptable Quality Levels

Type defect	Inspection level	Acceptable quality level (percent defective)
Major	II	1.0
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II, except that the acceptance number shall be zero for all sample sizes.

Table II. Tests

Characteristic	Requirement	Test procedure	Inspection level
Plating	3.3 and GG-I-526	4.4	S-2
Salt spray test	3.4 and GG-I-526	4.4	S-2
Boil test	3.4 and GG-I-526	4.4	S-2
Composition	3.1.1 and 3.1.2	4.4	*

* Sufficient amount of each lot of metal used in the construction of the dispensers shall be selected for composition analysis.

4.3 Examination. Dispensers shall be examined for defects including, but not limited to, those listed in table III.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

Categories	Defects
Critical:	None defined.
Major:	
101	Plating shows signs of peeling or flaking.
102	Openings in top of dispenser have rough edges.
103	Dispenser surfaces show signs of corrosion.
104	Edges of dispenser have burs or sharp edges.
105	Style and design of dispenser not as specified.
106	Dispenser shows fabrication imperfections such as cracks and tears.
Minor A:	
201	Plated surfaces show scratches and other surface imperfections.
202	Finish not mirror on exposed surfaces.
203	Packaging and marking not as specified.
Minor B:	
251	Dispenser dimensions not as specified.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements. Test procedures shall be as specified in GG-I-526.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One dispenser, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2-inch wide tape conforming to PPP-T-76. Closing of bottom flap with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with appendix of applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, constructed so as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Material required (see 3.1).

(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.