GG-D-441b

MAY 1, 1957

SUPERSEDING
Int. Fed. Spec. GG-D-00441a(GSA-FSS)
August 24, 1956, and
Fed. Spec. GG-D-441
~~December~~ 6, 1946

FEDERAL SPECIFICATION

DISPENSER; STRIP, DENTAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers dispensers for strip articulating paper and strip matrix bands used in dentistry.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

PPP-B-566 — Boxes, Folding, Paperboard.

PPP-B-585 — Boxes; Wood, Wirebound.

PPP-B-601 — Boxes, Wood, Cleated-Plywood.

PPP-B-621 — Boxes, Wood, Nailed and Lock-Corner.

PPP-B-676 — Boxes, Set-Up, Paperboard.

Federal Standard:

Fed. Std. No. 102—Preservation, Packaging and Packing Levels.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL-B-10377 — Box; Wood, Cleated, Veneer, Paper Overlaid.

MIL-L-10547 — Liners, Case, Waterproof.

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL-STD-129 — Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by the contractor in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material.—The dispensers shall be of molded plastic of a composition suitable for the intended purpose. Bidders under this specification shall state the type of plastic they propose to use.

3.2 Bid sample.—When specified, sample shall be furnished with bid for the purpose of determining conformance to the requirements of this specification with respect to material, design, construction, and dimensions.

3.3 Design.—The dispensers shall be provided with an outlet channel and finger control for dispensing the material in lengths desired. Style and design of dispenser shall be as indicated in figure 1.

3.4 Construction.—The dispensers shall be of two-piece construction, consisting of roll holder and cover. The construction shall be such that the parts may be easily taken apart and assembled, and the runway for the material shall permit free and easy passage.

3.5 Dimensions.—The dispensers shall be approximately 1.875 inches in diameter and 0.75 inch in depth, with a wall thickness of approximately 0.063 inch. The outlet channel shall extend from the bottom of the roll holder approximately 1.25 inches and shall accommodate material 0.625 inch in width and 0.009 inch in thickness.

3.6 Color.—The dispensers shall be either brown or black.

3.7 Workmanship.—The workmanship shall be first class in every respect. The dispensers shall be symmetrically made and smoothly and properly finished.

4. SAMPLING, INSPECTION AND TEST PROCEDURES

4.1 Sampling.—Unless otherwise specified, samples shall be submitted in accordance

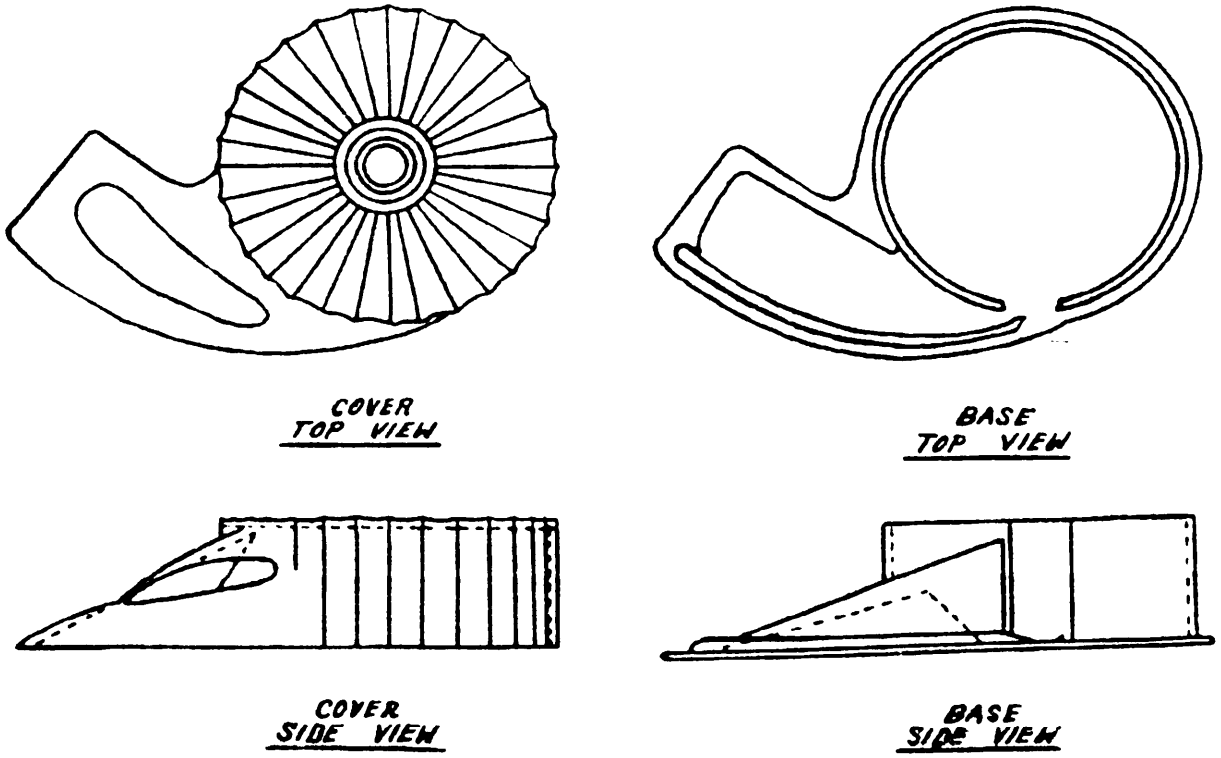


FIGURE 1.—Dispensers; for articulating paper, celluloid, and steel rolls (dental), and strip matrix bands (dental).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

with instructions furnished by the procuring activity (see 6.2). In addition, sampling procedures shall be conducted in accordance with the procedures set forth in Military Standard MIL-STD-105.

4.2 **Inspection.**—Samples shall be carefully inspected for defects in material and workmanship, dimensions, and other applicable requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 *Unit of issue.* — One dispenser, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each unit, intermediate and exterior containers as applicable, for the required level of protection specified in procurement document.

TABLE I.—*Packaging quantities*

Federal Stock Number	Unit package	Intermediate package	Shipping container
6520-523-6050 --	1 unit	12 units	288 units

5.1.2.1 *Packing variation permitted.*—If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676. Closure shall be effected in such manner as to prevent spillage of contents under normal handling.

5.1.3.2 *Intermediate package.*—Intermediate package shall be a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676. Closure shall be effected in such manner as to prevent spillage of contents under normal handling.

5.1.4 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be designed for type 3 load and constructed in accordance with Federal Specification PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or Military Specification MIL-B-10377, table II.

5.2.1.2 *Case liner.*—Each box shall be lined with a waterproof case liner conforming to Military Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.* — Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall conform to Federal Specification PPP-B-601, table I, using type III, class 1 plywood, or shall be designed for type 2 load and constructed in accordance with Federal Specification PPP-B-585, style 3, for class 2 use; Federal Specification PPP-B-621,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

table I; or Military Specification MIL–B–10377, table I.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *Unit package.*—Unit package shall be marked with stock number, item identification, unit, quantity, office identifying number, and name of contractor.

5.3.2 *Intermediate package.*—Intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.3 *Shipping container.* — Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color marking and symbol are not required on containers for level A packs when addressed to domestic establishments for the Medical Services of the Armed Forces.

6. NOTES

6.1 Federal Standard No. 102 should be referred to for definitions and applications of the various levels of packaging protection for supplies and equipment.

6.2 **Ordering data.** — Procurement documents should specify the following:

(*a*) Title, number, and date of this specification.
(*b*) Bid sample required (see 3.2).
(*c*) Sampling required (see 4.1).
(*d*) Selection of applicable level of packaging and packing (see 5.1 and 5.2).

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all types, classes, grades, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the type, etc., normally procured to meet Federal Government requirements.

6.5 **Transportation description.**—Transportation description applicable to this item is:

Holders, Cellulose Tape, Synthetic Plastic
Carload minimum weight 30,000 pounds.

Motor Volume minimum weight 30,000 pounds.

6.6 This specification covers the following item appearing in the Armed Services Medical Stock List:

6520-523-6050—Dispenser, Strip, Dental.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility, nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise, as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTEREST:
Army—M
Navy—Md
Air Force.

Copies of this specification may be purchased for 10 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.