FEDERAL SPECIFICATION

WIRE, SNARE (SPRING STEEL, MEDICAL)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. CLASSIFICATION

1.1 **Type.** — Snare wire covered by this specification shall be of one type, as hereinafter specified.

1.2 **Sizes.**—Snare wire covered by this specification shall be of the following sizes, as specified in the invitation for bids:

Size 24—0.022 inch diameter, 5½ inch lengths (shaped)
Size 27—0.016 inch diameter, 12½ foot lengths
Size 28—0.014 inch diameter, 9 foot lengths
Size 31—0.010 inch diameter, 11½ foot lengths

2. APPLICABLE SPECIFICATION

2.1 The following Federal Specification of the issue in effect on date of invitation for bids, forms a part of this specification:

QQ-M-151—Metals; General Specification for Inspection of.

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application, accompanied by money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D. C., or to the GSA Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, and Seattle. Prices may be obtained from the Superintendent of Documents or from the GSA Regional Offices.)

2.2 Specifications applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 **Material.** — The wire shall be cold-drawn and shall have a chemical composition conforming to the requirements shown in table I.

TABLE I.—*Chemical composition*

	Minimum percent	Maximum percent
Carbon	0.80	0.95
Manganese	0.30	0.50
Phosphorus	...	0.025
Sulphur	...	0.035
Silicon	0.15	0.30

3.2 **Coiling.** — The wire shall have the physical properties specified in table II and when tested as described in 4.3.2 shall show a uniform pitch with no splits or fractures.

3.3 **Wrapping.**—The wire shall withstand without fracture the test described in 4.3.3.

3.4 **Form.**

3.4.1 *Size 24.* — Size 24 wire shall be furnished in the shape as shown in figure 1.

3.4.2 *Sizes 27, 28, and 31.*—Sizes 27, 28, and 31 wire shall be furnished on spools.

3.5 **Dimensions and physical properties.**— The dimensions and physical properties of the wire shall conform to the requirements shown in table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

TABLE II.—*Dimensions and physical properties*

Size No.	Diameter	Tolerance in diameter	Gage No.		Tensile strength	Length
	Inch	Plus or minus *Inch*	*Music wire*	*Stubs*	*Pounds per square inch*	
24	0.022	0.0003	9	24	355,000 to 380,000	5½ inches ± 1/64 inch
27	0.016	0.0003	6	27	360,000 to 385,000	12½ feet ± 2 inches
28	0.014	0.0003	5	28	365,000 to 395,000	9 feet ± 2 inches
31	0.010	0.0002	1	31	375,000 to 415,000	11½ feet ± 2 inches

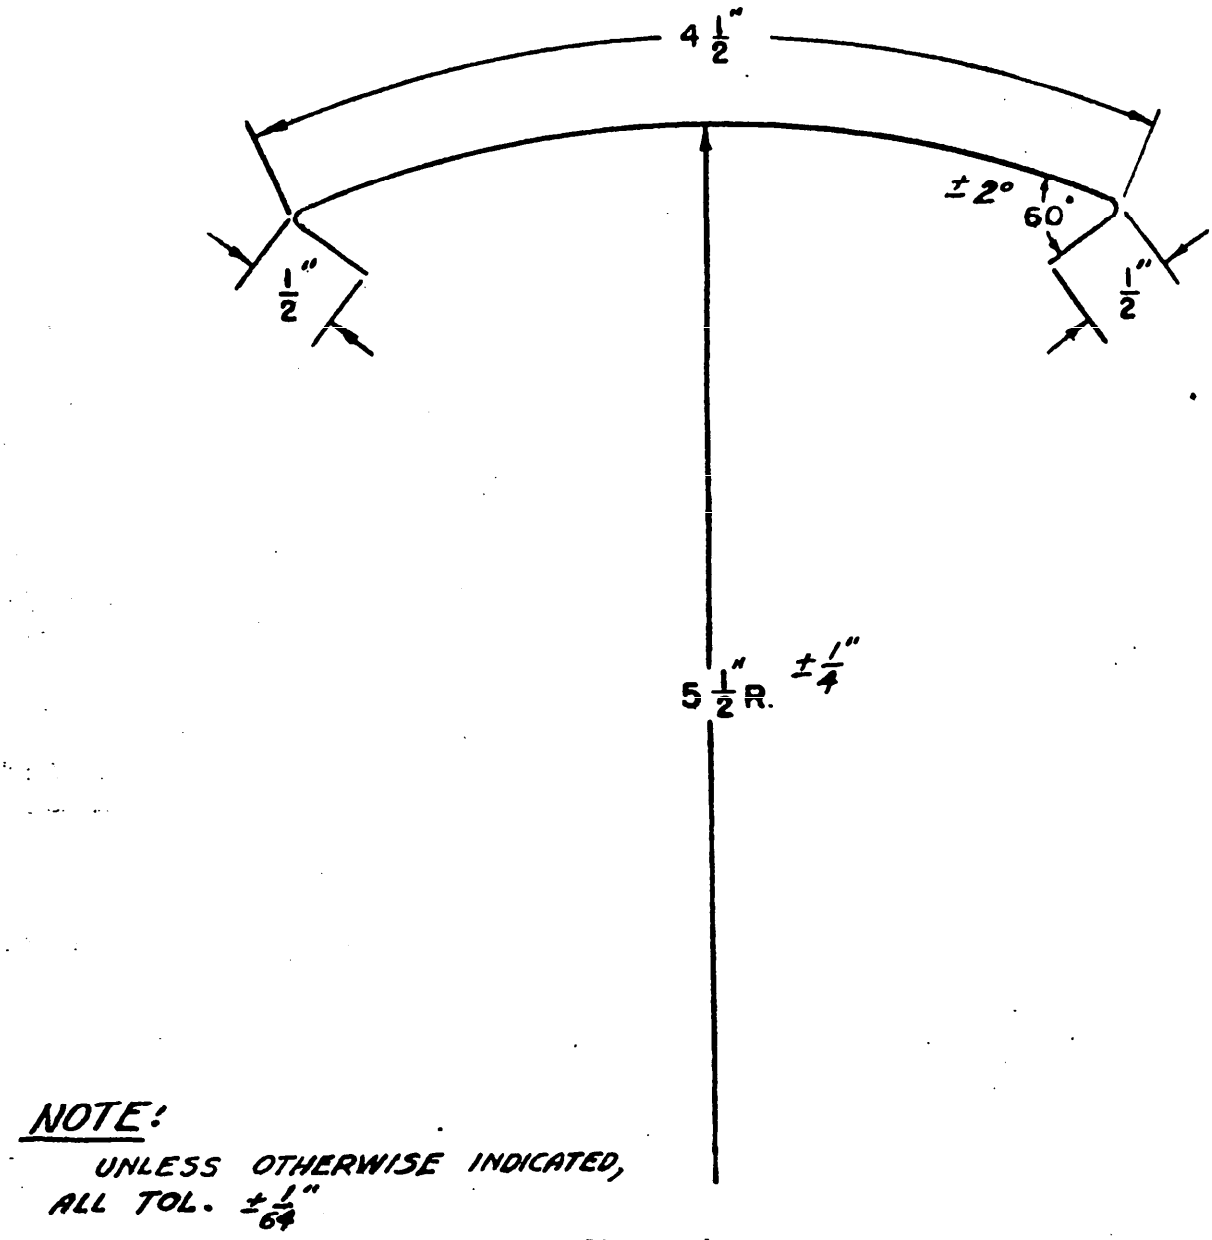


FIGURE 1.—*Size 24 wire snare*

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

3.6 **Workmanship.** — The wire shall be uniform in diameter, quality and temper, cylindrical and shall have a bright, smooth finish, free from pits, die marks, rust, excessive scale, scrapes, splits, laps, cracks, seams, excessive decarburization, and other injurious defects.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *Size 24.*—Unless otherwise specified, at least three samples (not less than 15 inches long) of the same lot of wire from which the wires are made shall be supplied with each delivery.

4.1.2 *Sizes 27, 28, and 31.*—Unless otherwise specified, at least three samples of each size shall be taken at random from each delivery of 200 or fraction thereof.

4.1.3 Unless otherwise specified, in addition to the above, not less than 2 ounces of each size shall be taken for chemical analysis.

4.2 **Inspection.** — Samples shall be inspected for material, dimensions, workmanship, packaging, packing, and marking.

4.3 Tests.

4.3.1 *Chemical analysis.* — The chemical analysis shall be performed in accordance with Federal Specification QQ–M–151. Samples shall consist of not less than 2 ounces.

4.3.2 *Coiling test.* — A length of tightly closed coil shall be wound around an arbor having a diameter approximately 3½ times the diameter of the wire and a 5-inch length of coil shall be stretched so that it sets to approximately three times its original length.

4.3.3 *Wrapping test.*—One sample of each size shall be wrapped eight consecutive turns, with pitch approximately equal to the diameter of the wire, around a wire of like diameter. The sample shall be examined for conformance to requirements of 3.3.

4.3.4 *Tensile strength.* — The tensile strength shall be determined in accordance with the tension test of Federal Specification QQ–M–151. The specimen shall be straight and not less than 15 inches long. The distance between the jaws of the testing machine, with specimen in place for testing, shall be not less than 10 inches.

5. PREPARATION FOR DELIVERY

5.1 **Packaging.**—Unless otherwise specified, snare wire shall be packaged in accordance with accepted commercial practice.

5.2 **Packing.** — The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Packages.*—Unless otherwise specified, packages shall be marked with the name and size of the commodity, the quantity contained therein, and the names of the manufacturer and the contractor.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name and size of the commodity as defined by the contract or order under which the shipment is made, quantity contained therein, name of the contractor, number of the contract or order, name and address of the consignee, and the gross weight.

6. NOTES

6.1 **Ordering data.** — Purchasers should specify size required and should exercise any

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

desired options offered herein. (See 1.2, 4.1, 5.1, 5.3, 6.2, and 7.2.5).

6.2 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.3 This specification covers the following items listed in the Armed Services Catalog of Medical Materiel and the Veterans Administration Supply Catalog No. 3:

3–674–140—Wire, Snare, No. 28 Stubs Gage: For ear snares.

3–674–142—Wire, Snare, No. 31 Stubs Gage: For ear snares.

3–674–780—Wire, Snare, No. 27 Stubs Gage: For nasal snares.

3–676–500—Wire, Snare, No. 24 Stubs Gage: For tonsil snares.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., normally procured to meet Federal Government requirements.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications.*

Federal Specification:

NN–B–621—Boxes, Wood, Nailed and Lock-Corner.

Military Specifications:

JAN–P–106—Packaging and Packing for Overseas Shipment — Boxes, Wood, Nailed.

JAN–P–120—Packaging and Packing for Overseas Shipment — Cartons, Folding, Paperboard.

JAN–P–125—Packaging and Packing for Overseas Shipment—Barrier-Materials, Waterproof, Flexible.

JAN–P–133—Packaging and Packing for Overseas Shipment — Boxes, Set-Up, Paperboard.

JAN–P–140—Packaging and Packing for Overseas Shipment — Adhesives, Water-Resistant, Case-Liner.

MIL–M–3157—Marking of Domestic Shipments by Contractors for Supplies and Equipment Consigned to the Medical Departments of the Armed Services.

Navy Department Specification:

General Specifications for Inspection of Material.[1]

(Copies of specifications, standards, and drawings required by the contractor in connection with specific procurement functions should be obtained from the procuring agency or as directed by the contracting officer.)

7.2.2 *Packaging.*

[1] Applicable to Navy purchases only.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

7.2.2.1 *Size 24.*

7.2.2.1.1 *Unit packaging.* — Twelve wires constitute one unit. Each unit shall be packaged in a sealed envelope of appropriate size and design.

7.2.2.1.2 *Intermediate packaging.*—Forty-eight packages (48 units) shall be packaged in a carton of appropriate size conforming to the requirements of Military Specification JAN–P–133. Each carton shall be adequately secured to prevent accidental opening.

7.2.2.2 *Sizes 27 and 31.*

7.2.2.2.1 *Unit packaging.* — One spool of wire constitutes one unit. Each spool (1 unit) shall be wrapped in anti-corrosive paper.

7.2.2.2.2 *Intermediate packaging.*—Twelve packages (12 units) shall be packaged in a carton of appropriate size conforming to the requirements of Military Specification JAN–P–120 or JAN–P–133. Each carton shall be adequately secured to prevent accidental opening.

7.2.3 *Packing.*

7.2.3.1 *Domestic.*—The number of intermediate packages specified in table III shall be packed in a shipping container conforming to the requirements of Federal Specification NN–B–621.

TABLE III.—*Number of packages in shipping container*

Sizes	Number of intermediate packages in each shipping container	Total number of unit packages in each shipping container
24	30	1440
27	120	1440
31	120	1440

7.2.3.2 *Overseas.*—The number of packages specified in table III shall be packed in a shipping container designed for type 2 load and conforming to the requirements of Military Specification JAN–P–106. Closure and strapping shall conform to the requirements of the appendix thereto. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Military Specification JAN–P–125 for case liners; seams and closures shall be completely sealed with a continuous seam at least ¾ inch wide of water-resistant adhesive conforming to the requirements of Military Specification JAN–P–140.

7.2.3.3 *Packing variation permitted.* — If the number of units in any shipment is not the exact multiple of the number of units specified to be contained in each shipping container, the units not constituting the nearest such multiple shall be packed in a shipping container of suitable size and design, so constructed as to insure safe delivery to specified destination.

7.2.4 *Marking.*

7.2.4.1 *Packages.*—Each unit package and each intermediate package shall be marked with the stock number, nomenclature, unit, quantity, and the name of the contractor. When the contractor is not the manufacturer, the name of the manufacturer shall also appear, as the manufacturer.

7.2.4.2 *Shipping containers.*

7.2.4.2.1 *Domestic.* — Each shipping container shall be marked in accordance with the requirements of Military Specification MIL–M–3157.

7.2.4.2.2 *Overseas.* — Each shipping container shall be marked as specified by the procuring agency.

7.2.5 *Ordering data.*—Procurement docu-

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

ments should specify whether the subject commodity is to be packed, and shipping containers marked for domestic or overseas shipment (see 7.2.3 and 7.2.4.2).

7.2.6 *Inspection procedures (Navy only).*— The general inspection procedures shall be in accordance with Navy Department Specification, General Specifications for Inspection of Material.

NAVY INTEREST: Md

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. (Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION

ORGANIZATION *(Of submitter)*

CITY AND STATE

CONTRACT NO.

QUANTITY OF ITEMS PROCURED

DOLLAR AMOUNT
$

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)*

DATE

DD FORM 1 APR 63 1426 REPLACES NAVSHIPS FORM 4863, WHICH IS OBSOLETE PLATE NO. 15419

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

FOLD

DEPARTMENT OF THE NAVY

POSTAGE AND FEI
NAVY DEPARTI

OFFICIAL BUSINESS

FOLD

PLATE NO. 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.