A-A-0051942(DM)
20 May 1987

INTERIM COMMERCIAL ITEM DESCRIPTION

FORCEPS, THORACIC (Mixter)

The General Services Administration has authorized the use of this interim commercial item description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This interim commercial item description covers a curved thoracic forceps (clamp) of the Mixter design.

Salient characteristics.

General. Forceps shall be in accordance with American Society for Testing and Materials (ASTM) Standard F1026, except as specified herein.

Hardness. Forceps shall have a Rockwell hardness of HRC 40-48.

Style and design. Forceps shall be in accordance with Figure 1.

Passivation. The forceps shall be passivated.

Tests. In addition to the tests specified in ASTM F1026, forceps shall be tested for corrosion-resistance as specified under Quality Assurance Provisions.

Markings. In addition to the requirements of ASTM F1026, forceps shall bear the word "stainless."

Workmanship. The forceps shall be processed in such a manner as to be uniform and free from defects which affect life, utility, or appearance.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The forceps shall be examined to determine compliance with all requirements contained in this specification.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:03Z
Check the source to verify that this is the currentversion before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one forceps. Sampling shall be level S-2 with an AQL 1.0.

Corrosion-resistance. Forceps shall be tested for corrosion-resistance in accordance with the Resistance to Boil and Resistance to Copper Sulfate tests of Federal Specification GG-I-526.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8938	FORCEPS, THORACIC, Curved, Mixter

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 50992

Project No. 6515-4104

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:03Z
Check the source to verify that this is the currentversion before use.

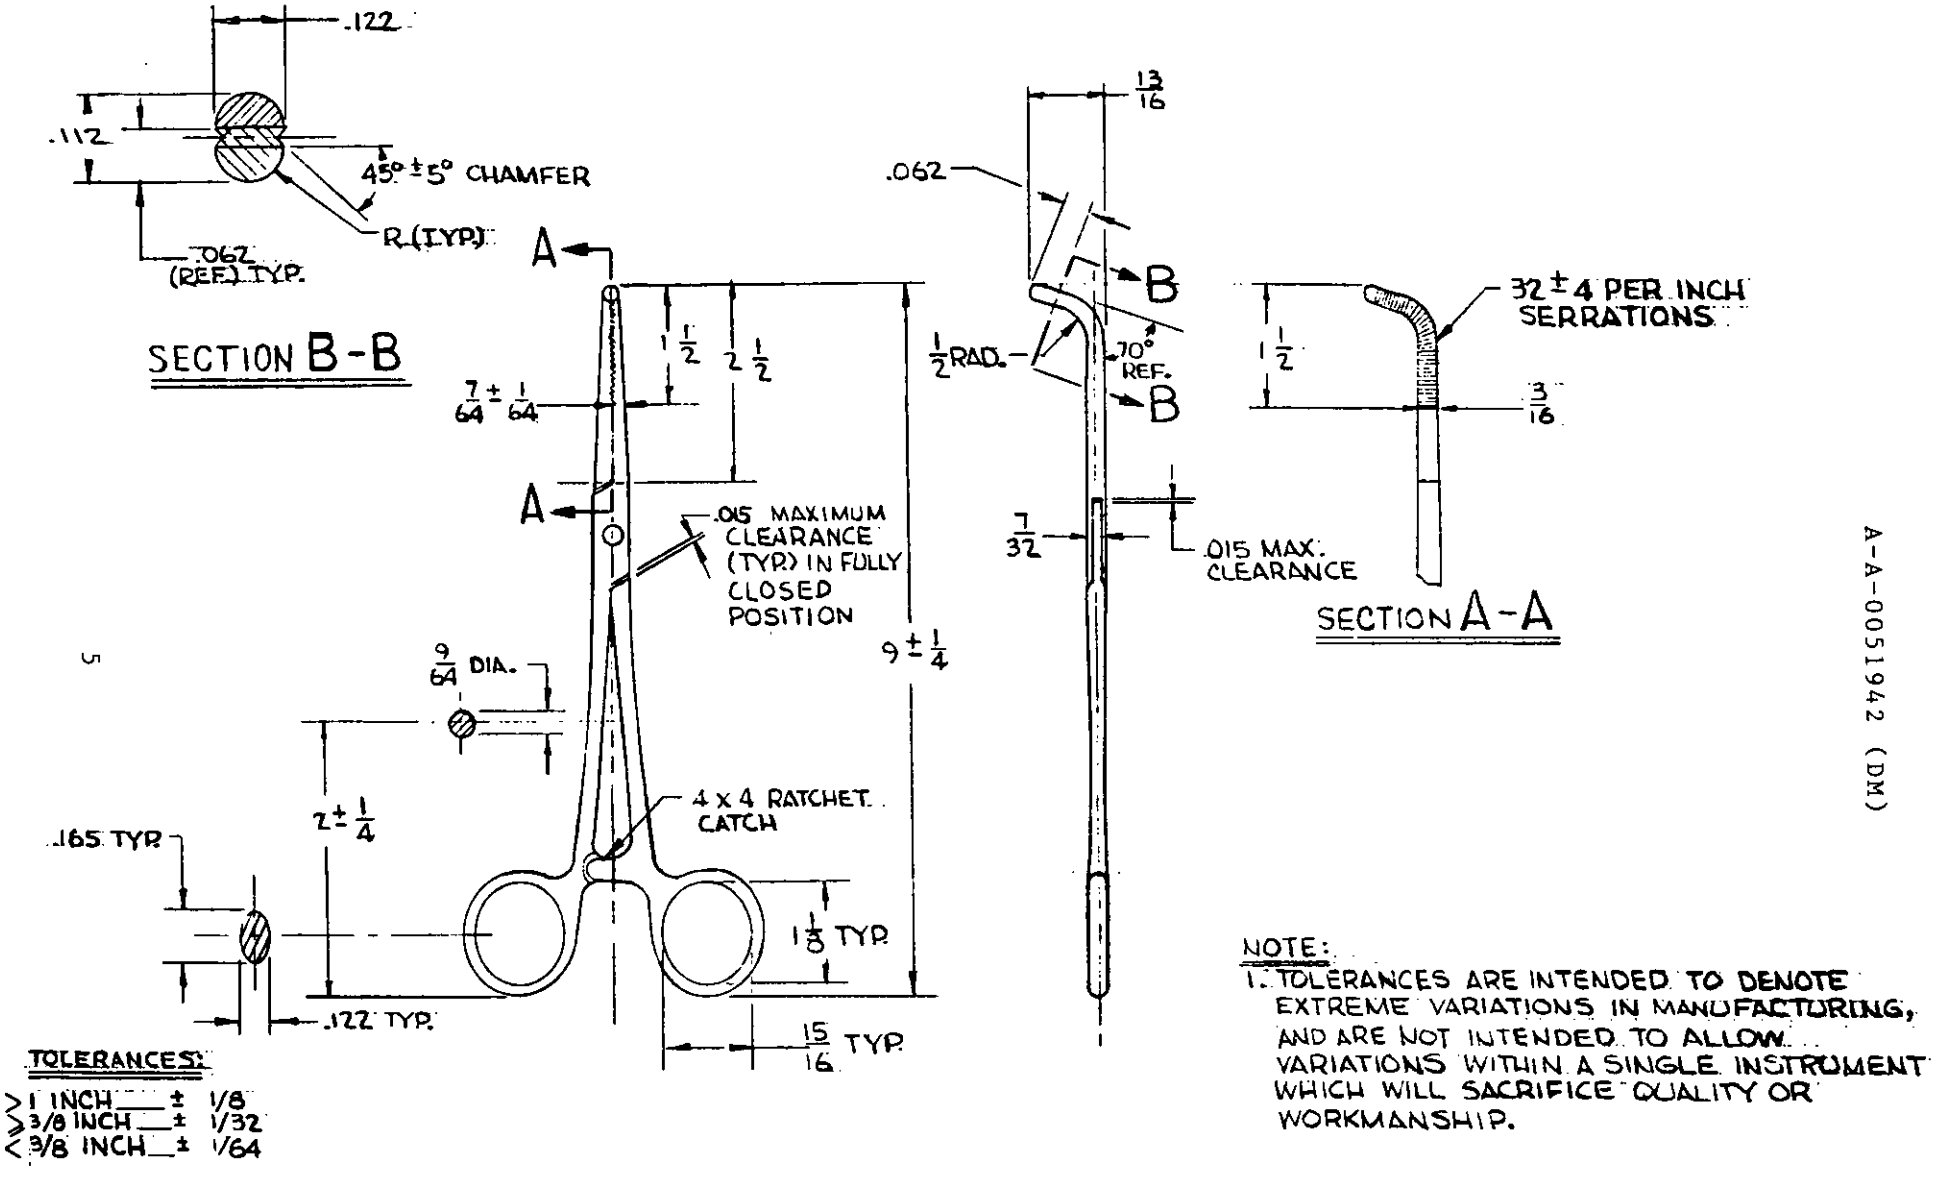

TOLERANCES:

> 1 INCH	±	1/8
≥ 3/8 INCH	±	1/32
< 3/8 INCH	±	1/64

NOTE:

1. TOLERANCES ARE INTENDED TO DENOTE EXTREME VARIATIONS IN MANUFACTURING, AND ARE NOT INTENDED TO ALLOW VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE QUALITY OR WORKMANSHIP.

FIGURE 1 FORCEPS, THORACIC, CURVED, MIXTER

A-A-0051942 (DM)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.