A-A-51954A
6 February 1989
SUPERSEDING
A-A-0051954(DM)
4 May 1987

COMMERCIAL ITEM DESCRIPTION

CURETTE, BONE (Brun)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers 9 sizes of cutting bone curettes of the Brun design.

Salient characteristics:

Material. Curettes shall be manufactured from Class 4 corrosion resistant steel in accordance with ASTM Designation F899.

Hardness. The shank and cup of the curette shall have a Rockwell Hardness C scale (HRC)of 50 to 55 when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Style, design and dimensions. Curettes shall be in accordance with Figure 1 for the size specified. The edge of the cup shall be uniformly sharp around its perimeter.

Passivation. The curettes shall be properly passivated.

Finish. The finish of the curette shall be mirror and satin, or entirely satin. The finish shall be uniform and free from burrs, pits, scale, rough areas, sharp edges (except cup perimeter), and grind or tool marks.

Corrosion resistance. The curettes shall show no signs of corrosion resistance when tested in accordance with ASTM Designation F1089.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Identification marking and labeling. Curettes shall be permanently and legibly marked with the contractor's name or registered trademark and the word "stainless." Curettes of foreign manufacture shall bear the name of the country of origin.

Workmanship. The curettes shall be processed in such a manner as to be uniform and free from cracks, pits, burrs, sharp edges, scale, rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One curette, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one curette. Sampling shall be inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Curettes shall be examined to determine compliance with specification requirements.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one curette. Inspection level shall be S-1 with an AQL of 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-122-0688	CURETTE, BONE, Brun, 11 mm, Size 6
6515-01-124-9765	CURETTE, BONE, Brun, Spoon, Size 0
6515-01-124-9766	CURETTE, BONE, Brun, Spoon, Size 00
6515-01-124-9767	CURETTE, BONE, Brun, Spoon, Size 000
6515-01-124-9768	CURETTE, BONE, Brun, Spoon, Size 1
6515-01-124-9769	CURETTE, BONE, Brun, Spoon, Size 2
6515-01-124-9770	CURETTE, BONE, Brun, Spoon, Size 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

NSN	ITEM IDENTIFICATION
6515-01-124-9771	CURETTE, BONE, Brun, Spoon, Size 4
6515-01-125-3264	CURETTE, BONE, Brun, Spoon, Size 5

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4541

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

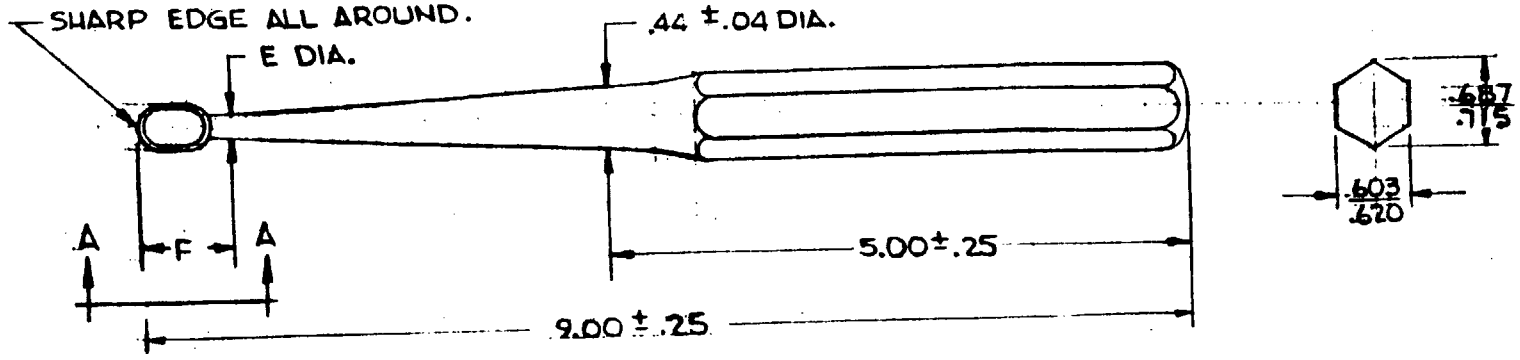

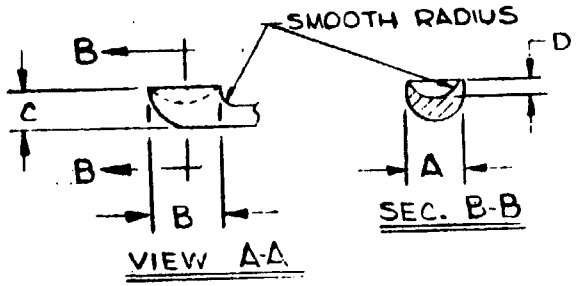

NOTE:
ALL DIMENSIONS ARE IN INCHES.

NSN	SIZE	A±.010	B±.010	C±.010	D	E±.010	F±.02
6515-01-124-9767	000	.118	.183	.098	.027±.003	.077	.31
6515-01-124-9766	00	.158	.183	.115	.042±.004	.092	.34
6515-01-124-9765	0	.198	.223	.133	.042±.004	.135	.38
6515-01-124-9768	1	.198	.263	.148	.063±.006	.135	.38
6515-01-124-9769	2	.238	.348	.178	.077±.008	.142	.50
6515-01-124-9770	3	.278	.443	.208	.092±.010	.172	.63
6515-01-124-9771	4	.318	.483	.228	.122±.010	.187	.69
6515-01-125-3264	5	.358	.568	.258	.122±.010	.202	.75
6515-01-122-0688	6	.418	.628	.303	.137±.010	.232	.75

FIGURE 1, CURETTE, BONE, BRUN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51954A	CURETTE, BONE (Brun)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.