RR-C-00633b
28 March 1968
Interim Revision of
Fed. Spec. RR-C-633a
11 August 1961

INTERIM FEDERAL SPECIFICATION

CRADLE, HOSPITAL BED CLOTHING

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification RR-C-633a.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers folding cradles for hospital bed clothing, suitable for forming a vault for the suspension of bed clothing above a bed patient.

1.2 Classification.

1.2.1 Types. Cradles shall be of the following types, as specified (see 6.1).

Type I - For general hospital use.
Type II - For field hospital use.

2. APPLICABLE DOCUMENTS

2.1 Specifications, standards and drawings. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547 Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

Federal

FED-STD-66 Steel, Chemical Composition and Hardenability.
FED-STD-123 Marking for Domestic Shipment (Civilian Agencies).
Fed. Test Method Std. 151 Metals: Test Methods.

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C., 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

(Copies of Military specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS.

3.1 First Article. Unless otherwise specified, prior to the start of production of the contract quantity, one sample of the cradle shall be assembled, completely finished, and tested by the contractor. The sample shall be submitted, together with the contractor's inspection and test reports, to the procuring contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the procuring contracting officer, or his authorized representative,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

prior to the manufacture and assembly of the remaining quantity to be manufactured. Pending approval of the first article, acquisition of materials, components, or commencement of production is at the sole risk of the contractor. Accepted sample shall be returned to the cognizant Quality Assurance Representative for retention and use as a guide for inspection during production.

3.2 Material. All material used in the fabrication of the cradles shall be AISI 302 or 304 corrosion-resisting steel, conforming to FED-STD-66 when tested as specified in 4.4.1.

3.3 Design and construction. Design and construction shall be in accordance with figures 1 and 2, as applicable, and as hereinafter specified.

3.3.1 Type I. Type I cradle shall be in strict accordance with figure 1. The cradle shall be so designed as to fold compactly for easy storage. The hoops and longitudinal members shall be 5/8-inch-wide steel strips having a finished thickness not less than 0.125 inch No. 11, United States Standard Revised (U.S.S.) Gage, cut and formed to proper shape. Each hoop shall be riveted loosely to the longitudinal members. A round washer shall be located between the hoops and the longitudinal members at the riveting points. The rivets shall be peened in such a manner as to hold the frame securely and still allow rotation of the hoops.


3.3.2 Type II. Type II cradle shall be in strict accordance with figure 2. The cradle shall be a compact, folding, portable, lightweight, single integral unit, which can be easily set up and collapsed. Cradles shall be of all riveted construction. Steel strip used in the fabrication of the cradle shall be 5/8 inch with a finished thickness of not less than 1/8 inch No. 11 U.S.S. Gage, cut and formed to proper shape. Peening of the rivets shall be in such a manner as to hold the frame securely and still allow the cradle to fold.

3.3.3 Finish. All surfaces of the cradles shall be given a No. 4 commercial finish. The finished article shall be clean, free of oil, grease, buffing compound, and other foreign matter.

3.4 Identification marking. Each cradle shall be permanently and legibly die stamped with the name or registered trademark of the manufacturer, the contract or purchase order number, and the letters "U.S.". Marking secured by adhesives shall not be used.


3.5 Workmanship. Workmanship shall be first class throughout. All ends of braces, sharp corners, and edges shall be rounded and polished smooth before finishing. Riveting shall be neatly done without projections or burrs. The cradles shall be free from defects which detract from their appearance or which may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.





CRADLE IN CLOSED POSITION

VIEW A-A



SEC. C-C

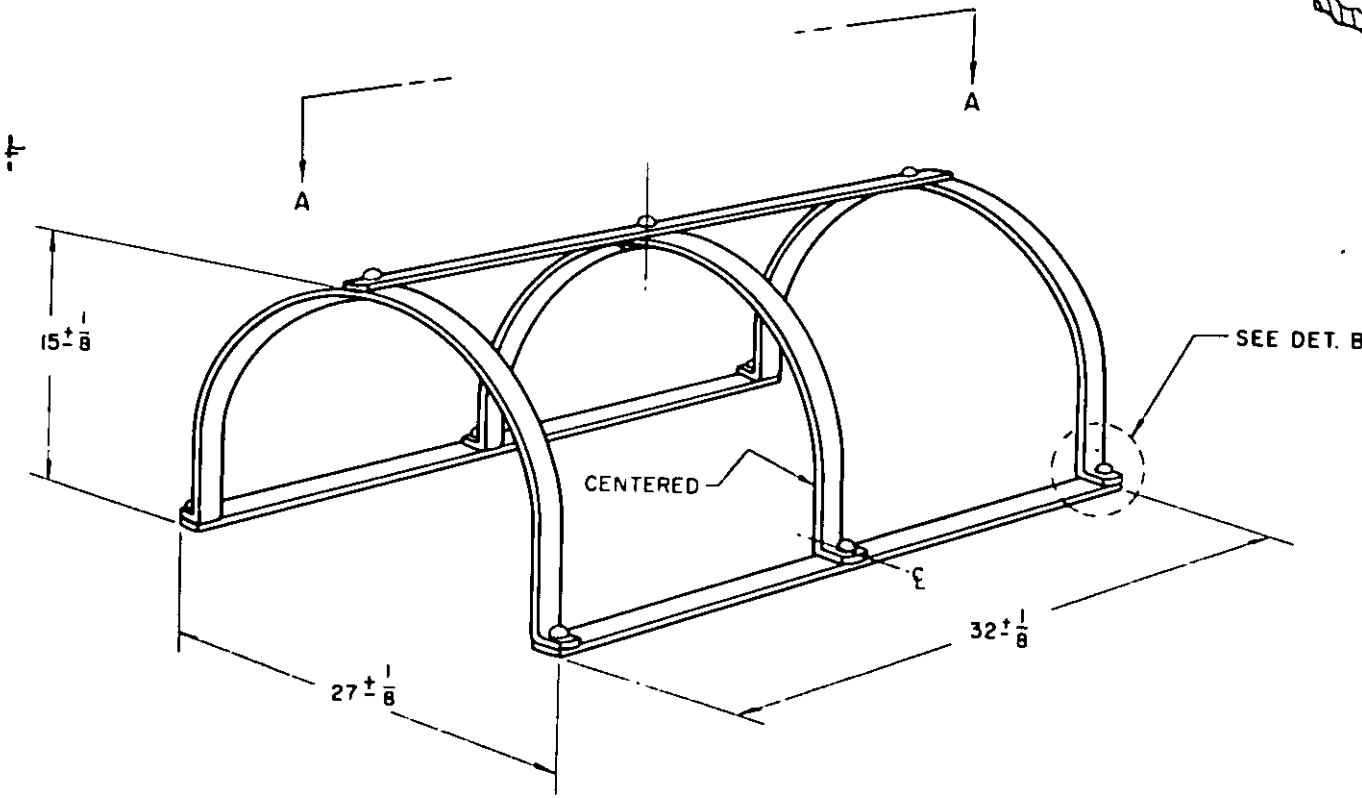


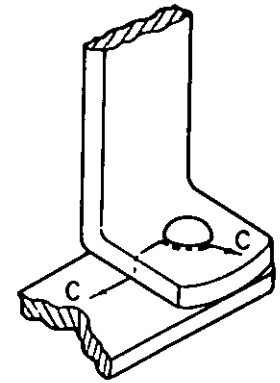


DET. B

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

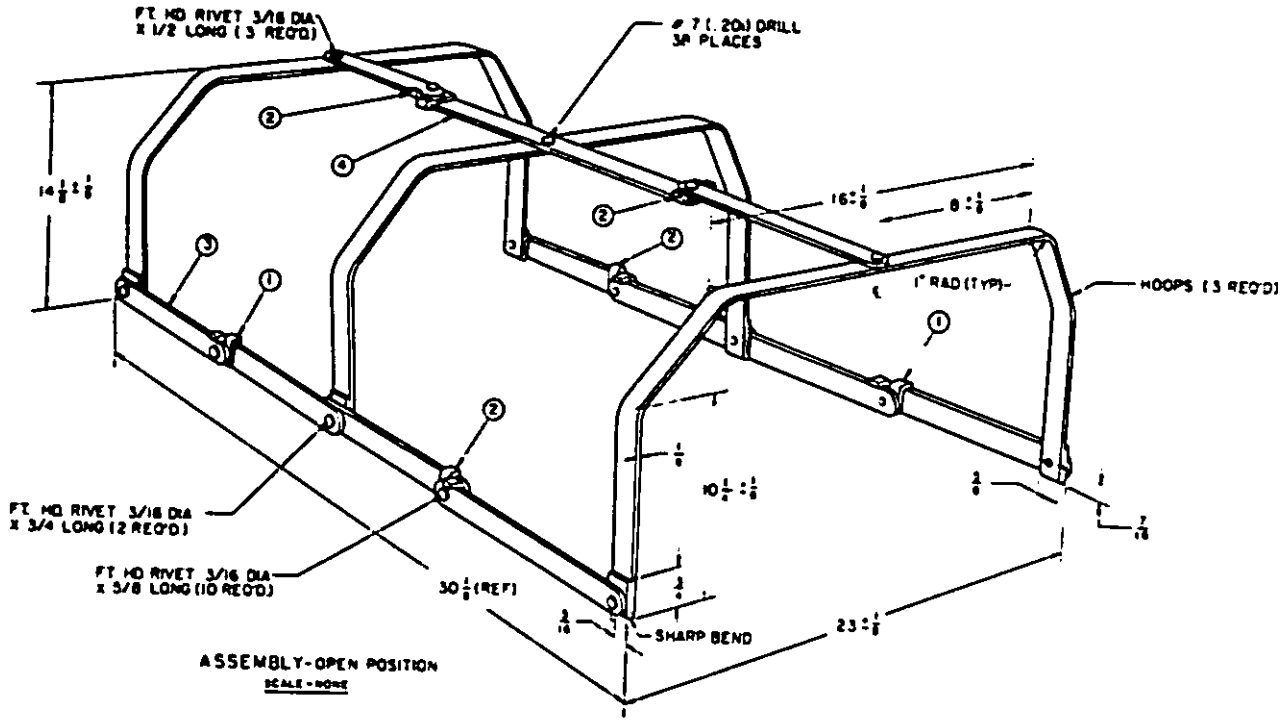

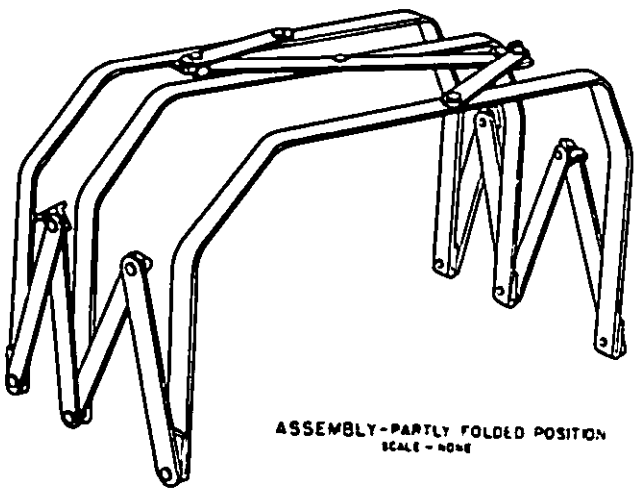


GENERAL NOTES:
1- REMOVE BURRS & ROUND OFF ALL SHARP EDGES TO 1/32 R. MIN.
2- COUNTERSINK ALL DRILLED HOLES TO BREAK SHARP EDGES UNLESS OTHERWISE NOTED.

NOTE
MEMBERS MUST MOVE SMOOTHLY WITHOUT BINDING OR EXCESSIVE PLAY

FIGURE 2
SHEET 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

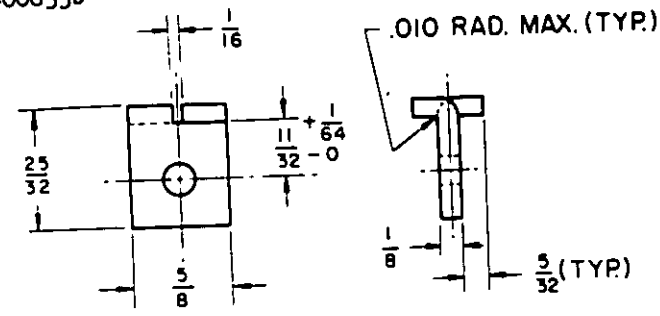

① STOP WASHER (2 REQ'D.)

SCALE 2=1


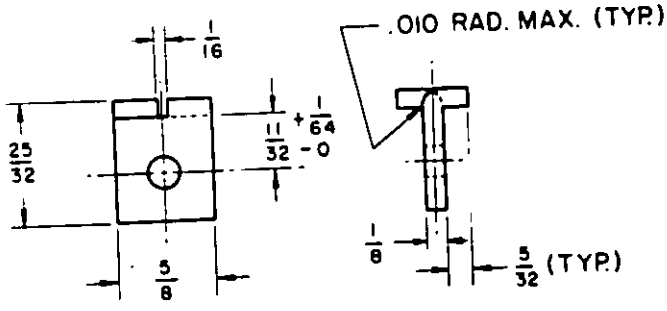


FIGURE 2
SHEET 2


② STOP WASHER (4 REQ'D.)

SCALE 2=1

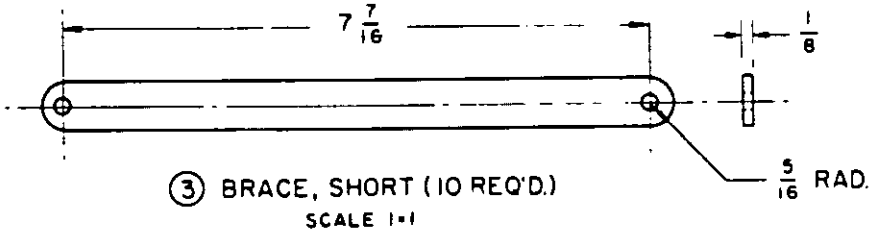

③ BRACE, SHORT (10 REQ'D.)

SCALE 1=1

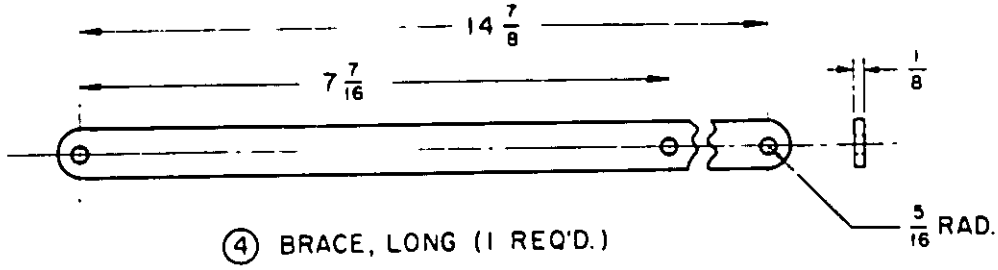

④ BRACE, LONG (1 REQ'D.)

SCALE 1=1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier shall utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to insure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling. Sampling for examination shall be conducted in accordance with MIL-STD-105.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	1.0
Total Major and Minor	II	4.0
For dimensional examination	S-2	2.5

4.2.2 Raw material. Four ounces of each lot of each metal used in the construction of the cradles shall be selected for chemical analysis.

4.3 Examination. The cradles shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

Categories and defects*

Major
101 Cradles cannot readily be set up or collapsed.
102 Component parts improperly aligned or fitted.
103 Cradles not free of cracks, tears, ruptures, and deformed areas.

Minor
201 Joints bind in operation.
202 Rivets not properly set, peened, and deburred.
203 Finish not free of coarse grind marks and scratches.
204 Cradles not clean, and free from foreign matter.
205 Identification marking missing, incomplete, impermanent, or illegible.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The cradles shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical composition shall be conducted in accordance with method 111.1 or 112.1 of FED-STD-151.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A, B, or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit package. Each cradle of the same type shall be packaged in a fiberboard box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening.

5.1.2 Level B.

5.1.2.1 Unit package. Each cradle shall be packaged as described in 5.1.1.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Six (6) type I or twelve (12) type II cradles packaged as specified in 5.1 shall be packed in containers designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; or PPP-B-621, table III. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.1.2 Case liner. Each box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.2 Level B.

5.2.2.1 Exterior container. Six (6) type I or twelve (12) type II cradles packaged as specified in 5.1 shall be packed in containers designed for type 2 load, and constructed in accordance with PPP-B-601, table I, using type III, class 1 plywood; PPP-B-585, style 3, for class 2 use; or PPP-B-621, table I. Closure shall be in accordance with appendix of applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. In addition to any special marking specified in the contract or order, each unit and shipping container shall be marked in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contract shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Military hospital and medical facilities.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).
(c) When First Article shall not be sent (see 3.1).
(d) Where First Article shall be sent (see 3.1).

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL CODE: ATS
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

☆ U. S. GOVERNMENT PRINTING OFFICE: 1968-301-518/5332

DPSC FORM 2418
AUG 68

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements .

SPECIFICATION

RR-C-00633b

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 44, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.