RR-C-633a
August 11, 1961

SUPERSEDING
Fed. Spec. RR-C-633
August 10, 1948

FEDERAL SPECIFICATION

CRADLE, HOSPITAL BED CLOTHING

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers folding hospital bed clothing cradles, suitable for forming a vault for the suspension of bed clothing above a bed patient.

1.2 Classification.

1.2.1 *Types.* Cradles shall be of the following types, as specified (see 6.1):

Type I.—For general use.
Type II.—For field use.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

PPP-B-585—Boxes; Wood, Wirebound.
PPP-B-601—Boxes, Wood, Cleated-Plywood.
PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636—Box, Fiberboard.

Federal Standards:

Fed. Std. No. 66—Steel: Chemical Composition and Hardenability.

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.

Fed. Std. No. 123—Marking for Domestic Shipment (Civilian Agencies).

Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL-B-10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

MIL–L–10547—Liners, Case, Waterproof.

Military Standards:

MIL–STD–105—Sampling Procedures and Tables for Inspection by Attributes.

MIL–STD–129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. All material used in the fabrication of the cradles shall be AISI 302 or 304 corrosion-resisting steel, conforming to the requirements of Federal Standard No. 66 when tested as specified in 4.4.1.

3.2 Construction.

3.2.1 *Type I.* Type I cradle shall be in strict accordance with figure 1. The cradle shall be so designed as to fold compactly for easy storage. The hoops and longitudinal members shall be ⅞-inch-wide steel strips having a finished thickness not less than 0.125 inch (No. 11, United States Standard Revised gage), cut and formed to proper shape. Each hoop shall be riveted loosely to the longitudinal members. A round washer shall be located between the hoops and the longitudinal members at the riveting points. The rivets shall be peened in such a manner as to hold the frame securely and still allow rotation of the hoops.

3.2.2 *Type II.* Type II cradle shall be in strict accordance with figure 2. Cradle shall be compact, folding, portable, lightweight, and a

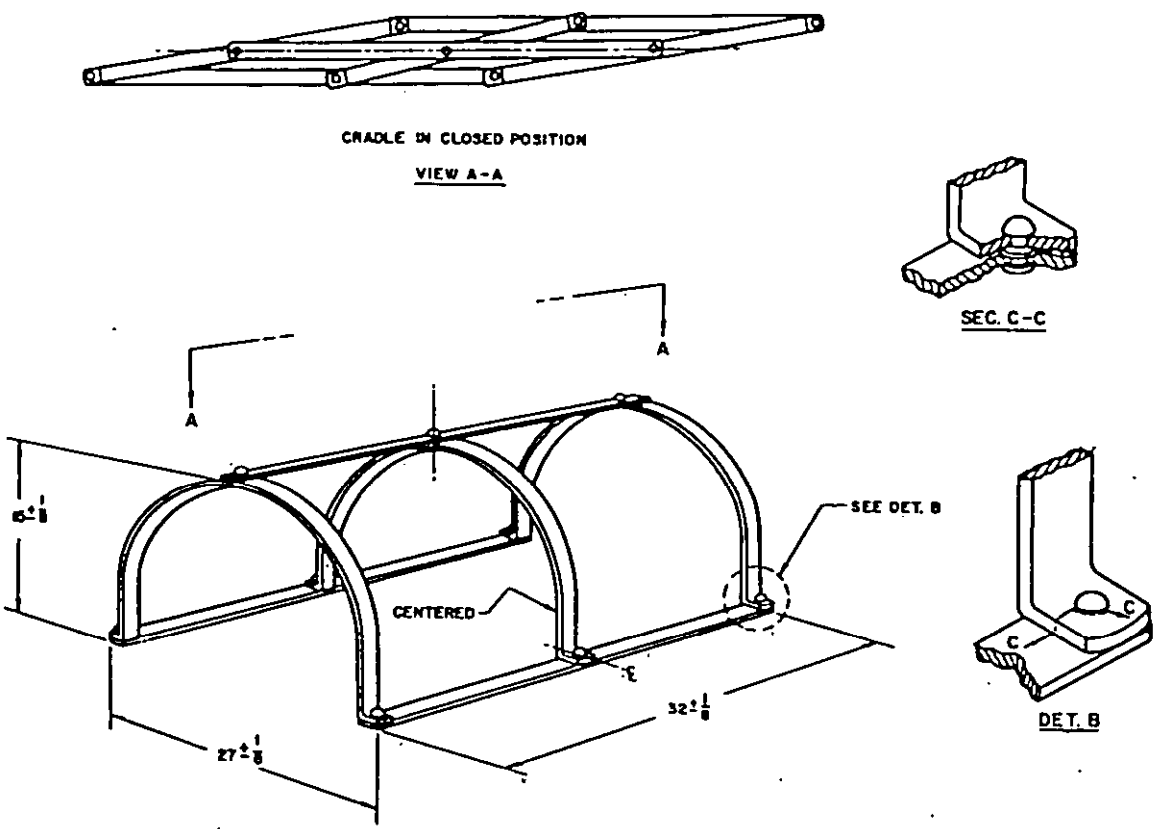


FIG. 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

single integral unit which can be easily set up and collapsed. Cradles shall be of all riveted construction. Steel strip used in the fabrication of the cradle shall be ⅝ inch wide having a finished thickness of not less than 0.125 inch (No. 11, United States Standard Revised gage), cut and formed to proper shape. Peening of the rivets shall be in such a manner as to hold frame securely and still allow the cradle to fold.

3.3 Finish. All surfaces of the cradles shall be given a No. 4 commercial finish. The finished article shall be clean, free of oil, grease, buffing compound, and other foreign matter.

3.4 Identification marking. Each cradle shall be permanently and legibly die stamped with the name or registered trademark of the manufacturer, the contract or purchase order number, and the letters "U. S.". Marking secured by adhesives shall not be used.

3.5 Workmanship. Workmanship shall be first class throughout. All ends of braces, sharp corners, and edges shall be rounded and polished smooth before finishing. Riveting shall be neatly done without projections or burrs. The cradles shall be free from defects which detract from their appearance or which may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Supplier responsibilities for inspection. The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 *Inspection,* Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.* When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling. Sampling shall be conducted in accordance with Military Standard MIL–STD–105.

	Inspection level	AQL (percent defective)
For visual examination:		
Major defects	II	1.0
Total (major and minor combined) defects	II	4.0
For dimensional examination	L5	2.5

4.2.1 *Raw materials.* Four ounces of each lot of each metal used in the construction of the cradles shall be selected for chemical analysis.

4.3 Examination. The cradles shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 *Classification of defects.* Examination shall be conducted in accordance with the following classification of defects:

Categories and defects

Major

101. Cradles cannot readily be set up or collapsed.
102. Component parts improperly aligned or fitted.
103. Cradles not free of cracks, tears, ruptures, and deformed areas.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

Minor

201. Joints bind in operation.
202. Rivets not properly set, peened, or deburred.
203. Finish not free of coarse grind marks and scratched areas.
204. Cradles not cleaned and free of foreign matter.
205. Identification marking missing, incomplete, impermanent, or illegible.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 *Dimensional examination.* The cradles shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 **Tests.** Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 *Chemical composition.* Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard 151.

5. PREPARATION FOR DELIVERY

For civil agency procurement only, Federal Standard No. 102 should be referred to for definitions and applications of the various levels of packaging and packing protection for supplies and equipment.

5.1 Packaging.

5.1.1 *Level A or B.* Each cradle of the same type shall be packaged in a fiberboard box of appropriate size constructed in accordance with Federal Specification PPP–B–636, type I, class 1. Each container shall be adequately secured to prevent accidental opening.

5.1.2 *Level C.* Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.* Six type I and twelve type II cradles packaged as specified in 5.1.1 shall be packed in containers designed for type 2 load, and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; PPP–B–621, table III; or Military Specification MIL–B–10377, table II. Each box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Strapping, when required, shall be in accordance with applicable box specification.

NOTE: Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.* Six type I and twelve type II cradles packaged as specified in 5.1.1 shall be packed in containers constructed in accordance with Federal Specification PPP–B–585, style 3, for class 2 use; PPP–B–621, table I; or PPP–B–636, type I, class 1, of not less than 275-pound test fiberboard.

5.2.3 *Level C.* The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or order.

5.2.4 *Standard pack for civil agency procurement.* The standard pack for this commodity shall be as specified in 5.1.1 and 5.2.2.

5.3 Marking.

5.3.1 *Civil agencies.* In addition to any special marking specified in the contract or order, each unit and shipping container shall be marked in accordance with Federal Standard No. 123.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5.3.2 *Military agencies.* In addition to any special marking required by the contract or order, each unit package and shipping container shall be marked in accordance with Military Standard MIL–STD–129.

6. NOTES

6.1 *Ordering data.* Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Type required (see 1.2.1).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(d) Standard pack requirements (see 5.2.4 and 6.4).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.3 Transportation description. Transportation description and minimum weights applicable to this commodity are:

Rail:

Frames, bed canopy, metallic, folded flat.
Carload minimum weights:
In cars 40 feet 9 inches or less in length, inside measurements—10,000; 12,000; 15,000; 18,000; 22,000; and 30,000 pounds.
In cars exceeding 40 feet 9 inches in length, inside measurements—16,000; 18,000; 21,000; 24,000; 30,000; and 40,000 pounds.

Motor:

Frames, bed canopy, metallic, folded flat.
Truckload minimum weights: 10,000; 12,000; 15,000; 18,000; 22,000; and 30,000 pounds, subject to Rule 34, National Motor Freight Classification.

6.4 The standard pack requirements in 5.1.1 and 5.2.2 are intended for use in procurements of stores stock replenishments. Procuring officers should use the standard pack requirements when it is known that the material will be shipped from a supplier to a domestic warehouse, supply depot, or intermediate storage point for temporary storage, subsequent issue and/or shipment to eventual user.

Notice. When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.


MILITARY CUSTODIANS:

Army—MI
Navy—Md
Air Force—AFCSC


☆ U. S. GOVERNMENT PRINTING OFFICE: 1961

Copies of this specification may be purchased for — cents each.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

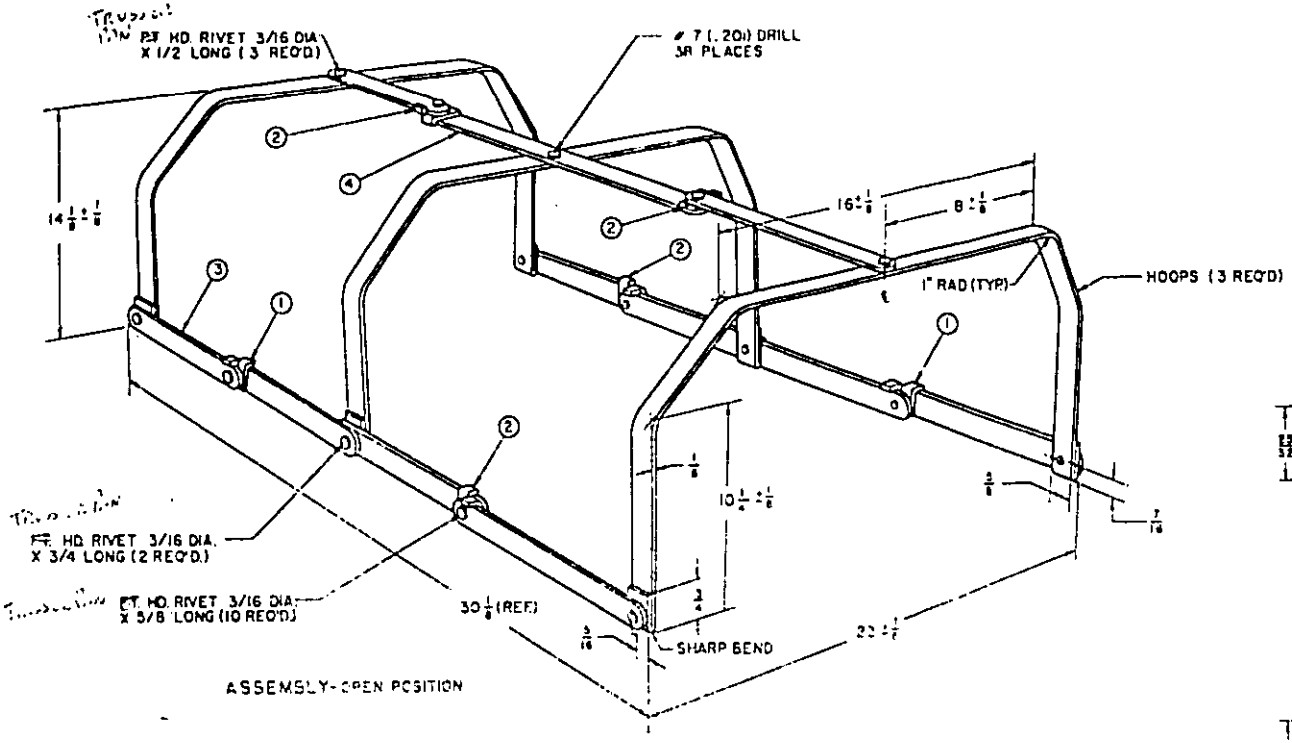


ASSEMBLY-OPEN POSITION

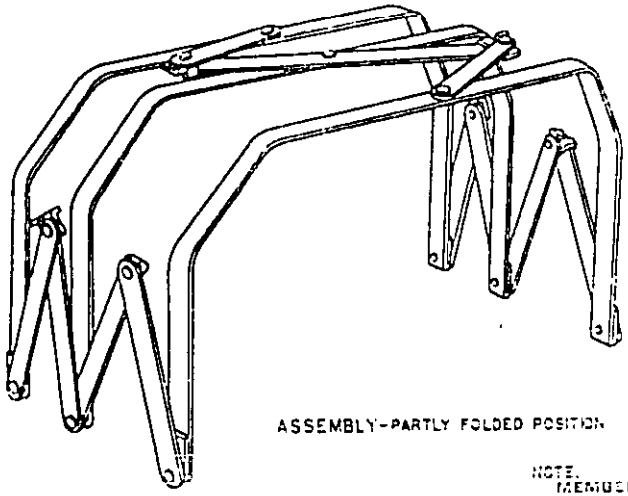


ASSEMBLY-PARTLY FOLDED POSITION

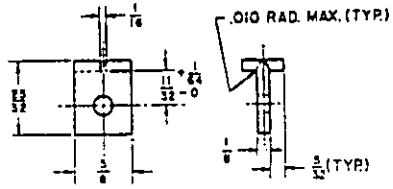


① STOP WASHER (2 REQ'D.)

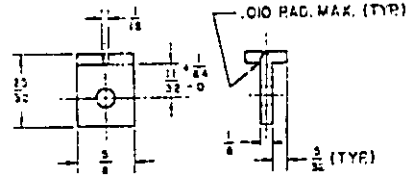

② STOP WASHER (4 REQ'D.)

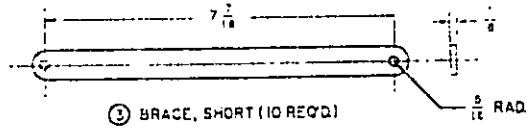

③ BRACE, SHORT (10 REQ'D.)

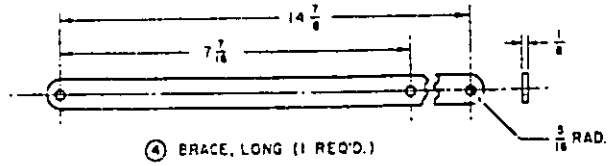

④ BRACE, LONG (1 REQ'D.)

GENERAL NOTES:
1- REMOVE BURRS & ROUND OFF ALL SHARP EDGES TO 1/32 R. MIN.
2- COUNTERSINK ALL DRILLED HOLES TO BREAK SHARP EDGES UNLESS OTHERWISE NOTED.

FIG. 2

NOTE:
MEMBERS MUST MOVE SMOOTHLY WITHOUT BINDING OR EXCESSIVE PLAY

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.