RR-I-68lb
September 21, 1961

SUPERSEDING
Fed. Spec. RR-I-681a
December 13, 1956

FEDERAL SPECIFICATION

IRRIGATOR, CORROSION-RESISTING STEEL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers one type of corrosion-resisting steel irrigator, without a handle, of 2-quart capacity, suitable for use in hospitals and medical offices.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification to the extent specified herein:

Federal Specifications:

PPP-B-585—Boxes; Wood, Wirebound.
PPP-B-601—Boxes, Wood, Cleated-Plywood.
PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636—Box, Fiberboard.

Federal Standards:

Fed. Std. No. 66—Steel: Chemical Composition and Hardenability.
Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.
Fed. Std. No. 123—Marking for Domestic Shipment (Civilian Agencies).
Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specification:

MIL-L-10547—Liners, Case, Waterproof.

Military Standards:

MIL-STD-105—Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The irrigator shall be made of sheet steel and shall conform to AISI 304 of Federal Standard No. 66, when tested as specified in 4.4.1.

3.2 Design and measurements. Design and measurements shall be as shown on figure 1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

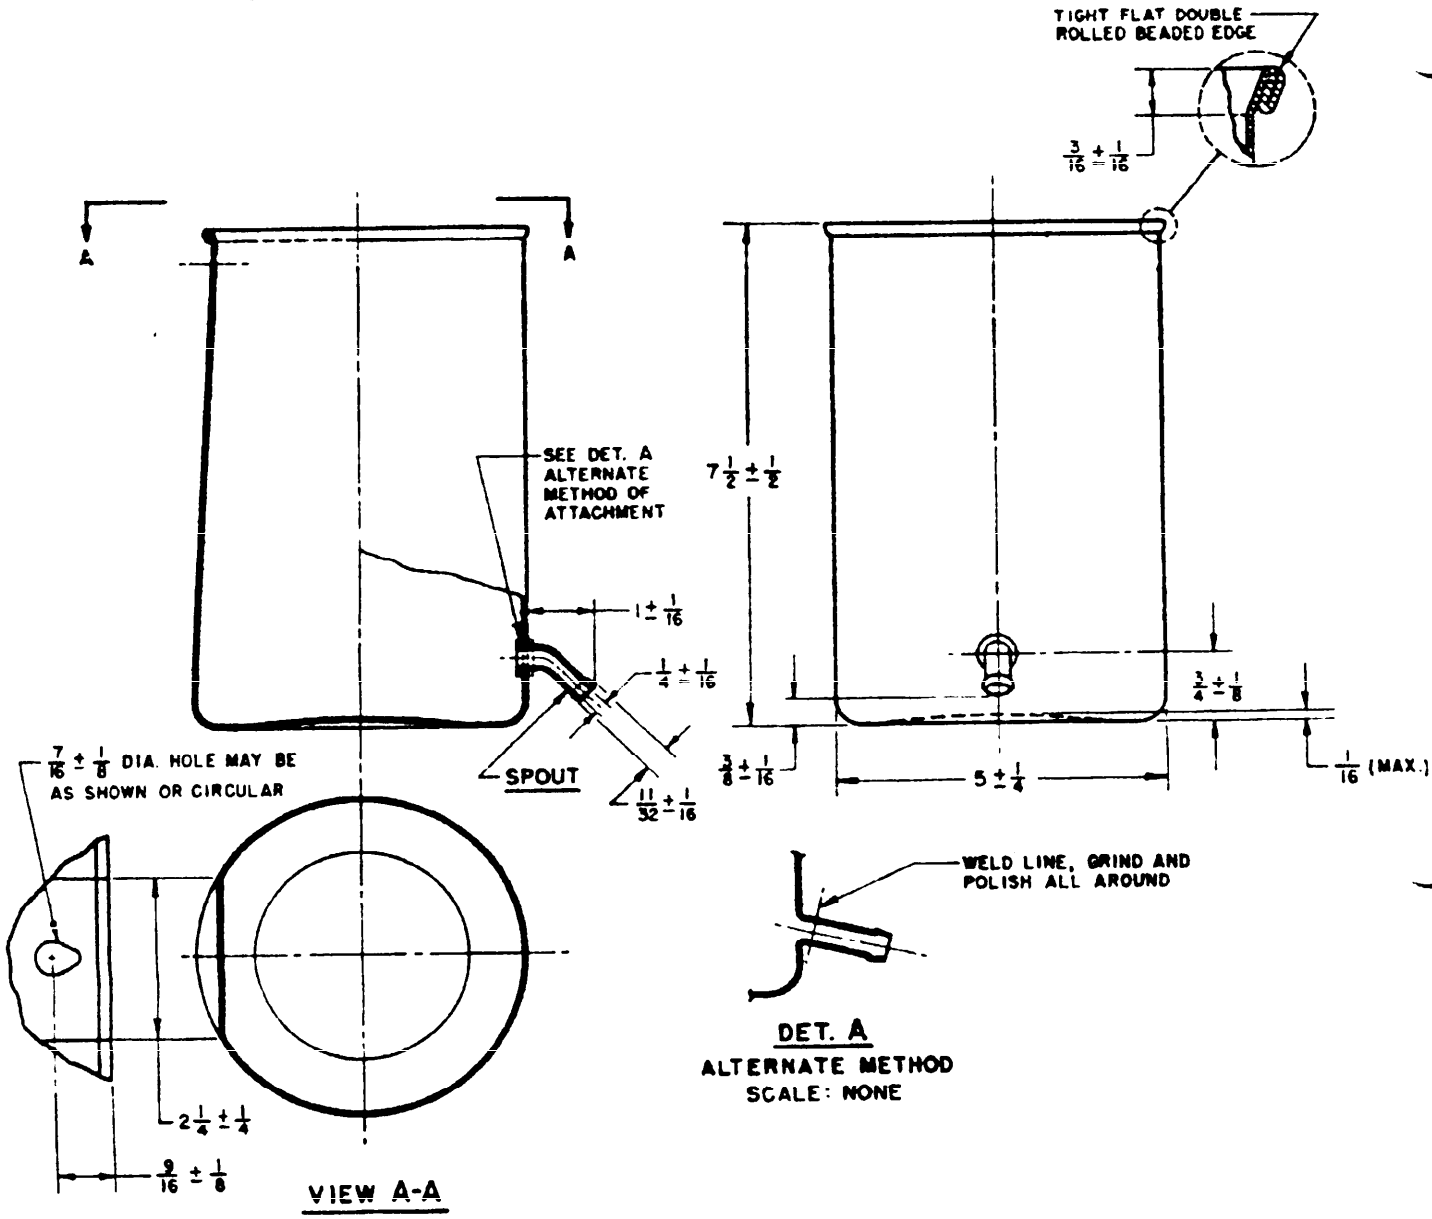


FIG.-1

3.2.1 *Body*. The body shall be formed seamlessly from one single piece of corrosion-resisting steel, not less than 0.031 inch thick (No. 22, United States Standard gage), which shall not be reduced below 0.027 inch thick at any point in the finished irrigator.

3.2.2 *Spout*. The spout shall be of seamless tubular form, either straight or slightly curved, and pitched downward. It shall have a wall thickness of not less than 0.03 inch and a lumen of uniform diameter not less than ¼ inch. Lumen surfaces shall be without depressions or irregularities of any sort where dirt may lodge, shall have a bulbous outer end to retain the rubber tube securely, and shall be attached to the body as shown on figure 1. Either method of attachment shall leave no corners, crevices, pits, or

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

other rough or uneven surfaces to retain dirt. The spout shall terminate above the bottom of the irrigator, so that it will sit evenly on a flat surface with rubber tubing attached. (See figure 1.)

3.3 Finish.

3.3.1 *Grinding and polishing.* Finish shall be smooth on all surfaces and edges, and shall be free of rough grind marks, trimming marks, pits, scales, die marks, and other defects. The final finish shall be obtained with a grind of No. 200 emery or its equivalent, and shall present a uniformly finished surface substantially similar to a No. 4 commercial finish. The thickness of the sheet forming the irrigator shall not be reduced below the thickness specified in 3.2.1 by grinding to remove surface imperfections.

3.3.1.1 *Alternate interior finish.* As an alternate, the interior of the irrigator may be finished by electropolishing. The electropolishing shall result in a uniform, bright, shiny surface which can be readily cleaned.

3.3.2 *Cleaning.* As a final operation, the irrigator shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

3.3.3 *Corrosion-resistance.* When tested as specified in 4.4.2, slight surface corrosion of the finished irrigator which can be washed off shall not be considered cause for rejection; but if the irrigator should rust or show continuous bleeding from pits, it shall be considered as having failed to pass the test.

3.4 Identification marking. Each irrigator shall be impressed on the side or bottom with the manufacturer's name or registered trademark, the contract or purchase order number, and the letters U.S. All impressions shall be made at even pressure so as not to penetrate the inside surface of the irrigator.

3.5 Workmanship. Irrigators shall be free from defects which will affect the appearance or may affect the serviceability. All surfaces shall have a smooth finish and shall be free of sharp edges.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Supplier responsibilities for inspection. The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 *Inspection.* Inspection, as used in this specification, is defined as both examination such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.* When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling. Sampling shall be conducted in accordance with Military Standard MIL-STD-105.

	Inspection level	AQL (defects per hundred)
For visual examination:		
Major defects	II	1.0
Total (major and minor combined) defects	II	4.0
For dimensional examination	L2	2.5
For salt spray test	L3	*

* Acceptance number shall be zero. Not less than three samples shall be taken regardless of lot size.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.2.1 *Raw materials.* Four ounces of each lot of metal used in the construction of the irrigators shall be selected for chemical analysis.

4.3 Examination. The irrigators shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 *Classification of defects.* Examination shall be conducted in accordance with the following classification of defects:

	*Categories and defects**
Major	
101	Irrigator not complete with all component parts.
102	Component parts not properly aligned or fitted.
103	Metal components not free of cracks, tears, ruptures, and deformed surfaces.
104	Exposed or accessible edges, corners, and surfaces not free of burs, sharpness, and sharp projections.
105	Seam or welds not sound, not continuous, or not free of pits, seams, flux, splatter, and discoloration.
106	Irrigator not free of leaks.
107	Spout not securely and seamlessly attached.
108	Spout not pitched slightly downward.
Minor	
201	Irrigator does not rest evenly on a flat surface.
202	End of spout not designed to retain rubber tubing (bulbous in shape).
203	Seam or welds not ground smooth to blend with adjacent surfaces.
204	Finish not uniform and not free of coarse grind marks and scratched areas.
205	Irrigator not free of dirt, grease, and foreign particles.
206	Identification marking not present, legible, or permanently affixed.
207	Inside surface not free from penetration of identification marking.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 *Dimensional examination.* Irrigators shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 *Chemical composition.* Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard 151.

4.4.2 *Salt spray.* Irrigators shall be tested in accordance with method 811.1 of Federal Test Method Standard 151, for a period of 48 hours.

5. PREPARATION FOR DELIVERY

For civil agency procurement only, Federal Standard No. 102 should be referred to for definitions and applications of the various levels of packaging and packing protection for supplies and equipment.

5.1 Packaging.

5.1.1 *Level A or B.* Each irrigator shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP-B-636, type I, class 1. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Closure shall be effected in such manner as to prevent spillage of contents under normal handling.

5.1.2 *Level C.* Irrigators shall be wrapped in kraft paper and packaged individually in substantial cartons.

5.2 Packing.

5.2.1 *Level A.* Twelve irrigators, packaged as specified in 5.1.1 shall be packed in exterior containers designed for type 2 load and constructed in accordance with Federal Specification PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; or PPP-B-621, table III. Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL-L-10547.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

Closure and sealing shall conform to applicable paragraphs of appendix thereto. Strapping, when required, shall be in accordance with applicable box specification.

NOTE: Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.* Twelve irrigators, packaged as specified in 5.1.1 shall be packed in exterior containers conforming to Federal Specification PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with Federal Specification PPP-B-621, table I; PPP-B-585, style 3 for class 2 use; or PPP-B-636, type I, class 1, fabricated from not less than 275-pound test fiberboard.

5.2.3 *Level C.* The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or order.

5.2.4 *Standard pack (civil agencies).* The standard pack shall be as specified in 5.1.1 and 5.2.2, except shipping containers shall conform to Federal Specification PPP-B-636, type I, class 1 only.

5.3 Marking—nonmilitary.

5.3.1 Unless otherwise specified in the contract or order, interior packages and shipping containers shall be marked in accordance with Federal Standard No. 123.

5.4 Marking—military.

5.4.1 *Interior and exterior containers.* Unless otherwise specified interior and exterior containers shall be marked in accordance with Military Standard MIL-STD-129.

6. NOTES

6.1 Ordering data. Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number and date of this specification.

(*b*) Selection of applicable levels of packaging and packing. (See 5.1 and 5.2.)

(*c*) Standard Pack (see 5.1.1 and 5.2.2).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.3 The Standard Pack requirements in 5.1.1 and 5.2.2 are intended for use in Stores Stock Replenishments. Procuring officers should use Standard Pack requirements when it is known that the material will be shipped from a supplier to a domestic warehouse, supply depot, or intermediate storage point for temporary storage, subsequent issue and/or shipment to eventual user.

6.4 Transportation description. Transportation description and minimum weights applicable to this commodity are:

Rail:

Sheet steel ware not otherwise indexed by name (Irrigators). (Indicate nested, not nested, or nested solid, flat or folded flat.)
Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Motor:

Sheet steel articles, not otherwise indexed. (Indicate nested, not nested, or nested solid, flat or folded flat.)
Truckload minimum weight 20,000 pounds.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

Notice. When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTEREST:

Army—MI
Navy—Md
Air Force

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.