RR-T-626c
October 16, 1961
SUPERSEDING
Fed. Spec. RR-T-626b
January 27, 1958

FEDERAL SPECIFICATION

TRAY, CATHETER; CORROSION RESISTING STEEL, (WITH COVERS)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers catheter trays, with covers, designed to hold catheters used in hospital operating rooms and in medical offices.

1.2 Classification.

1.2.1 *Types, sizes, and styles.* Catheter trays shall be of the following types, sizes, and styles, as specified (see 6.1).

Type I.—Deep.

Type II.—Shallow.

Size 1. (See table I.)

Size 2. (See table I.)

Style A. (See Figure 1.)

Style B. (See Figure 2.)

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification to the extent specified herein:

Federal Specifications:

QQ-S-766—Steel Plates, Sheets, and Strip—Corrosion-Resisting.

PPP-B-566—Boxes, Folding, Paperboard.

PPP-B-585—Boxes; Wood, Wirebound.

PPP-B-601—Boxes, Wood, Cleated-Plywood.

PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.

PPP-B-636—Box, Fiberboard.

PPP-B-676—Boxes, Set-Up, Paperboard.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.

Fed. Std. No. 123—Marking for Domestic Shipment (Civilian Agencies).

Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

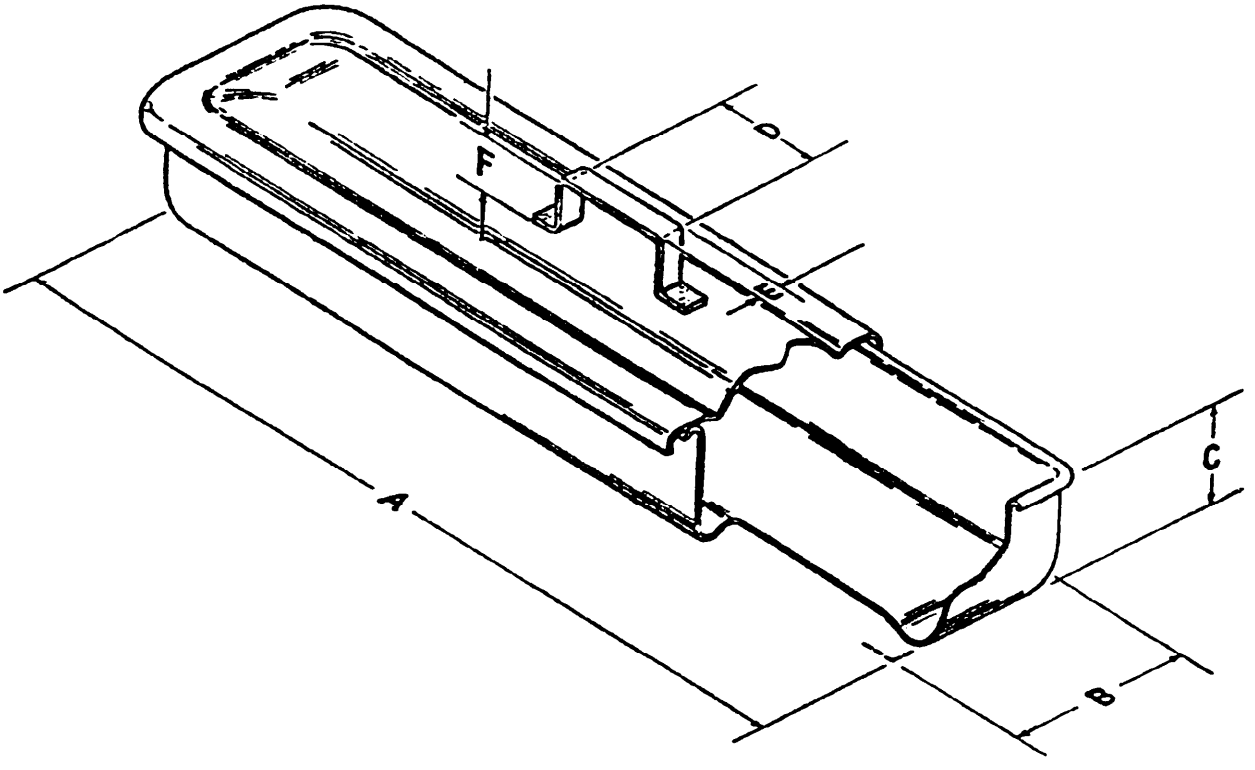


FIGURE 1.- Style A.

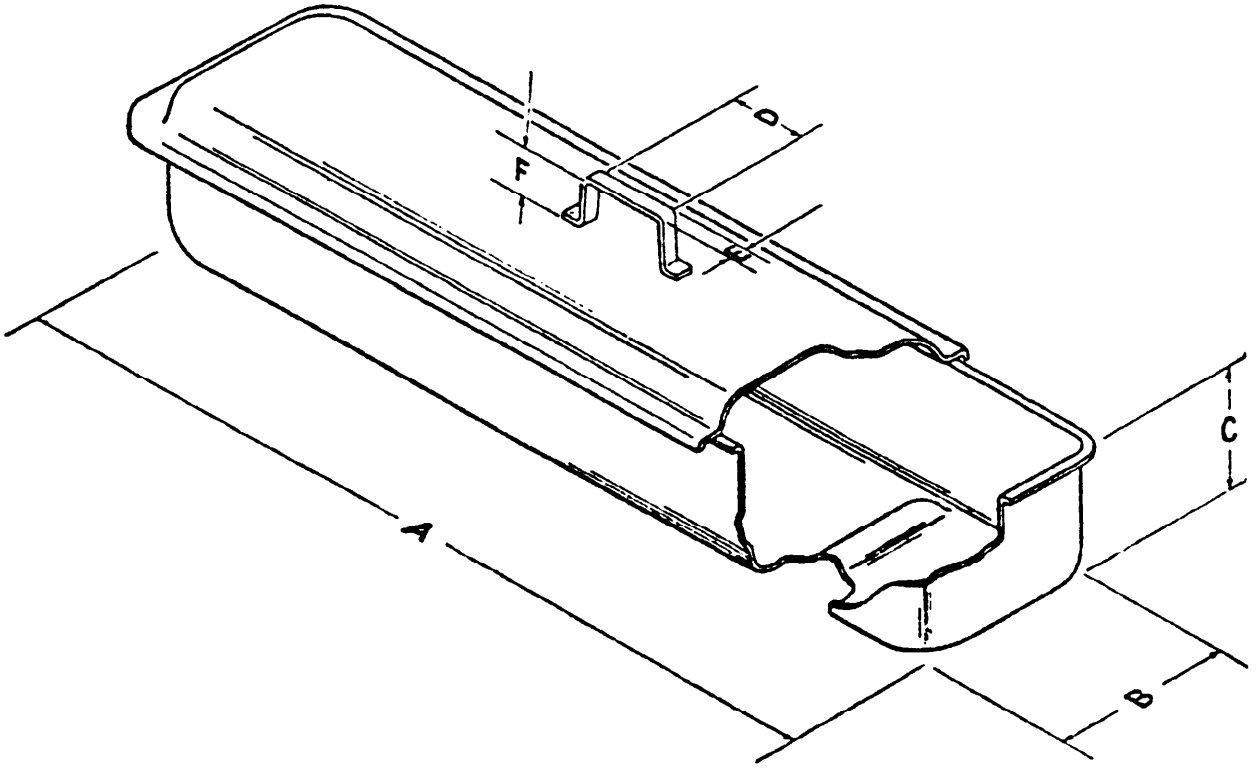


FIGURE 2.- Style B.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specification:

MIL-L-10547—Liners, Case, Waterproof.

Military Standards:

MIL-STD-105—Sampling Procedures and Tables for Inspection by Attributes.

MIL-STD-129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Trays shall be made of corrosion-resisting steel conforming to class 302 or 304 of Federal Specification QQ-S-766, and shall meet the chemical requirements specified therein when tested as specified in 4.4.1.

3.2 Design and dimensions. Grooves or embossing shall be used to reinforce the bottom surface of the trays. Covers shall be designed to fit trays squarely, without rock or tendency to rattle. Handles shall be square as shown in figures 1 and 2 or rounded provided finger clearance is within tolerances allowed in table I. All gages specified herein shall be minimum. Commercial tolerances shall apply. Dimensions shall be as shown in table I and in figures 1 and 2.

3.2.1 *Type I, deep.* The body of type I shall be formed seamlessly from one single piece of 0.050-inch-thick (No. 18, United States Standard (U.S.S.) gage) corrosion-resisting steel which shall not be reduced below 0.045-inch thickness at any point. The cover shall be 0.031-inch-thick (No. 22, U.S.S. gage) corrosion-resisting steel which shall not be reduced below 0.027-inch thickness. The cover of type I tray may be flat, or domed as shown on figures 1 and 2. The lift handle shall be formed of 0.050-inch-thick (No. 18, U.S.S. gage) corrosion-resisting steel.

3.2.2 *Type II, shallow.*

3.2.2.1 *Size 1.* Size 1 shall be as shown in figures 1 or 2 for either style A or style B. The body shall be formed seamlessly from one single piece of 0.031-inch-thick (No. 22, U.S.S. gage) corrosion-resisting steel, which shall not be reduced below 0.025-inch thickness at any point. The cover shall be formed of 0.025-inch-thick (No. 24, U.S.S. gage) corrosion-resisting steel which shall not be reduced below 0.021-inch thickness at any point. The lift handle shall be formed of 0.078-inch-thick (No. 14, U.S.S. gage) corrosion-resisting steel.

3.2.2.2 *Size 2.* Size 2 shall be as shown in figures 1 or 2 for either style A or style B. Each body and each cover shall be formed seamlessly from one single piece of 0.031-inch-thick (No.

TABLE I.

	Type I	Type II			
		Style A		Style B	
		Size 1	Size 2	Size 1	Size 2
	Inches	*Inches*	*Inches*	*Inches*	*Inches*
A	30 3/32	8 1/16	16 5/8	8 3/16	16 1/2
B	4	2 9/16	3 5/8	2 3/4	3 3/4
C	4	1 1/2	2 1/8	1 1/2	2 9/16
D	2 5/8	1 7/16	2 1/2	1 3/4	1 3/4
E	1/2	3/8	19/32	3/8	3/8
F	1	13/16	1 1/16	9/16	9/16

Tolerances: Under 12 inches ± 1/16 inch; 12 inches and over ± 1/4 inch.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:11Z
Check the source to verify that this is the current version before use.

22, U.S.S. gage) corrosion-resisting steel, which shall not be reduced below 0.025-inch thickness at any point. The lift handle shall be formed of 0.062-inch-thick (No. 16, U.S.S. gage) corrosion-resisting steel.

3.3 Finish. The entire inside and outside surfaces of the trays and covers shall be finished with a No. 200 emery, after all surface imperfections such as pits and die-forming marks have been removed by previous grinding. The last grinding shall produce a uniform finished surface with all imperfections and marks of previous grinds removed. The thickness of the sheet forming the trays and covers shall not be reduced below the thicknesses specified in 3.2 by grinding to remove surface imperfections. The resultant finish shall be that known commercially as a No. 4 finish. The interior of the trays and covers may be finished by electropolishing. The electropolishing shall result in a uniform, bright, shiny surface which can be readily cleaned. As a final operation, the trays with covers shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

3.3.1 *Resistance to corrosion.* When tested as specified in 4.4.2, slight surface corrosion of the specimen which can be easily washed off shall not be considered as cause for rejection, but if the specimen should rust or show continuous bleeding from pits, it shall be considered as having failed the test.

3.4 Identification marking. Trays shall be impressed with the manfaucturer's name or registered trademark. In addition, the bottom of the trays shall be die-stamped, or otherwise permanently marked, with the letters U. S. All impressions shall be made at even pressure so as not to penetrate the inside surfaces of the trays. Markings shall be legible and distinct.

3.5 Workmanship. Workmanship shall be first class throughout. Trays and covers shall be free of rough grind marks, trimming marks, pits, scales, and other defects or imperfections. All surfaces shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Supplier responsibilities for inspection. The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 *Inspection.* Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.* When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling. Sampling shall be conducted in accordance with Military Standard MIL–STD–105.

	Inspection level	AQL (percent defective)	Minimum sample size
For visual examination			
Major defects (Total (major and minor combined) defects ...	II	1.0	..
	II	4.0	..
For dimensional examination ..	L5	2.5	..
For salt-spray test	L2	*	3

* Acceptance number shall be zero for all sample sizes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.2.1 *Raw materials.* Four ounces of each lot of metal used in the construction of the trays shall be selected for chemical analysis.

4.3 Examination. The trays shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 *Classification of defects.* Examination shall be conducted in accordance with the following classification of defects:

	Categories and Defects*
Major:	
101.	Tray and cover not free of cracks, tears, ripples, and identification marking penetration (extending to the inside surface of the tray).
102.	Spotwelding of the handle to the cover not firmly secure, reasonably smooth, or otherwise not free of welding defects.
103.	Edges of the tray and cover not free of burs, sharpness, etc.
Minor:	
201.	Finish not as specified and not free of coarse grind marks, scratches, mar marks, etc.
202.	Tray and cover not free of grease, oil, dirt, chips, and foreign particles.
203.	Identification marking omitted, illegible, or not as specified.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 *Dimensional examination.* The trays shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 *Chemical composition.* Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard No. 151.

4.4.2 *Salt-spray test.* Sample trays selected at random shall be tested in accordance with method 811.1 of Federal Test Method Standard No. 151, for a period of 48 hours.

5. PREPARATION FOR DELIVERY

For civil agency procurement only, the definitions and applications of the levels of packaging and packing shall be in accordance with Federal Standard No. 102.

5.1 Packaging.

5.1.1 *Level A or B.* Each tray cover shall be wrapped in kraft paper and placed inverted into the tray. Each unit (tray and cover) shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP–B–636, table I, PPP–B–676, or PPP–B–566, style I. Closure shall be effected in such a manner as to prevent spillage of contents under normal handling.

5.1.2 *Level C.* Trays with covers shall be packaged in accordance with the manufacturer's normal commercial practice.

5.2 Packing.

5.2.1 *Level A.* Twelve units of type I; 50 units of type II, size 1; and 25 units of type II, size 2, packaged as specified in 5.1.1, shall be packed in exterior containers designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; or PPP–B–621, table III. Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Strapping, when required, shall be in accordance with applicable box specification.

NOTE. Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.* Twelve units of type I; 50 units of type II, size 1; and 25 units of type II, size 2, packaged as specified in 5.1.1, shall be packed in exterior containers conforming to Federal Specification PPP–B–601, table I, using class 1 plywood; or designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 2 use; PPP–B–621, table I; or PPP–B–636, type I, class 1, fabricated from not less than 275-pound test fiberboard.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

1. Containers of the type, size, and kind commonly used

5.2.3 *Level C.* The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or order.

5.3 Marking.

5.3.1 *Civil agencies.* In addition to any special marking specified in the contract or order, each unit package and exterior shipping container shall be marked in accordance with Federal Standard No. 123.

5.3.2 *Military agencies.* Each unit package and exterior shipping container shall be marked in accordance with Military Standard MIL–STD–129.

6. NOTES

6.1 Ordering data. Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number, and date of this specification.

(*b*) Type, style, and size required (see 1.2.1).

(*c*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.3 Transportation description. Transportation description applicable to this item is:

Rail:

Sheet steelware, not otherwise indexed by name.

(Specify nested or not nested.)

Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Motor:

Sheet steel articles, not otherwise indexed.

(Specify nested or not nested.)

Motor volume minimum weight 20,000 pounds.

Notice. When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY CUSTODIANS:

Army—MI

Navy—Md

Air Force—AFCSG

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.