RR-T-640
JUNE 27, 1958

FEDERAL SPECIFICATION

TRAY, MEDICINE

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers a corrosion-resisting steel, rectangular tray used to carry catheter trays, thermometer-technique equipment, and medicines to the patient's bedside.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

QQ–S–766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips and Structural Shapes.
PPP–B–585—Boxes, Wood, Wirebound.
PPP–B–601—Boxes, Wood, Cleated-Plywood.
PPP–B–621—Boxes, Wood, Nailed and Lock-Corner.
PPP–B–636—Boxes, Fiber.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.
Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL–B–10377—Box, Wood, Cleated, Veneer, Paper Overlaid.
MIL–L–10547 — Liners, Case, Waterproof.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL–STD–129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material.

3.1.1 *Sheet steel.*—Sheet steel, from which the tray is made, shall conform to class 1 or 2 of Federal Specification QQ–S–766, and shall meet the requirements for chemical composition specified therein, when tested as specified in 4.3.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

3.2 Design.—The tray shall be designed as shown on figure 2. The tray shall be formed seamlessly from one single piece of 0.031-inch (No. 22, United States Standard) steel, which shall not be reduced below 0.025 inch thick at any point. Dimensions shall be as shown on figure 2.

3.3 Finish.—The entire inside and outside surfaces of the trays shall be finished with a No. 200 emery after all surface imperfections such as pits, scratches, and die-forming marks have been removed by previous grinding. This last grinding shall produce a uniform finished surface with all imperfections and marks of previous grinds removed. The thickness of the sheet forming the trays shall not be reduced below the thicknesses specified in 3.2 by grinding to remove surface imperfections. The resultant finish shall be that known commercially as a No. 4 finish. The interior of the tray may be finished by electropolishing. The electropolishing shall result in a uniform, bright, shining surface which can be readily cleaned. As a final operation, the trays shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

3.3.1 *Resistance to corrosion.*—When tested as specified in 4.3.2, slight surface corrosion of the specimen, which can be washed off, shall not be considered cause for rejection, but if the specimen should rust or show continuous bleeding from pits, it shall be considered as having failed to pass the test.

3.4 Identification marking. — Each tray shall be impressed with the manufacturer's name or registered trade-mark. All impressions shall be made at even pressure so as not to penetrate the inside surface of the tray. Markings shall be legible and distinct.

3.4.1 *Marking for Military Medical Supply Agency procurement.* — In addition to the manufacturer's name or registered trade-mark required in 3.4, the bottom of the trays shall be die stamped with a caduceus centered

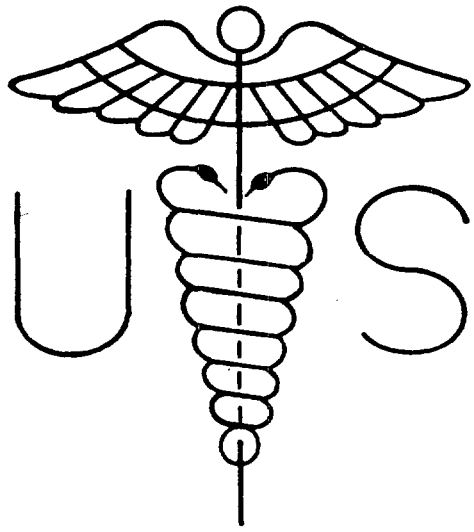


FIGURE 1.

between the letter "U" and "S" conforming to figure 1. The letters shall be ¼ inch high, and the caduceus shall be of appropriate size. All impressions shall be made at even pressure so as not to penetrate the inside surface of the tray. Markings shall be legible and distinct.

3.5 Workmanship.—Workmanship shall be first class throughout. Trays shall be free from defects which detract from their appearance or which may impair their serviceability. Trays shall be free of rough grind marks, trimming marks, pits, scales, or other defects or imperfections. All surfaces shall have a smooth finish and shall be free of sharp edges.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.*—Sampling procedures for visual examination shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105. Unit of product for inspection purposes shall be the individual tray, unless otherwise specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.1.2 *For tests.*

4.1.2.1 *Components.*—Four ounces of corrosion-resisting steel, representative of each lot used in the manufacture of the trays, shall be selected for test.

4.1.2.2 *End item.*—Sample sizes for tests shall be as indicated for inspection level L2 in Appendix to Military Standard MIL–STD–105, except that the acceptance number shall be zero (0) for all sample sizes, and a minimum of three (3) samples shall be taken.

4.2 Inspection.—The inspector shall ascertain that the trays have been examined and tested in accordance with specification requirements.

4.2.1 *Classification of defects.*—Inspection shall be conducted in accordance with the following classification of defects:

Categories and defects

Major AQL 1.0 percent defective

101. Finished thickness of tray material not 0.025 minimum.
102. Tray not free of cracks, tears, ripples, or identification marking penetration (extending to inside surface of tray).
103. Edges of tray not free of burrs or sharpness.
104. Tray fails to bear evenly (without rocking) on a flat surface.

Minor—A AQL 2.5 percent defective

201. Dimensions (except finished thickness) not as specified.
202. Finish not as specified or not free of coarse grind marks, scratches, or mar marks.
203. Tray not free of chips, grease, oil, dirt, or other foreign matter.
204. Identification marking omitted, illegible, or otherwise not as specified.

Minor—B AQL 2.5 percent defective

(Unit of inspection—package)

251. Labels or printing not legible and free of defacing marks, scratches, and tears.

Special requirements*

501. Style and design shall conform to figure 2.
502. Tray material shall be corrosion-resisting steel conforming to the requirements for class 1 or 2 of Federal Specification QQ–S–766.
503. Tray shall be formed or drawn seamlessly from a single piece or blank.
504. Tray shall comply with requirements of 48-hour salt-spray test.
505. Packaging and packing material shall be as specified.
506. Marking material shall be as specified.
507. Marking: Containers shall bear the information as specified.
508. Labeling shall bear the information as specified.

* Noncompliance with any one of the special requirements is cause for rejection.

Note.—Any defect not specifically covered above, but which adversely affects the appearance or serviceability of the tray, shall be added to the above defects in the proper classification as determined by the inspector.

4.3 Tests.

4.3.1 *Chemical composition.* — Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of Federal Test Method Standard No. 151. In lieu of the above, a certificate of quality, showing results of tests performed to indicate that material is as specified in 3.1.1, may be furnished.

4.3.2 *Salt spray.*—Tray(s) shall be tested as specified in method 811 of Federal Test Method Standard No. 151, for a period of 48 hours.

4.4 Supplier responsibilities for inspection.—The supplier shall perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government upon the Government's request, at any time, or from time to time, for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

specification, and all other technical requirements of the contract.

5. PREPARATION FOR DELIVERY

The levels of preservation, packaging, and packing used are defined in Federal Standard No. 102 (for civil agencies only).

5.1 Packaging.

5.1.1. *Unit of issue.*—One tray, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

TABLE I.—*Packaging quantities*

Federal stock number	Unit package	Intermediate package	Shipping container
6530–794–0600	1 unit	6 units	72 units

5.1.2.1 *Packing variation permitted.*—If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be completely wrapped in kraft paper of suitable weight. Wrapper shall be secured to prevent accidental opening.

5.1.3.2 *Intermediate package.*—Intermediate package shall be a carton of appropriate size and design constructed in accordance with Federal Specification PPP–B–636. Carton shall be designed with suitable interior fittings, or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.4 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; PPP–B–621, table III; or Military Specification MIL–B–10377, table II.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.*—Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall conform to Federal Specification PPP–B–601, table I, using type III, class 1 plywood, or shall be designed for type 2 load, and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 2 use; PPP–B–621, table I; or Military Specification MIL–B–10377, table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carrier, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 **Marking.**

5.3.1 *Interior packages.*—Each unit package and each intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 **Ordering data.** — Procurement documents should specify the following:

(*a*) Number and date of this specification.
(*b*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following item appearing in the Armed Services Medical Stock List:

6530–794–0600 TRAY, MEDICINE, Corrosion-Resisting Steel, 13½ by 9⅝ by ⅝ inches.

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the type, etc., which is normally procured to meet Federal Government requirements.

6.4 **Transportation description.**—Transportation applicable to this item is:

Sheet steelware, not otherwise indexed by name. (Specify nested or not nested.)
Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.
Sheet steel articles, not otherwise indexed. Motor volume minimum weight 20,000 pounds.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

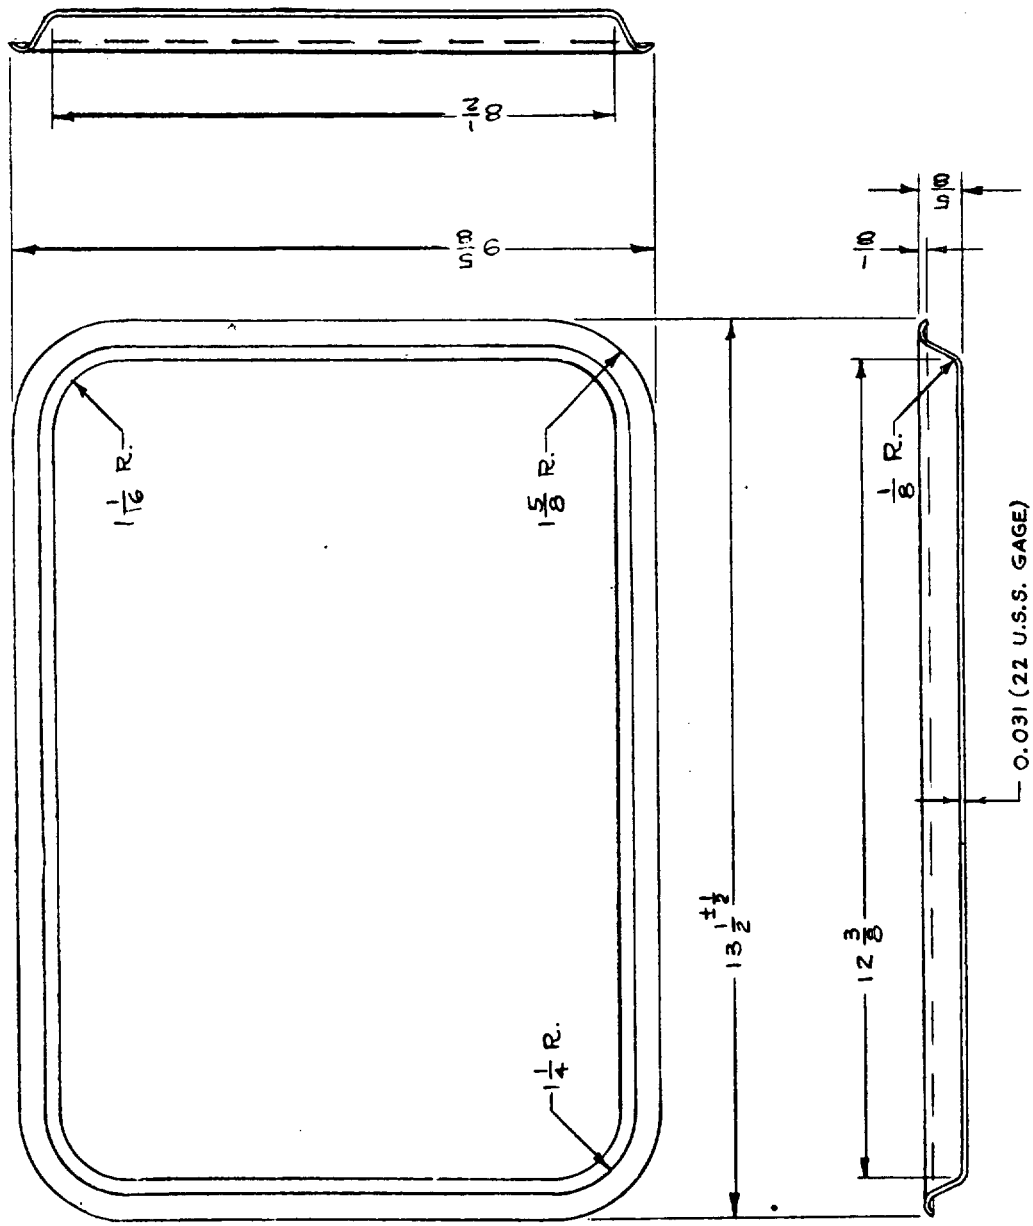


FIGURE 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.