RR-T-00640a (DSA-DM)
January 19, 1971
Interim Revision of
Fed. Spec. RR-T-640
June 27, 1958

INTERIM FEDERAL SPECIFICATION

TRAY, MEDICINE

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification RR-T-640.

1. SCOPE

1.1 This specification covers a corrosion-resisting steel, rectangular tray for use in carrying catheter trays, thermometer-technique equipment, and medicines to the patients bedside.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive, Water Resistant (For Sealing Waterproofed Paper).
PPP-B-566	Box, Folding Fiberboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.
PPP-T-76	Tape, Pressure, Sensitive Adhesive Paper, Water Resistant (For Carton Sealing).

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-66	Steel; Chemical Composition and Hardenability.
FED-STD-151	Metals; Test Methods.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specification and Standards and the Index of Federal Specification and Standards from established distribution points in their agencies.)

(Copies of Military specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Trays shall be corrosion-resisting steel conforming to class 302 or 304 of FED-STD-66, and shall meet the requirements for chemical composition specified therein when tested as specified in 4.4.1.

3.2 Construction. The tray shall be as shown in Figure 1 and as hereinafter specified. The tray shall be formed seamlessly from one piece of corrosion-resisting steel, which shall not be reduced below 0.025 inch thick at any point. The bottom shall concave inward so that the highest point shall be no more than 1/16 inch above the surface upon which the tray rests. The tray shall rest on all four bottom corners without rock or wobble.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:11Z
Check the source to verify that this is the current version before use.

3.3 Finish. The entire inside and outside surfaces of the tray shall be finished with a No. 200 emery after all surface imperfections such as pits, scratches, and die-forming marks have been removed by previous gringing. The last grinding shall produce a uniform finished surface with all imperfections and marks of previous grinds removed. The thickness of the sheet forming the trays shall not be reduced below the thicknesses specified in 3.2 by grinding to remove surface imperfections. The resultant finish shall be that known commercially as a No. 4 finish. The interior of the tray may be finished by electropolishing. The electropolishing shall result in a uniform, bright, shining surface which can be readily cleaned. As a final operation, the trays shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

3.3.1 Resistance to corrosion. When tested as specified in 4.4.2, slight surface corrosion of the specimen, which can be washed off with water shall not be considered cause for rejection, but if the specimen should rust or show continuous bleeding from pits, it shall be considered as having failed to pass the test.

3.4 Identification marking. Each tray shall be impressed with the following:

Manufacturer's name or registered trademark
Contract or purchase order number
Federal Stock Number
U.S.

Lettering shall be not less than 1/4 inch high. All impressions shall be made at even pressure so as not to penetrate the inside surface of the tray. Marking shall be legible and distinct. Marking secured by adhesives shall not be used.

3.5 Workmanship. Workmanship shall be first class throughout. Trays shall be free from defects which detract from their appearance or which may impair their serviceability. Trays shall be free of rough grind marks, trimming marks, pits, scales, or other defects or imperfections. All surfaces shall have a smooth finish and shall be free of sharp edges.

4. QUALITY ASSURANCE PROVISIONS

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

* 4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

* 4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the trays may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the component material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Classification of Inspections.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and Table I.

Table I.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	S-4	1.0
Minor defects	S-4	2.5
For dimensional examination	S-1	2.5

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:11Z
Check the source to verify that this is the currenversion before use.

* 4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as shown in Table II.

Table II.

Component	Characteristic	Requirement	Test Procedure	Inspection level	AQL Percent defective
Tray	Chemical composition	3.1	4.4.1	**	***
Tray	Corrosion resistance	3.3.1	4.4.2	S-1	***

** Sample as specified in 4.2.2.1.
*** Acceptance number shall be zero (0) for all sample sizes, and a minimum of three (3) samples shall be taken regardless of lot size.

4.2.2.1 Raw material. Four ounces of corrosion-resisting steel, representative of each lot used in the manufacture of the trays, shall be selected for chemical analysis.

4.3 Examination. The trays shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects shown in Table III.

* Table III. Classification of Defects

Categories	Defects
Major	
101	Finished thickness of tray material not 0.025 minimum.
102	Tray not free of cracks, tears, ripples, or identification marking penetration (extending to inside surface of tray).
103	Edges of tray not free of burrs or sharpness.
Minor	
201	Dimensions (except finished thickness) not as specified.
202	Finish not as specified or not free of coarse grind marks, scratches, or mar marks.
203	Tray not free of chips, grease, oil, dirt, or other foreign matter.
204	Identification marking omitted, illegible, or otherwise not as specified.
205	Tray fails to bear evenly (without rocking) on a flat surface.

* Examination shall not be restricted to the classified possible defects listed above.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The trays shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of FED-STD-151. In lieu of the above, a certificate of quality, showing results of tests performed to indicate that material is as specified in 3.1 may be furnished.

4.4.2 Salt spray. Tray(s) shall be tested as specified in method 811.1 of FED-STD-151 for a period of 48 hours.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One tray, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	72 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5.1.3.1 Unit package. Each tray shall be thoroughly cleaned, wrapped in tissue paper or other suitable material. The unit shall be further packaged in a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to Method II of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

* 6. NOTES

6.1 Use. Transportation of thermometer technique equipment, cotton pledgets, and medicines, to patients' bedsides, in military medical facilities.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).

6.3 This specification covers the following item appearing in the Federal Supply Catalog:

FSN	Item
6530-794-0600	Tray, Medicine

6.4 This specification does not include all types, classes, grades, and sizes, of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, which are normally procured to meet Military requirements.

* 6.5 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6530-1189

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

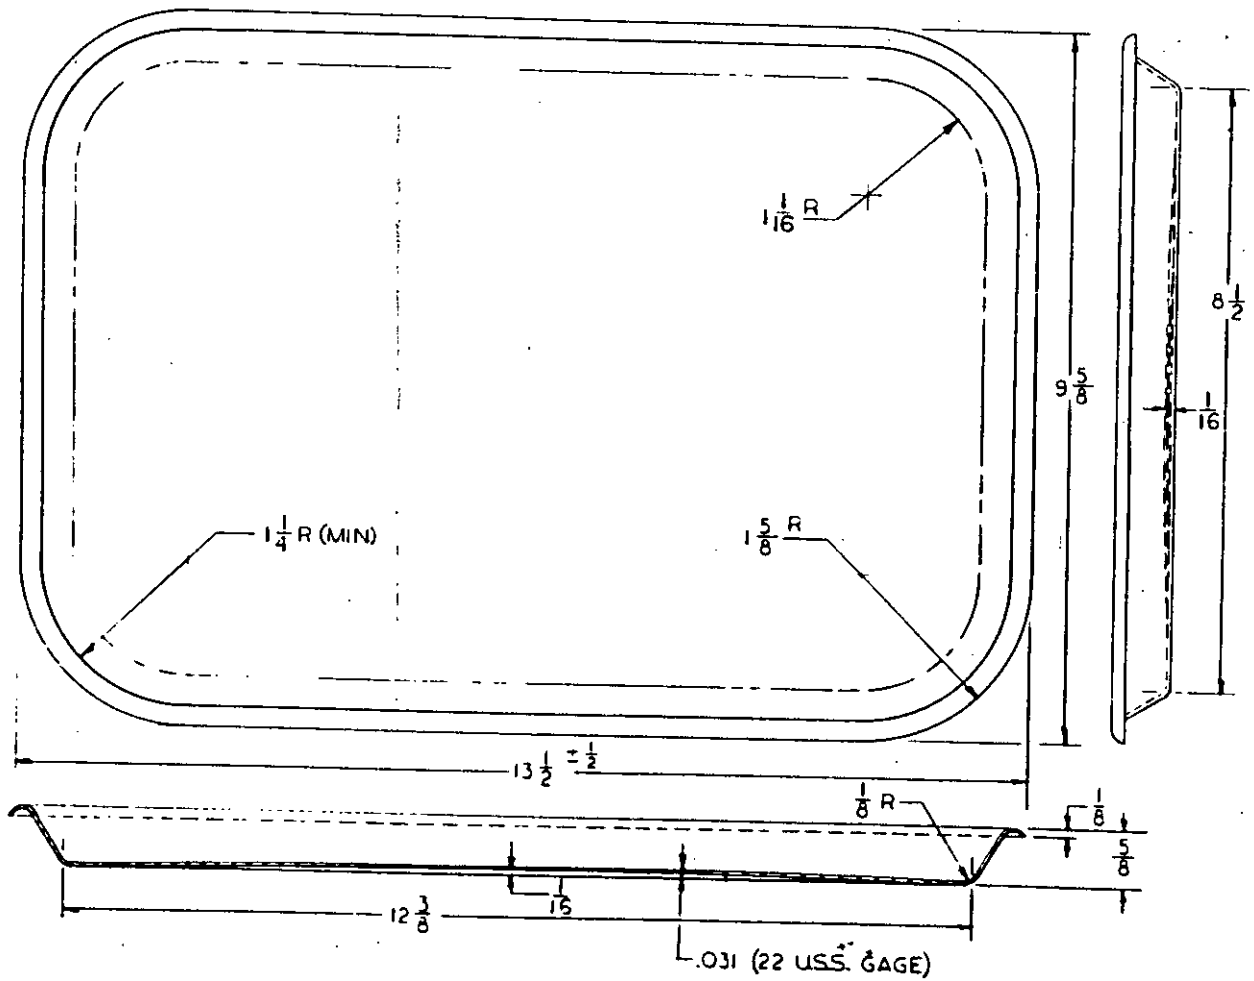

UNLESS OTHERWISE INDICATED:
DIMENSIONS OVER 1 INCH ± 3/8
DIMENSIONS UNDER 1 INCH ± 1/16

FIGURE -1-

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION
RR-T-00640a(DSA-DM) FSN:

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?
   ☐ YES ☐ NO (If "yes", in what way?)

4. REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)

SUBMITTED BY (Printed or typed name and activity - Optional) | DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 54, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.