A-A-50223
September 23 1986

COMMERCIAL ITEM DESCRIPTION

SCALE, BEAM INDICATING: WEIGHING, SPECIFIC GRAVITY; CAPACITY 0.01 NOT LESS THAN 200 GRAMS, THREE OR FOUR WEIGHT BEAMS: 0.01 GRAM SENSITIVITY

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-S-11510.

This description covers a three or four beam type scale with an adjustable platform as shown on figures 1 and 2.

Design. The scale shall have a capacity of 0.01 gram to not less tha 200 grams, a sensitivity of 0.01 gram at the capacity load. The scale shall consist of a weight beam, stirrup, pan, platform, and include a damping feature.

Metal. Corrosion-resistant or metal made corrosion-resistant by a suitable treatment.

Weight beam. The weight beam shall be equipped as follows:

a. Two or three bars with hanging, sliding poises, or riders.
b. Fractional bar having a capacity of 1 gram, graduated in 0.01-gram increments, and provided with a sliding poise or rider.
c. An adjustment for setting zero point.
d. An adjustment means for leveling the scale when out of level condition affects accuracy.

Stirrup. This stirrup shall be corrosion-resisting steel approximately 8 inches (203.2 mm) high and approximately 4 inches (101.6 mm) wide.

Pan. The pan shall be made from aluminum, polypropylene or corrosion-resisting steel, shall be removable from the stirrup, or movable to a vertical position within the stirrup.

Platform. The platform for specific gravity determinations shall be adjustable.

Damping. Damping shall be incorporated into the scale. The following methods are acceptable: Magnetic, air or oil.

Accuracy. Accuracy shall not be effected by the scale being out-of-level.

Plastic cover. A plastic cover designed to fit the scales specified herein, shall be provided.

AMSC N/A FSC 6670

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:41Z
Check the source to verify that this is the current version before use.

Regulatory requirements. The offeror/contractor is encouraged to use recovered materials in accordance with Public Law 94-580 to the maximum extent practical.

Packaging and marking. Military packaging shall be specified when shipments are to overseas Department of Defense (DOD) connsignees. Commercial packaging may be specified for shipments to DOD consignees within the Continental United States and to non-DoD cosignees worldwide. When a supplier's normal packaging will satisfy the requirements for military packaging, it may be used.

Military packaging. Each scale shall be preserved and packed to protect against physical damage and deterioration in a logistic environment characterized by the following:

1. Multiple handling during transportation and intransit storage.
2. Shock, vibration, and static loading forces during worldwide shipment by all transport modes.
3. Uncontrolled warehouse storage for extended periods.
4. Weather exposure during shipment and intransit transfers.
5. Stacking loads during shipment and storage.

Quantities of scale of like description destined to a single addressee may be untized into one or more unit loads.

Commerical. Each scale shall be packed in accordance with the supplier's normal method for retail distribution. Individually poackaged scales of like description shipped to a single destination may be unitized to permit handling as a single unit. Shipping containers shall comply with Uniform Freight Classification or National Motor Freight Classification rules.

Marking. Unit, intermediate (when provided), and exterior packs shall be marked with the item nomenclature, stock or part number, quantity per pack, and contract number as a minimum; additional marking shall be as specified in the contract or order. Exterior packs shall have in addition the complete consignee's address. Markings shall be applied in a legible manner, in a contrasting color, of an appropriate size, and of water-proof materials.

Quality assurance. The scales shall be examined for the following defects. Presence of one or more defects shall be cause for rejection.

1. Capacity and sensitivity not as specified.
2. Materials not as specified.
3. Not equipped as specified.
4. Dimensions not as specified.
5. Damping not as specified.
6. Accuracly effected by scale out-of-level.
7. Packaging and marking not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026t0-26T08:41Z
Check the source to verify that this is the currentversion before use.

Certification of commercial item. The contractor shall certify that the product offered to the Government meets the salient characteristics of this description and that the product conforms to the producer's own drawings, specifications, standards, and quality assurance practices and is the same product as the manufacturer's current product offered by the contractor in the commerical market place for at least one year preceding the solicitation. The Government reserves the right to require proof of such conformance prior to first delivery thereafter as may be otherwise provided for under the provisios of the contract.

Small business. A small business that cannot meet the certification-of-commercial-item requirement of this document, may make an offer under this solicitation; and, if such small business is theapparent successful offeror, the Government may require the small business to submit a sample scale. Any such scale may be evaluated for this solicitation if time to contract award permits. Such evaluation would be to determine conformance to all requirements of this commercial item description and to determine equivalency to scales available in the commercial market-place in the areas of durability, human factors engineering and safety. It should be noted that bid samples are not required unless specifically requested by the contracting officer. Note. The Government may elect not to evaluate a bid sample from an apparent low bidder for award for this solicitation if a determination of urgency is made by the contracting officer. The bid sample would then be evaluated prior to future solicitation for comparable items.

Notes.

1. Figures 1 and 2 are included for illustration only and are not intended to preclude the furnishing of other scales which conform to this description.
2. When this commercial item description is used for procurement, the commercial item certification clause must appear in the solicitation.

MILITARY INTERESTS:

Custodians
Army - ME
Air Force - 99

Review Activities
Army - MD
Air Force - 82
DLA - GS

User Activity
Army - GL


CIVIL AGENCY COORDINATING ACTIVITY:

GSA-FCGC

PREPARING ACTIVITY:
Army - ME

Project 6670-0152

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:41Z
Check the source to verify that this is the current version before use.

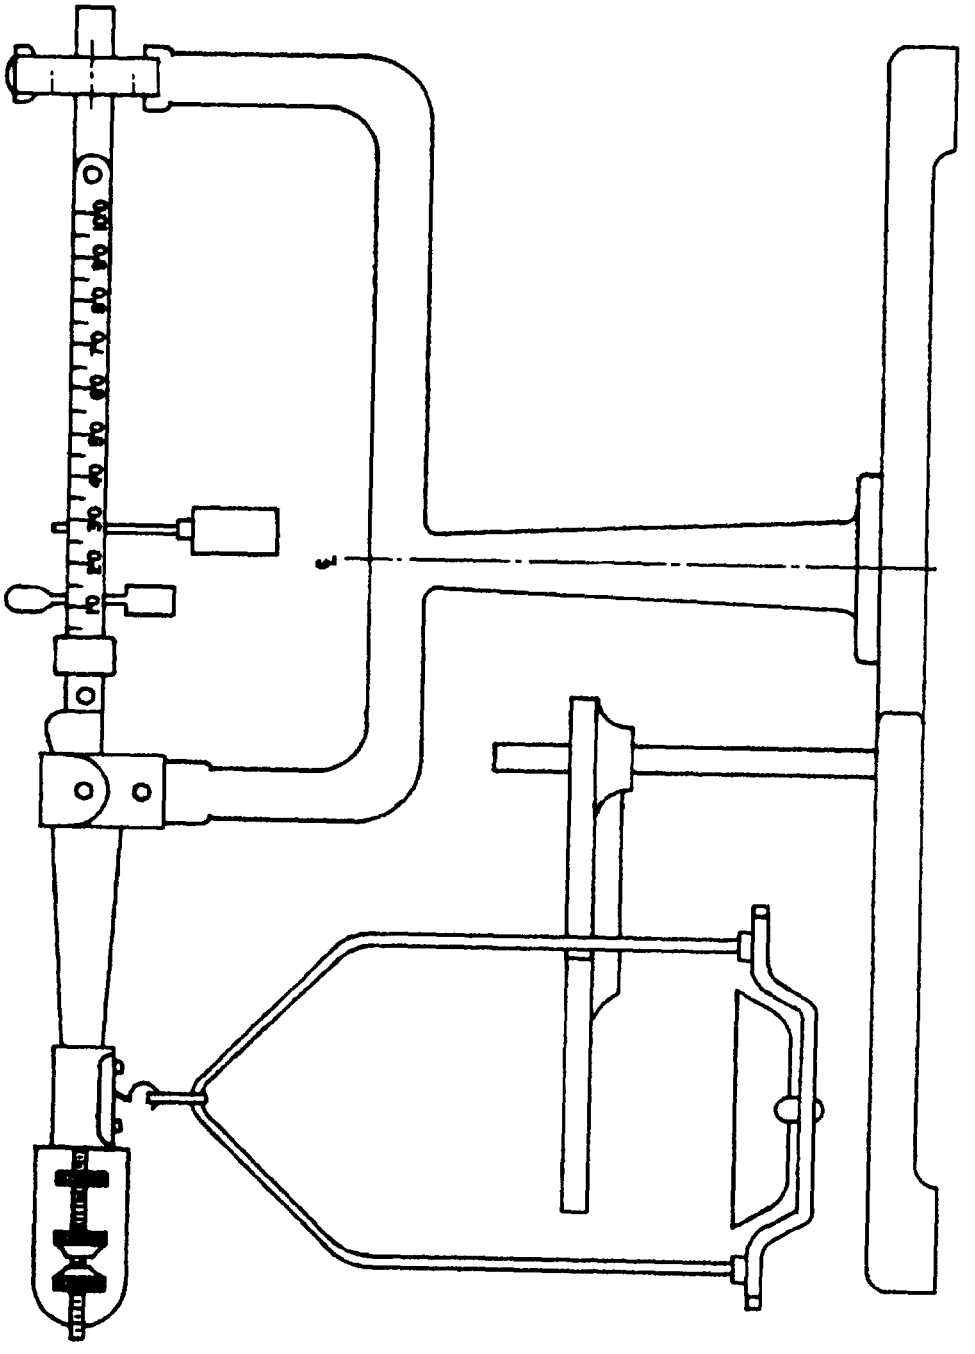

X-1009A

FIGURE 1. Scale, beam indicating.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:41Z
Check the source to verify that this is the current version before use.

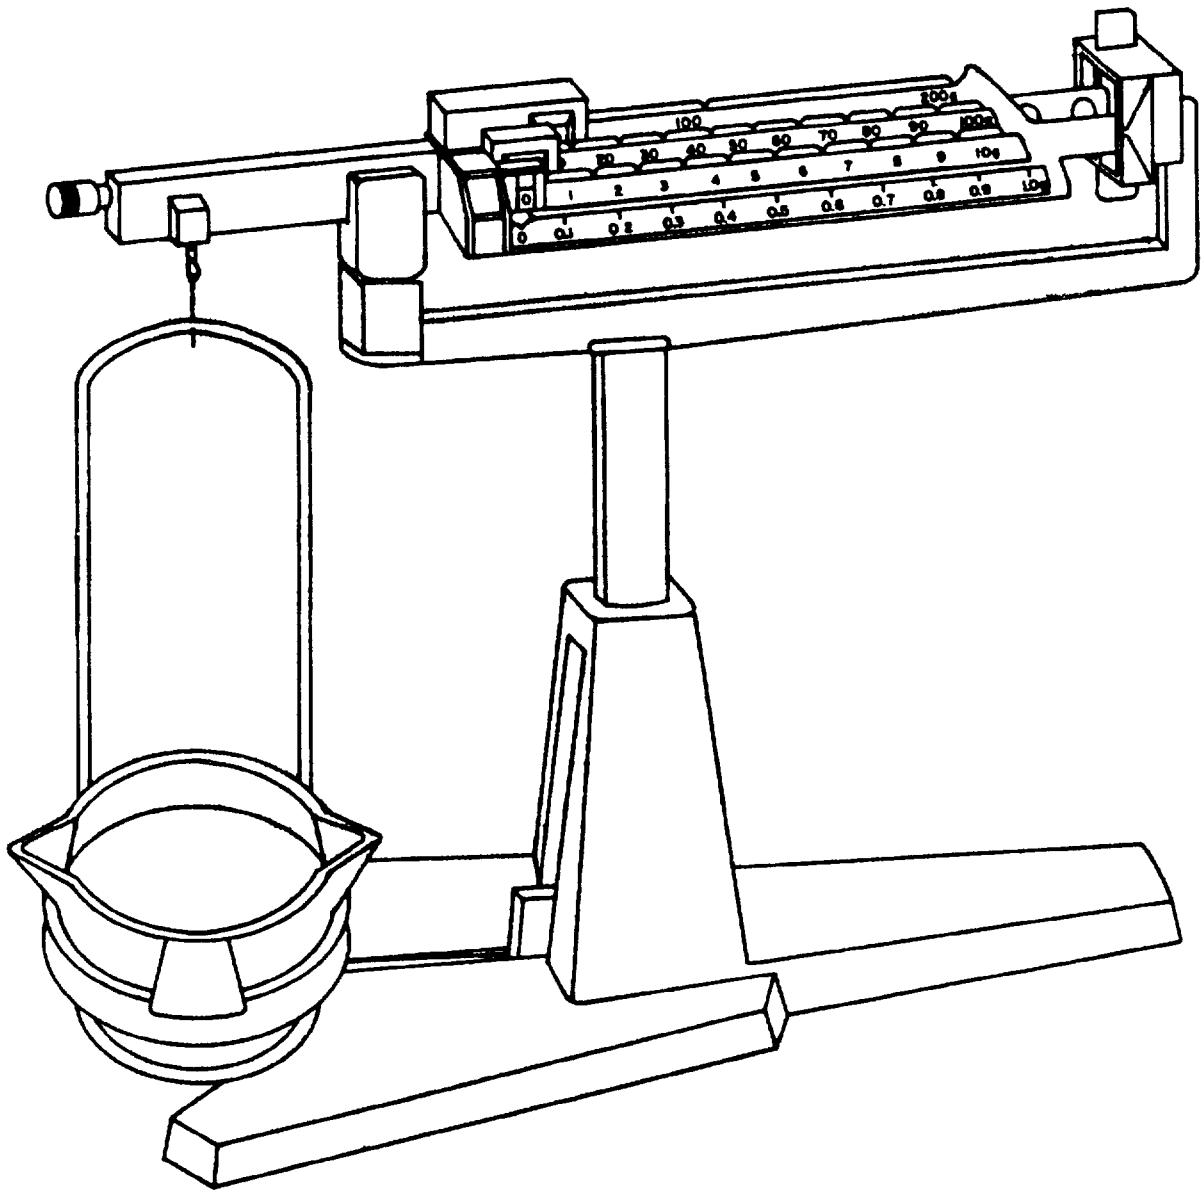


FIGURE 2. Scale, beam indicating.

X-1964

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:41Z
Check the source to verify that this is the current version before use.