MIL-C-36757A
8 September 1976
SUPERSEDING
MIL-C-36757
11 March 1971

MILITARY SPECIFICATION

CEMENT, ZINC OXIDE AND EUGENOL, DENTAL
(Intermediate Restorative Material)

This specification is approved for use by all the Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers zinc oxide and eugenol dental cement suitable for use as an intermediate restorative material.

1.2 Classification. The cement shall be of the following colors as specified (see 3.4 and 6.1):

Color 1 - Ivory
Color 2 - Red
Color 3 - Blue

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

PPP-B-566 - Boxes, Folding, Paperboard.
PPP-B-585 - Boxes, Wood, Wirebound.
PPP-B-601 - Boxes, Wood, Cleated-plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-corner.
PPP-B-636 - Boxes, Shipping, Fiberboard.
PPP-B-676 - Boxes, Setup.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, Code ATT, 2800 South 20th Street, Philadelphia, Pa. 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

MILITARY

MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN CHEMICAL SOCIETY (ACS) PUBLICATIONS

Reagent Chemicals, ACS Specifications

(Application for copies should be addressed to the American Chemical Society Publications, 1155 Sixteenth Street, N.W., Washington, D.C. 20036.)

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM D2240 - Tests for Identification Hardness of Rubber and Plastics by Means of a Durometer.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa. 19103.)

THE UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The Pharmacopeia of the United States of America (U.S.P)

(Application for copies should be addressed to the Mack Publishing Company, Easton , Pa. 18042.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

U.S. DEPARTMENT OF HEALTH, EDUCATION, AND WELFARE
FOOD AND DRUG ADMINISTRATION

Federal Food, Drug, and Cosmetic Act and regulations promulgated thereunder.

(Application for copies should be addressed to the Food and Drug Administration, Washington, D.C. 20204.)

3. REQUIREMENTS

3.1 Materials. The materials shall be of a high quality and purity suitable for purpose intended and as specified below. The materials shall be free of extraneous material such as dirt or lint and shall be furnished clean and ready for use.

3.1.1 Powder. The composition of the cement powder shall be essentially zinc oxide, Lake Number 3 red pigment (for color 2), Lake Number 1 blue pigment (for color 3), a zinc acetate accelerator, and high molecular weight polymethyl methacrylate. Cement powder shall contain no abrasive fillers such as quartz or alumina. The quality of the materials shall be as follows:

a. Zinc oxide shall be in accordance with the tests, standards, and requirements of the current Pharmacopeia of the United States of America (U.S.P.), including any supplements or revisions thereto, for lead and arsenic content only.

b. Pigments used for colors 2 and 3 shall be of drug or cosmetic grade. The pigment shall be suitable for coloring drugs or cosmetics under the Federal Food, Drug and Cosmetic Act and the Color Additive Regulations.

c. Zinc acetate shall be in accordance with the tests, standards, and requirements of the current U.S.P., including any supplements or revisions thereto.

d. The polymethyl methacrylate shall be nontoxic. The manufacturer shall submit a statement to the contracting officer that the polymer furnished has no toxic effect on the normal, healthy person.

3.1.2 Liquid. The composition of the liquid shall be eugenol, with acetic acid added as an accelerator. Eugenol shall conform to the tests, standards and requirements of the current U.S.P., including any supplements or revisions thereto. The acetic acid shall conform to the requirements of analytical reagent chemicals of American Chemical Society (A.C.S.) grade contained in the American Chemical Society publication, "Reagent Chemicals, A.C.S. Specifications."

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

3.2 Description. Zinc oxide and eugenol dental cement shall consist of a plastic bottle containing a minimum of 38.0 grams (g) of cement powder, an amber glass bottle containing a minimum of 14.0 milliliters (ml) of liquid (closed by a screw cap), a plastic dropper assembly with butyl rubber cap for dispensing liquid, and a plastic powder scoop. The dental cement shall be suitable as a sedative intermediate restorative material which may also be used as a base under amalgam restorations. The cement shall not form lumps, granules, or evolve gas when mixed according to manufacturer's instructions (see 3.6).

3.2.1 Accessories. The powder scoop shall be fabricated of clear styrene and shall deliver 0.20 to 0.24 grams of powder. The plastic dropper shall be designed to deliver 5.2 to 6.3 powder-liquid ratio by weight, when tested as specified in 4.3.7.

3.3 Physical properties. The physical properties of dental cement shall comply with the requirements of table I.

TABLE I. Physical Properties.

Characteristics	Requirements
Setting time	7.5 to 9.5 minutes.
Compressive strength	9000 pounds per square inch, minimum.
Solubility and disintegration	0.12 percent by weight, maximum.
Film thickness	50 to 90 microns.
Consistency	16.5 - 19.5 millimeters.

3.4 Color.

3.4.1 Color 1. Cement shall be ivory in color to indicate cement is for use in anterior teeth or when color coding is not required.

3.4.2 Color 2. Cement shall be red in color to indicate that dental caries remain.

3.4.3 Color 3. Cement shall be blue in color to indicate that all dental caries have been removed.

3.5 Compatibility. The immediate containers and all components shall be compatible, and shall not interact physically or chemically with the dental cement.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

3.6 Instructions. Adequate and accurate instructions for using the dental cement shall accompany each unit package. In addition, the instructions shall include setting time, mixing time, powder-liquid ratio, and methods for proportioning and manipulating the cement, including number of drops of liquid required to mix with one scoop of powder to make a mix of 5.2 to 6.3 powder-liquid ratio by weight. Two copies of instructions shall be forwarded to the contracting officer for information purposes.

3.7 Shelf life. The shelf life of the cement shall be no less than 24 months from date of manufacture when stored at controlled room temperature (59 to 86 degrees Fahrenheit (^{o}F)).

3.8 Labeling. Each bottle and individual bottle carton shall be permanently and legibly labeled with the name of contents and the manufacturer's name or registered trademark. In addition, each bottle shall be marked with a serial number or combination of letters and numbers which shall refer to the manufacturer's record for that particular lot or batch. The year and month of manufacture shall be suitably coded as part of the lot number.

3.9 Workmanship. Workmanship shall be first class throughout. The immediate containers shall be free from all dirt, foreign materials, and impurities which detract from their appearance or which may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of supplies to which such records relate.

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials specified in 3.1.1 and 3.1.2, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties). Sampling for inspection shall be performed in accordance with MIL-STD-105, except where otherwise indicated hereinafter.

4.2.1 Examination. The dental cement shall be examined for defects including, but not limited to, those listed in table II.

TABLE II. Classification of defects.

Categories	Defects
Major:	
101	Color not as specified.
102	Material not free from foreign matter.
103	Broken or cracked bottle.
Minor:	
201	Instructions not present with unit package, incorrect, incomplete or not applicable to material furnished.
202	Accessories (powder scoop and liquid dropper) not present in unit container.
203	Powder scoop and liquid dropper not of proper size.

The inspection levels and acceptable quality levels (AQL) shall be as listed in table III. The unit of product for examination shall be one package (unit of issue) of dental cement.

TABLE III. Examination criteria.

Type defect	Inspection level	AQL (percent defective)
Major	S-2	1.0
Minor	S-2	2.5

4.2.2 Packaging inspection. The inspection of the unit, intermediate package, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

4.2.3 Testing. Cement shall be tested as specified in table IV and 4.3. The unit of product for testing shall be one package (unit of issue) of dental cement.

TABLE IV. Sampling for tests.

Characteristic	Reqmt.	Test procedure	Units of products to be tested per lot or batch number	Number of determinations per unit of product	Total number of determinations per lot or batch number
Consistency	3.3	4.3.2	1	3/1	3
Setting time	3.3	4.3.3	1	3/2	3
Compressive strength	3.3	4.3.4	1	5/1	5
Solubility and disintegration	3.3	4.3.5	2	1/1	2
Film thickness	3.3	4.3.6	1	3/1	3
Power-liquid ratio	3.2.1	4.3.7	1	5/1	5

/1 A lot shall be rejected if the average of the determinations per unit of product fails the test.

/2 A lot shall be rejected if any of the determinations per unit of product fails the test.

4.2.4 Sample unit usage. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Tests.

4.3.1 Preparation of test specimens. The preparation of test specimens shall be conducted at a temperature of 21 to 24 degrees Centigrade (^{o}C) (70 to 75° F), and 45 to 55 percent relative humidity with a powder-liquid ratio of 5.2 to 6.3 by weight (standard consistency), when mixed on glass slab or parchment dental mixing pad.

4.3.2 Consistency. The apparatus used for measuring consistency consists of two flat glass plates, a weight, a gauge plug, and a glass tube (inside diameter approximately 6.5 millimeters (mm), which will deliver 0.50 millileter (ml), of mixed cement (see figure 1). The combined weight of the top plate and the weight shall be 520 g. First, 0.50 $\pm$ 0.02 ml of sample, prepared as specified in 4.3.1, shall be delivered from the glass tube onto a flat glass plate. Two minutes after the mixing is started, the top glass plate weighing

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

approximately 20 g, and the necessary additional weight required to total 520 g shall be carefully lowered onto the soft cement. Ten minutes after starting the mix, the average of the major and minor diameters of the slumped mass of cement shall be the consistency of the mixed cement. One type of apparatus for measuring test consistency is shown in figure 1. The average of three such determinations shall be the consistency of the mixed cement.

4.3.3 Setting time. A mix of cement using 0.25 ml of liquid and an amount of powder in proportion specified in 4.3.1, shall be loaded into a polyethylene crown form cap with approximate internal dimensions of 9.5 mm diameter by 7 mm deep. Type A durometer hardness shall be determined as described in American Society for Testing and Materials (ASTM) Designation D2240. Readings shall be taken at 0.5 minute intervals. Hardness shall be plotted against time, and the setting time in minutes shall be the interpolated value of time when durometer reading equals 50. Setting time shall be reported to the nearest 0.5 minute.

4.3.4 Compressive strength. Five test specimens shall be prepared. The test specimens shall be cylinders 12 mm (0.472 inch (in.) high and 6 mm (0.236 in.) in diameter. The ends of the specimens shall be flat and smooth and shall be parallel to each other and at right angles to the long axis of the cylinder. An apparatus found convenient for forming these test cylinders is shown in figure 2. A cylinderical mold 12 mm (0.472 in.) high and 6 mm (0.236 in.) in diameter shall be placed on a flat glass plate and slightly overfilled with cement of standard consistency within three minutes after commencing the mixing. A second flat glass plate shall be pressed on top of the mold. The mold and plates shall be held firmly together with a small "C" clamp. All apparatus shall be at room temperature. The molds shall be made of hard rubber, glass, stainless steel or any other substance which will not react with the cement. The molds may be coated with a 3 percent solution of a micro-crystalline wax (melting point 86 to 91°C (187° to 196° F) in benzene. Three minutes after starting the mix, the mold and clamp shall be transferred to an atmosphere of 100 percent relative humidity at 37° C (99°F). One hour later the ends of the cylinder shall be surfaced plane at right angles to the axis. The ends of the specimens may be ground flat by the use of a small amount of 200-mesh silicon carbide powder and water. The molds containing the specimens shall be drawn back and forth across a glass plate coated with the abrasive and water. They shall be rotated about one-fourth turn every few strokes. The test specimens shall be kept wet during the grinding. A small piece of cloth, wet with distilled water, shall be wrapped around circumference of the specimen. After surfacing, the specimens may be removed from the mold by a screw jack (figure 2) and shall be stored for one week in water at 37° C before crushing. Test equipment used for determining compressive strength shall be the Instron Engineering Corporation's Test Machine, or other suitable equipment, provided prior approval is received from the contracting officer. Testing conditions on the Instron test machine shall be as follows:

a. Crosshead speed of 0.2 inches per minute.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

b. Force range of 1000 pounds.
c. Chart speed of 10 inches per minute.

The value for compressive strength shall be reported as the average of three or more from a lot of five specimens and shall be rounded off to the nearest 50 pounds. If the values for individual specimens fall more than 15 percent below the average of the five, they shall be discarded and the average of the remaining specimens shall be reported. In case more than two of the specimens are eliminated, the test shall be repeated.

4.3.5 Solubility and disintegration. One half milliliter of mixed cement shall be prepared in accordance with 4.3.1. The mix shall be placed in a split stainless steel ring (inside diameter 20 mm (0.79 in.) and 1.5 mm (0.059 in.) thick) which is sitting on a thin polyethylene sheet backed by a flat plate. Another flat plate faced with a sheet of thin polyethylene shall be used to press the cement into the ring. A piece of fine platinum or corrosion-resistant wire shall be placed in the soft cement as the specimens are formed to provide a convenient means of holding the specimens. Three minutes after the mix is started, the plates and cement shall be placed for one hour in an atmosphere having a relative humidity of 100 percent at 37° C (99° F). After one hour, the specimens shall be withdrawn from the oven and two specimens shall be placed in each of two tared weighing bottles and weighed (figure 3). The combined weight of the two specimens and the weighing bottle, less the weight of weighing bottle and the platinum wire, shall be taken as the weight of the specimens of cement. The specimens shall immediately be submerged by pouring 50 ml of distilled water into the weighing bottle, which shall be stored for 23 hours at 37° C (99° F). The specimens shall then be removed from the water. There shall be no evidence of crystal growth on the surface of the specimens. The water shall be evaporated from the weighing bottle at a temperature just below 100° C (212° F). The weighing bottle shall then be dried at 150° C (302° F) to constant weight. After cooling to room temperature in a desiccator, containing thoroughly dry anhydrous calcium sulfate ($CaSO_4$) or silica gel (freshly dried at 130° C), the weighing bottle and contents shall be weighed with a precision of 0.2 milligram (mg). This cycle of heating the weighing bottle to 150° C, cooling over a desiccant and reweighing shall be repeated until the weight loss of each bottle is no more than 0.5 mg in any 24 hour period. The difference between the final weight of the weighing bottle and its initial weight shall be the amount of disintegration. The gain in weight divided by the weight of the specimens times 100 gives the percent of disintegration. The average of duplicate tests (two weighing bottles containing two specimens each) shall be reported to the nearest 0.1 percent.

4.3.6 Film thickness. A portion of a mix of standard consistency (see 4.3.1) shall be placed between two flat square or round glass plates of uniform thickness. The surface areas of the plates between which the cement is spread shall be approximately 2 square centimeters (0.31 square in.). Three minutes after the mix is started, a load of 15 kilograms (33 pounds) shall be applied

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

vertically on the top plate. Ten minutes after the mix is started, the thickness of the two plates with the cement film between them shall be determined. The difference in the thickness of the plates with and without the cement film shall be considered as the film thickness. An average of three tests shall be reported to the nearest 5 microns (0.0002 in.).

4.3.7 Powder-liquid ratio. The powder-liquid ratio shall be determined by weighing the powder dispensed from the powder scoop and weighing the liquid dispensed by dropper in the number of drops stated in the manufacturer's instructions. Five determinations of the weight of powder, and of liquid shall be made and the average weights calculated. The powder-liquid ratio shall be calculated using the average weight values.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.1).

5.1.1 Unit of issue. One package containing one bottle of powder, one bottle of liquid, measuring scoop, dropper, and instructions as specified, constitutes one unit of issue.

5.1.1.1 Level A.

5.1.1.1.1 Unit packaging. Each bottle of liquid (along with one dropper), and each bottle of powder shall be individually packaged in a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676. Both of the above cartons, along with the instructions and measuring scoop, shall be further overboxed in a carton of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676. Closure of box shall be as specified in the appendix of the applicable box specification.

5.1.1.1.2 Intermediate packaging. Six (6) units of issue shall be packaged in a box of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic. Closure of box shall be as specified in the appendix of PPP-B-636.

5.1.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.1).

5.2.1 Level A. Ninety six (96) units of issue shall be packed in a box designed for a type 2 load, and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2 or PPP-B-636, class weather resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with the appendix of PPP-B-636.

5.2.2 Level B. Ninety six (96) units of issue shall be packed in a box designed for a type 2 load, and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, type CF, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. Contract or purchase order number, lot (control) number, name of contractor, date of manufacture (in lieu of date packaged), and the following legend shall be shown:

"STORE AT CONTROLLED ROOM TEMPERATURE 15° - 30° C, (59° - 86° F)".

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot (control) number, date of manufacture (in lieu of date packed), and the following legend shall be shown:

"STORE AT CONTROLLED ROOM TEMPERATURE (15° - 30° C (59° - 86° F)".

6. NOTES

6.1 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents:

(a) Title, number, and date of this specification.
(b) Color required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

6.2 National Stock Number (NSN) Coverage. This specification covers the following items appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6520-00-181-7732	CEMENT, ZINC OXIDE AND EUGENOL, DENTAL, Intermediate Restorative, Ivory, 38 Gram
6520-00-181-7735	CEMENT, ZINC OXIDE AND EUGENOL, DENTAL, Intermediate Restorative, Red, 38 Gram
6520-00-181-7736	CEMENT, ZINC OXIDE AND EUGENOL, DENTAL, Intermediate Restorative, Blue, 38 Gram

6.3 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to the previous issue, due to extensiveness of the changes.


Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA-DM

Project No. 6520-1426

☆U.S. GOVERNMENT PRINTING OFFICE: 1976–703-020/92

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

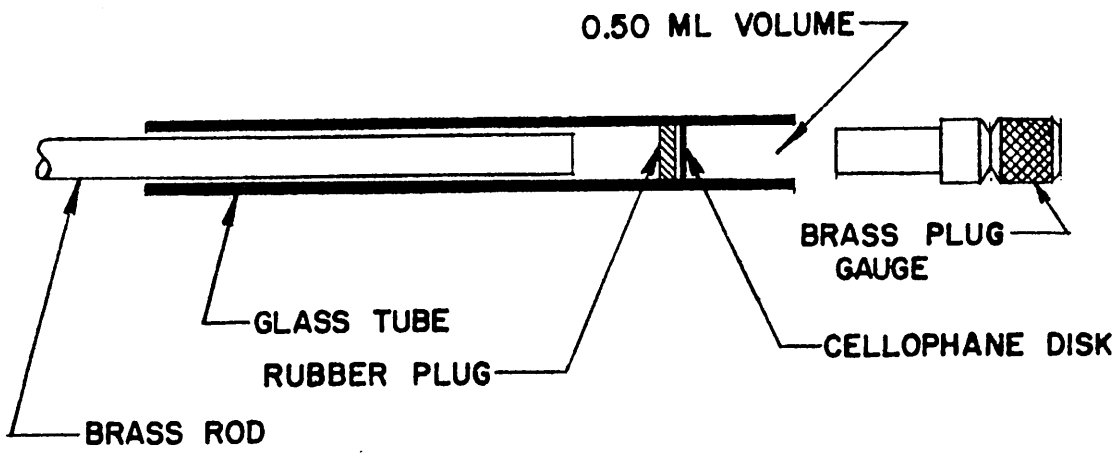

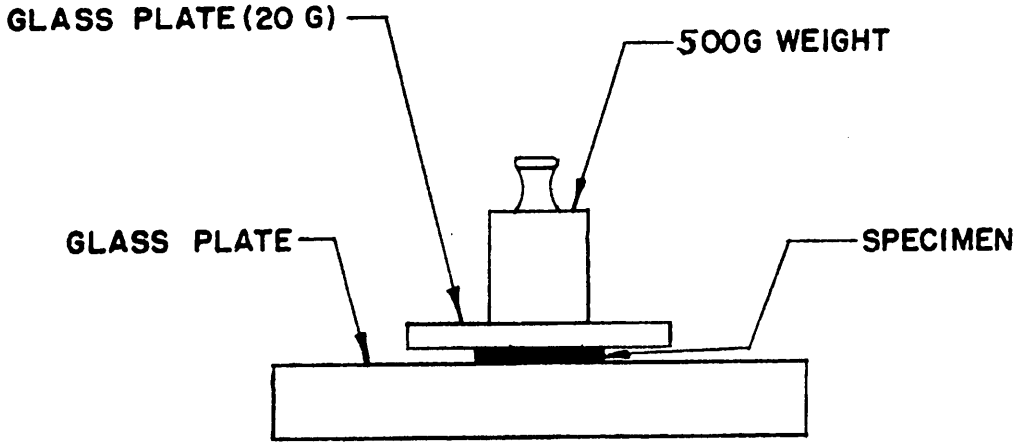


FIGURE 1, APPARATUS FOR CONSISTENCY TESTS

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

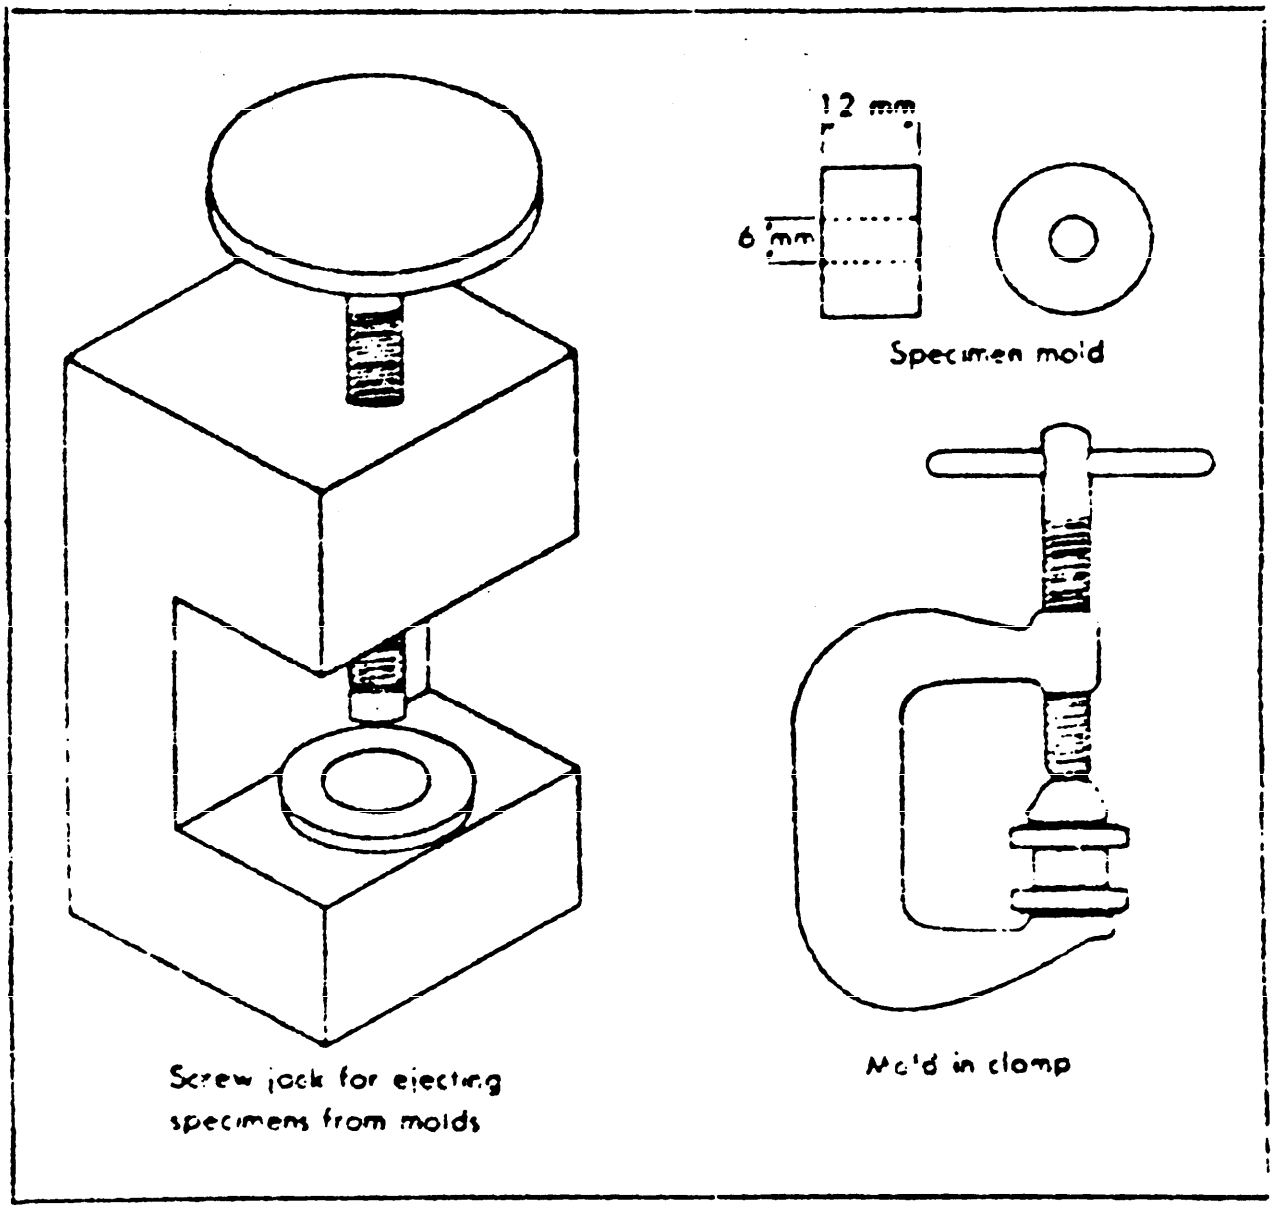


Fig. 2 Apparatus used in forming ultimate compressive strength specimens

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

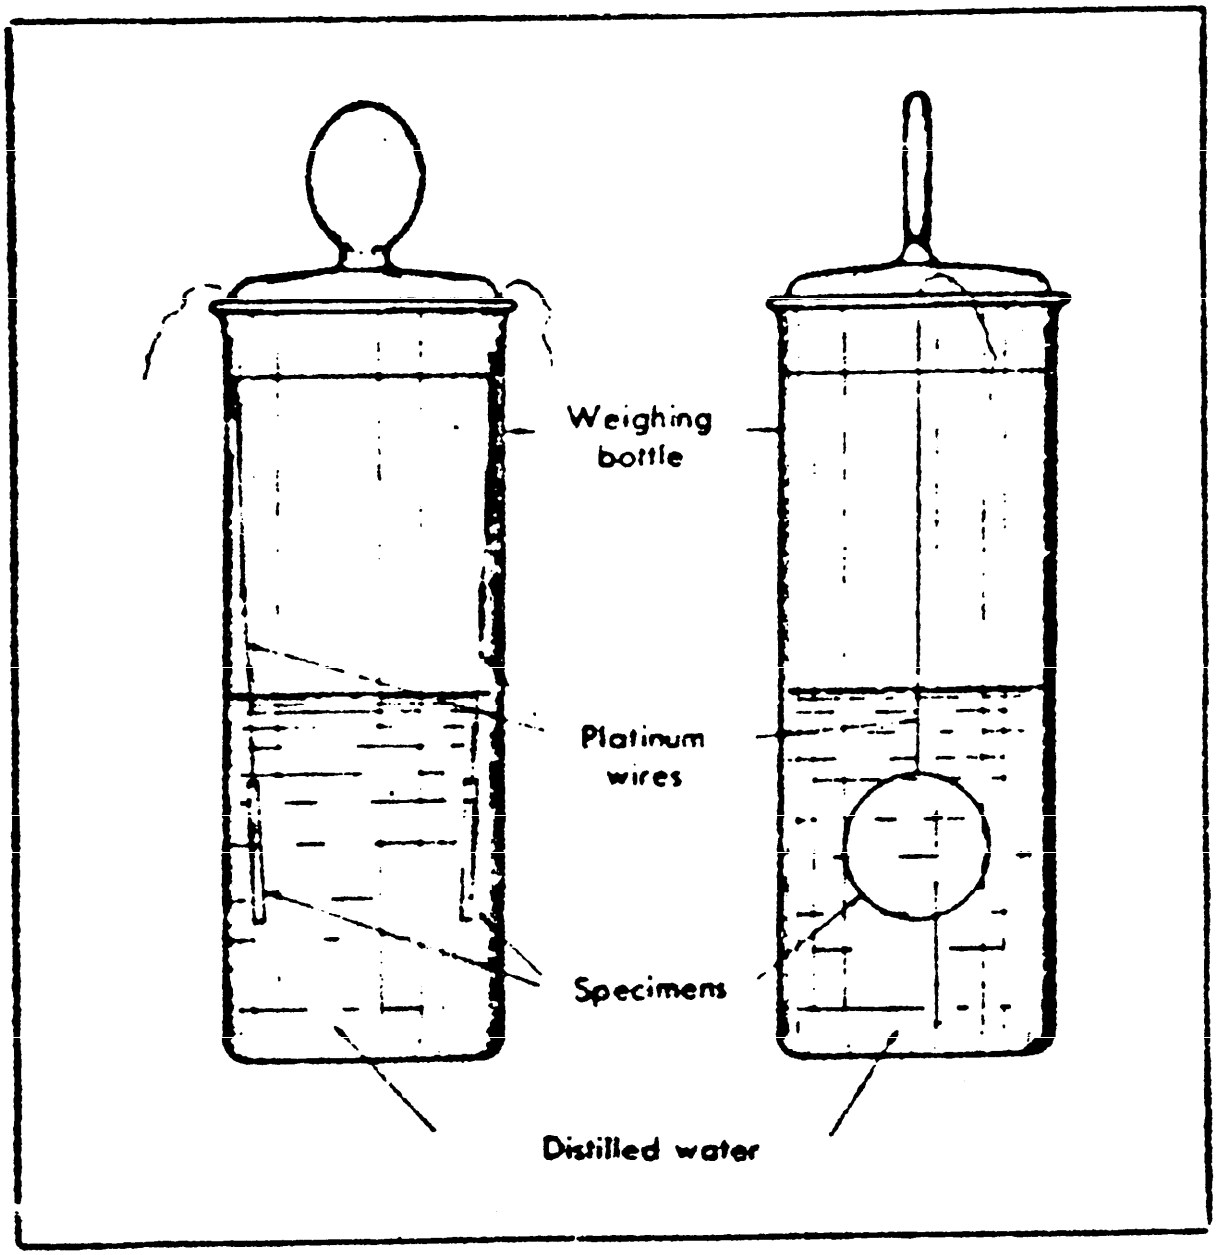


Fig. 3 Weighing bottle containing solubility specimens

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-C-36757A CEMENT, ZINC OXIDE AND EUGENOL, DENTAL (Intermediate Restorative Material)

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:16Z
Check the source to verify that this is the current version before use.