MILITARY SPECIFICATION

CANNULA, TRACHEOTOMY, NYLON

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers molded nylon tracheotomy cannulae used to provide a continuous airway when inserted in a surgical tracheotomy opening, and to maintain the opening.

1.2 Classification. The nylon tracheotomy cannula shall be of the following sizes, as specified (see 6.2):

Size 3
Size 4
Size 5
Size 6
Size 7

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive, Water Resistant (for Sealing Fiberboard Boxes).
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper, (for Carton Sealing).

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:18Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Each component of the cannula shall be molded of high quality, natural colored, hydrolysis resistant, translucent nylon.


3.2 Style, design, and dimensions. The cannula shall consist of two concentric tubes, one fitting inside the other, and an obturator for insertion into the outer tube. Each component shall be integrally molded. The outer tube shall have a neck plate which shall be elliptical in shape and be provided with two slots to accept tie tapes for securing cannula to patient. The outside diameter of the inner tube shall form a contact fit at the distal end of the outer tube, and when so fitted, shall insert without drag. The distal end of the obturator shall be rounded and shall extend beyond the distal end of the outer tube to form a pilot for the introduction of the outer tube. The obturator shall be so fitted as to insert into, and remove from, the outer tube without drag. Cannulae and obturators shall be interchangeable when tested as specified in 4.4.1. Wherever components are required to be integrally molded, they may be attached by means of ultrasonic welding. Cannula shall be in accordance with Figure 1.


3.3 Sterilization. When submitted to the sterilization test specified in 4.4.2, the cannula (including the three components) shall not become distorted, cracked, or be adversely affected so as to impair its use.


3.4 Finish. Each component of the cannula shall be smooth finished.


3.4.1 Identification marking. The tracheotomy cannula shall be permanently and legibly marked with the contractor's name or registered trademark. All component parts (i.e. outer tube, inner tube, and obturator) shall have a 3 mm. raised molded number, designating size, at proximal end of each component as shown on figure.


Source: https://assist.dla.mil -- Downloaded: 20261O-21T09:18Z
Check the source to verify that this is the current version before use.

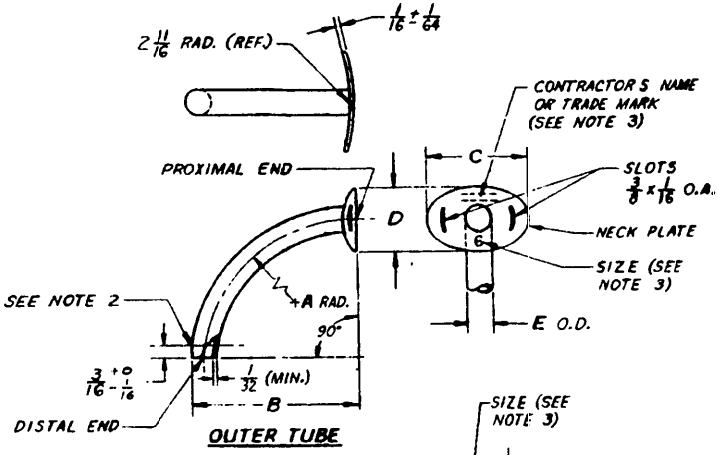


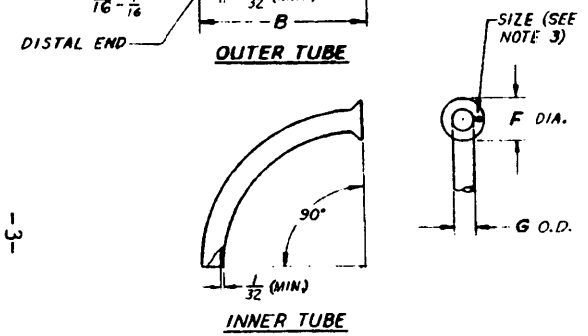

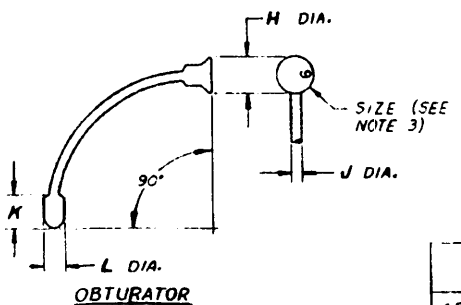


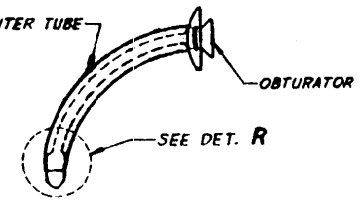

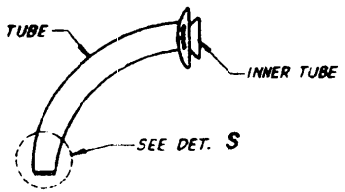

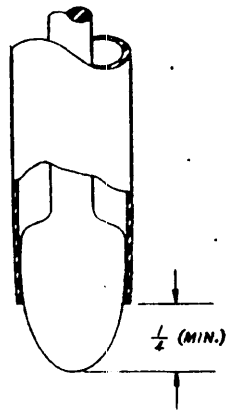

DET. R
SCALE: NONE



DET. S
SCALE: NONE

NOTE

1. ALL COMPONENTS SHALL BE INTEGRALLY MOLDED.
2. THE I.D. SHALL BE UNIFORM FROM NECK PLATE TO A POINT 3/16 +0 -1/16 INCH SHORT OF DISTAL END WHERE IT SHALL DECREASE SUFFICIENTLY TO FORM A CONTACT FIT WITH O.D. OF INNER TUBE.
3. CONTRACTOR'S NAME (OR TRADEMARK) AND SIZE SHALL BE 3MM RAISED MOLDED LETTERS (OR NUMBERS).

FSN	SIZE	DIMENSIONS										
		A (±1/16)	B (±1/16)	C	D	E	F	G (REF)	H	J (±1/64)	K	L (±1/64)
6515-663-1550	4	1 3/4	2	1 3/8	7/8	.315	9/16	1/4	1/2	5/32	1/2	1/4
6515-663-1551	5	1 7/8	2 1/16	1 7/16	29/32	.354	5/8	9/32	9/16	5/32	1/2	1/4
6515 663-1554	3	1 5/8	1 3/4	1 5/16	27/32	.236	9/16	13/64	1/2	1/8	13/32	5/16
6515 663-1561	16	2	2 3/16	1 1/2	15/16	.394	5/8	19/64	9/16	5/32	17/32	5/16
6515-913-5876	7	2 3/16	2 7/16	1 9/16	31/32	.450	11/16	23/64	9/16	5/32	5/8	3/8

FIGURE 1

MIL-C-36774

Source: https://assist.dla.mil -- Downloaded: 20260-21T09:18Z
Check the source to verify that this is the current version before use.

3.5 Workmanship. Workmanship shall be first class throughout. Cannulae shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the nylon, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection level and Acceptance Quality Level (AQL) shall be as indicated in Table I. The unit of product for examination purposes shall be one cannula.

Table I. Sampling for examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor A	II	2.5
Minor B	S-1	1.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:18Z
Check the source to verify that this is the current version before use.

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Table II. Sampling for Tests

Component	Characteristic	Reqmt.	Test procedure	Unit of product	Insp. level	AQL (percent defective)
Cannula (end item)	Sterilization test	3.3	4.4.2	1-Cannula (all 3 components)	S-2	*

*Acceptance number shall be zero for all sample sizes.

4.2.3 Raw materials. A sufficient quantity of each lot of nylon used in the construction of the cannulae shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The cannulae shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified below. Inspection, however, shall not be restricted to defects listed. Any cannulae in the sample containing one or more defects shall be rejected and if the number of defective cannulae in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

Table III. Classification of defects

Categories	Defects
Critical:	None defined.
Major	
101	Cannula not size indicated for stock number specified in contract.
102	Cannula not complete with all specified component parts.
103	Mating parts fail to fit and/or seat properly into each other.
104	Cannulae not interchangeable.
105	Edges of component parts not free from burs or sharpness.
106	Components not free from cracks and deformed areas or sections.
107	Distal ends of inner and outer tubes not smooth.
108	Obtruators not interchangeable.
109	Finish of component parts not smooth, uniform and free from roughness.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:18Z
Check the source to verify that this is the current version before use.

Table III. Classification of defects (cont'd.)

Categories	Defects
Major	
110	Labels or printed marking on unit container not correct (particularly stock number and nomenclature.)
Minor A	
201	Size markings on component parts not present or not legible.
202	Obturator stylet not uniformly curved or not free from irregular bends.
203	Labels or printed marking on unit container not legible and free from defacing marks, scratches and tears.
Minor B	
251	Dimensions not within tolerances specified on the figure.

4.4 Tests.

4.4.1 Interchangeability test. As a means to control continuity of interchangeability, 20 cannulae with stylets, randomly selected, shall be tested as follows:

Inner and outer cannulae and obturators shall be completely separated. The inner and outer cannulae shall be reassembled, making certain that no inner cannula is mated with the same outer cannula from which it had been removed. The inner cannula shall be capable of moving in and out of the outer cannula without evidence of objectionable sticking and shall seat completely in the outer cannula as indicated on the drawing. Obturators shall be inserted in outer cannulae, making certain that no obturator is mated from the same set from which it had been removed. Obturators shall fit outer cannulae as indicated on the drawing.

4.4.4 Sterilization test. All 3 components shall be subjected to autoclave sterilization for 20 minutes at 20 pounds per square inch gage steam pressure.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:18Z
Check the source to verify that this is the current version before use.

5.1.1 Unit of issue. One cannula, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be over-packed in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A. Each unit consisting of the inner and outer tubes assembled along with the obturator shall be thoroughly cleaned and packaged in a bag fabricated from polyethylene seamless tubing having an average wall thickness of not less than 0.003 inch, with no wall thickness at any point below 0.00225 inch. Excess air shall be expelled or evacuated from the bag and closure effected by heat sealing. Each bag shall be further packaged in a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:18Z
Check the source to verify that this is the currentversion before use.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to Military Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of Federal Specification PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. In addition, each unit package shall include sterilization instructions. The instructions may be printed on the polyethylene bag or on a label inserted within the bag in such a manner as to permit ready identification. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Intermediate package. Each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:18Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. The tracheotomy cannula is intended for use to provide a continuous airway when inserted in a surgical tracheotomy opening, and to maintain the opening.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) Federal stock number.

6.3 This specification is intended to cover the following items appearing in the Federal Supply Catalog:

Federal Stock No.	Item Identification
6515-663-1550	CANNULA, TRACHEOTOMY, Nylon, Size 4
6515-663-1551	CANNULA, TRACHEOTOMY, Nylon, Size 5
6515-663-1554	CANNULA, TRACHEOTOMY, Nylon, Size 3
6515-663-1561	CANNULA, TRACHEOTOMY, Nylon, Size 6
6515-913-5876	CANNULA, TRACHEOTOMY, Nylon, Size 7

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 7, dated 11 October 1968.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1587

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:18Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:18Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements .

SPECIFICATION

MIL-C-36774

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:18Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
MAR 68

EDITION AUG 66, WILL BE USED UNTIL EXHAUSTED

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:18Z
Check the source to verify that this is the current version before use.