MILITARY SPECIFICATION

FILES, PULP CANAL, DENTAL, HEDSTROM

This military specification has been prepared by the Defense Personnel Support Center (DM), based upon currently available technical information, but it has not been approved for promulgation as a coordinated revision of MIL-F-36782. It is subject to modification. However, pending its promulgation as a coordinated military specification, it may be used in acquisition.

1. SCOPE

1.1 Scope. This specification covers standardized pulp canal files of the Hedstrom design for use in endodontic procedures.

1.2 Classification. Hedstrom files shall be of the following classes and sizes as indicated:

Class I. - 21 millimeter, operative end.

Sizes

15	50
20	55
25	60
30	70
35	80
40	90
45	100

Class II. - 25 millimeter, operative end.

Sizes:

25	55
30	60
35	70
40	80
45	90
50	100

2. APPLICABLE DOCUMENTS

2.1 Government documents.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.
Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

2.1.1 Specifications and standards. Unless otherwise specified, the following specifications and standards of the issue listed in that issue of the Department of Defense Index of Specifications and Standards (DoDISS) specified in the solicitation form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-566 - Boxes, Folding, Paperboard.
PPP-B-636 - Boxes, Shipping, Fiberboard.
PPP-B-676 - Boxes, Setup.

MILITARY

MIL-P-116 - Preservation-Packaging, Methods Of.

STANDARDS

FEDERAL

FED-STD- 66 - Steel: Chemical Composition and Hardenability.
FED-STD-151 - Metals: Test Methods.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications and standards required by manufacturers in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting officer.)

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. The issues of the documents which are indicated as DoD adopted shall be the issue listed in the current DoDISS and supplement thereto if applicable.

U. S. PHARMACOPEIAL CONVENTION, INC.

The National Formulary (NF)

(Application for copies should be addressed to the Mack Publishing Company, Easton, PA 18042.)

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:19Z
Check the source to verify that this is the currentversion before use.

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence.

3. REQUIREMENTS

3.1 Materials.

3.1.1 Operative end. The operative end of the Hedstrom files shall be fabricated of AISI 302 or 304 stainless steel in accordance with Federal Standard Number 66, with a minimum tensile strength of 270,000 pounds per square inch (psi) for sizes 15 through 80 files and a minimum tensile strength of 237,000 psi for sizes 90 and 100 files, when tested as specified in 4.4.2.

3.1.2 Handle. Handle of the files shall be fabricated of plastic material which is rigid and of a quality suitable to withstand normal operative procedures. Handles shall be capable of being autoclaved or dry heat sterilized without losing the shape of the handle or leaching out of the color, when tested as specified in 4.4.6.


3.2 Style, design, and dimensions. The style, design, and dimensions of the Hedstrom files shall be of the standardized system conforming to the requirements of figure 1 and table I (dimensions), when tested as specified in section 4.4.2. The files shall be suitable for use as cutting instruments for gaining access to, clearing, enlarging, and smoothing the walls of a root canal during endodontic procedures. Hedstrom files shall be of two-piece construction, comprised of an operative end and a handle. File shall be furnished in class I, sizes 15 through 100 and class II, sizes 25 through 100, as specified (see 6.1).

3.2.1 Operative end. The operative end shall consist of a conical distal tip, a uniformly tapered spiral cutting portion, and a non-tapered round shank. Spirals forming the cutting edges shall be right hand and shall extend to the tip.

3.2.1.1 Taper. The taper of the cutting portion of the Hedstrom file shall be 0.02 mm per millimeter of cutting length when tested as specified in 4.4.2.2.

3.2.1.2 Tip. The tip length of the instrument shall be no greater than twice the diameter of D1 of the respective size number, when tested as specified in 4.4.2.3. Shape of tip is optional.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

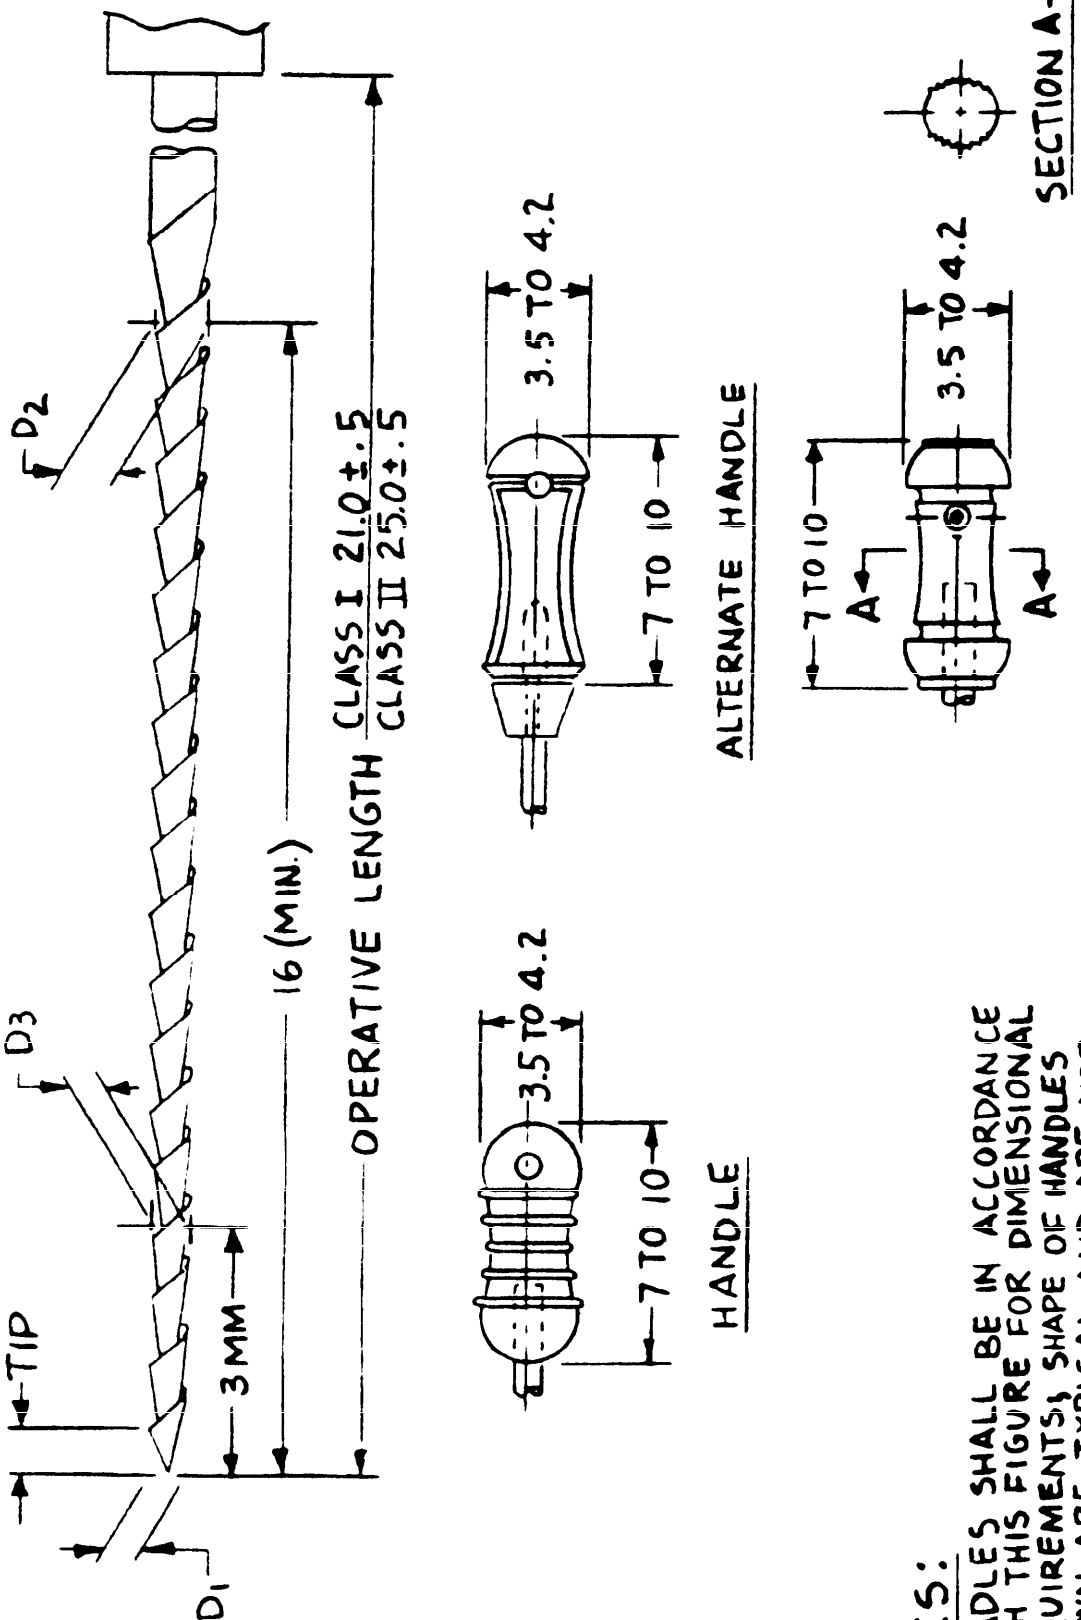

NOTES:
1. HANDLES SHALL BE IN ACCORDANCE WITH THIS FIGURE FOR DIMENSIONAL REQUIREMENTS; SHAPE OF HANDLES SHOWN ARE TYPICAL AND ARE NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF FILES WHICH ARE OTHERWISE IN ACCORDANCE WITH THIS SPECIFICATION.
2. HOLE IN HANDLE SHALL BE OPTIONAL.
3. ALL DIMENSIONS ARE IN MILLIMETERS.

FIGURE 1 - FILES, PULP CANAL, HEDSTROM

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

Table I. Dimensions.

Size	Diameter (Tolerance ± 0.02 mm) D_1 mm	D_2 mm	D_3 mm	Number of spirals ±2
15	0.15	0.47	0.21	21
20	0.20	0.52	0.26	21
25	0.25	0.57	0.31	20
30	0.30	0.62	0.36	20
35	0.35	0.67	0.41	19
40	0.40	0.72	0.46	18
45	0.45	0.77	0.51	17
50	0.50	0.82	0.56	17
55	0.55	0.87	0.61	17
60	0.60	0.92	0.66	16
70	0.70	1.02	0.76	16
80	0.80	1.12	0.86	15
90	0.90	1.22	0.96	14
100	1.00	1.32	1.06	14

3.2.1.3 Handles. Operative ends of files shall be securely and permanently affixed in the handles with no movement of operative end within the handles permitted. Color shall be incorporated in the plastic composition.

3.2.3 Figures. The figures forming a part of this specification are specification control figures. The supplier shall be responsible for preparing his own shop drawings. Where tolerances prescribed could cumulatively result in improper design, the supplier shall provide a product with dimensions within the tolerances prescribed on the drawing to insure proper design, function, fit, assembly, and operation of the item. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer.

3.3 Resistance to fracture by twisting. The torsional load or torque at various angular deflection for each instrument shall not be less than that given in Table II for each size when tested as specified in 4.4.3.

3.4 Stiffness. The stiffness of all instruments shall not be greater than that given in Table III for each size when tested as specified in 4.4.4.

3.5 Corrosion resistance. The operative ends of the files shall not show evidence of corrosion of their surface when subjected to the corrosion tests as specified in 4.4.5.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

3.6 Finish. Spiral section of operative ends of the files shall have a bright and smooth finish. Handles shall be longitudinally serrated or shall have crosscut serrations. The entire handle may be serrated or only the finger-gripping portion need be serrated. Handles shall be suitable for proper finger gripping. Entire instrument shall be free from laminations, cracks, gouges, chips, or broken areas.

3.7 Identification marking. Handles shall be color coded and numbered with respective size for identification of instrument as specified in table IV.

3.8 Workmanship. The files shall be free from defects which may detract from their appearance or impair their serviceability.

Table II.

Torque and Angular Deflection (Minimum Values) Twisted in Clockwise Rotation.

Size	Torque (gm. cm.)	Angular Deflection (Degrees)
15	8.0	180
20	12.0	180
25	20.0	180
30	35.0	180
35	50.0	180
40	65.0	120
45	90.0	120
50	120.0	120
55	160.0	90
60	250.0	90
70	350.0	90

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:19Z
Check the source to verify that this is the current version before use.

Table III. Stiffness (Bending Moment) Maximum Values at 45° Bend.

Size	Bending Torque (gm. cm.)
15	35.0
20	65.0
25	100.0
30	135.0
35	170.0
40	220.0
45	320.0
50	520.0
55	720.0
60	920.0
70	1120.0

Table IV. Color Coding

Size	Color	Abbreviation
15	White	Wh
20	Yellow	Yel
25	Red	Red
30	Blue	Blu
35	Green	Grn
40	Black	Blk
45	White	Wh
50	Yellow	Yel
55	Red	Red
60	Blue	Blu
70	Green	Grn
80	Black	Blk
90	White	Wh
100	Yellow	Yel

4. QUALITY ASSURANCE PROVISIONS.

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables II, III, and IV (see 4.2.1, 4.2.2 and 4.3) and 4.3.1.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality lvels (AQLs) shall be as indicated in table V. Unit of product for examination purposes shall be the unit of issue (6 files).

TABLE V. Sampling for examination.

Type defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-2	1.5
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table VI. Unit of product for test purposes shall be as indicated in table VI.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

TABLE VI. Sampling for tests.

Component	Characteristic	Requirement	Test procedure	Unit of product	Inspection level	AQL (percent defective)
Operative ends	Tensile strength	3.1.1	4.4.2	Lot of steel stock	*	---
	Resist. to frac. by twisting	3.3	4.4.3	one file	S-2	**
	Stiffness test	3.4	4.4.4	one file	S-2	**
Entire Instrument	Corrosion resistance	3.4	4.4.5	one file	S-2	**
Handles	Sterilization	3.1.2	4.4.6	one file	***	**

*Average of a minimum of three specimens from each lot of steel stock.
**Acceptance number shall be zero for all sample sizes.
***Separate S-2 level quantities for both autoclave and dry heat tests.

4.2.3 Raw materials. Sufficient material from each lot of metal used in the construction of the files shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where feasible, the same sample unit shall be tested for the determination of two or more test characteristics.

4.3 Examination. The files shall be examined for defects including, but not limited to, those listed in table VII.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

TABLE VII. Classification of defects.

Categories	Defects
Major A:	
101	Class and size not as specified.
102	Style and design not as specified.
103	Handles not properly color coded.
104	Operative ends do not have a bright smooth finish.
105	Cutting edges not sharp.
106	Operative ends not firmly affixed in the handles.
107	Laminations or cracks present.
108	Operative end bent, deformed, or otherwise damaged.
Major B:	
151	Number of spirals not as indicated for size number.
152	Dimensions of operative end not as specified.
Minor A:	
201	Finish of handles not as specified.
202	Color coding and size number marking not present on handle or incorrect.
Minor B:	
251	Dimensions of handles not as specified.

4.3.1 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests.

4.4.1 Chemical analysis and tensile strength of the metals. In the absence of certificates of quality for the raw material, the samples selected in accordance with 4.2.3 shall be analyzed in conformance with methods 111 or 112 of Federal Test Method Number 151. In case of dispute, method 111 shall be used for referee analysis. Tensile strength shall be performed in a tension tester on an 8-inch sample of steel stock used to produce the files.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

4.4.2 Equipment. The diameter and tip length of an instrument shall be measured using a shadowgraph, measuring microscope, or other suitable device capable of measuring the diameter and length with the accuracy specified in 3.2.1.2 and Table I.

4.4.2.1 Diameters. A Hedstrom file to be measured shall be inserted into a shadowgraph, measuring microscope, or other suitable device and the diameters D_1 and D_2 shall be measured. As an alternate to measuring the D_1 diameter, the D_3 diameter may be measured at a location 3 mm from the tip point.

4.4.2.2 Taper. A Hedstrom file to be measured shall have its diameter determined at 1 mm increments along the cutting section beginning 1 mm from the tip point up to 6 mm from the tip point.

4.4.2.3 Tip. The tip length of the instrument shall be determined by a suitable measuring device.

4.4.3 Resistance to fracture by twisting. Samples of a given size shall be tested for resistance to fracture by twisting as follows:

4.4.3.1 Equipment. The testing equipment shall be capable of measuring torque with an accuracy of ± 1 gm. cm. and angular deflection with an accuracy of ± 2°. The equipment described below shall be used for compliance testing and is presented as the preferred type of equipment for all purposes. The equipment as shown in Figure 2 shall consist of: a reversible geared motor revolving at a speed of 2 RPM which drives a test instrument by means of a separate hardened steel chuck; a torque measuring device fixed on two linear ball bearings, mounted to the shaft of the device is the chuck with jaws made of brass (70% copper-35% zinc) used to clamp the test instrument at the tip along a length of 3 mm. See Figure 3. A separate amplifier and digital display controls the operation of the motor and records the torque and angular deflection. The circuitry of the amplifier should include the feature of retaining for display the maximum torque 1 mm from the tip point up to 6 mm from the tip point.

4.4.3.2 Procedure for twist test. Calibrate the device for the torque range of the test instrument size to be tested. The Hedstrom file to be tested shall have its handle removed with a suitable wire cutter at the point at which the handle is attached to the instrument shaft. Set the test instrument shank into the driving chuck leaving a maximum of 1 mm of the unground portion of the shank out of the chuck. Tighten the chuck. Slowly slide the torque device along the linear ball bearing until the tip of the test instrument enters 3 mm into the brass jaws. Check to assure that the test instrument is straight and centered into the jaws. Tighten the chuck. Since clamping will probably induce a pre-stress of the test instrument, the gear motor must be activated in steps until the torque digital display or the strip chart recorder shows a zero reading. After insuring that the geared motor is set for clockwise rotation as viewed from the test instrument shank end, activate the device. The test device will cease operation when the test instrument fails. The maximum torque and angular deflection shall be recorded for each Hedstrom file tested.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

4.4.4 Stiffness. Samples of a given size shall be tested for stiffness as follows:

4.4.4.1 Equipment. The equipment as described in 4.3.3.1 shall be used with the modification of the clamping jaws and the bending device or catch pin as shown in Figure 4. The amplifier of the device must be capable of obtaining a pre-selected angular deflection (45°) at which point the test stops. The testing equipment shall be capable of measuring torque with an accuracy of $\pm$ 1 gm. cm.

4.4.4.2 Procedure for stiffness test. Calibrate the device for the torque range of the test instrument size to be tested. The Hedstrom file to be tested shall have its handle removed with a suitable wire cutter at the point where the handle is attached to the instrument shaft. Set the device to stop the angular deflection at 45°. Place the chuck onto the shaft of the torque meter device. Set the tip of the test instrument into the jaws of the chuck perpendicular to the axis of the motor. When the tip enters 3 mm into the brass jaws, tighten the chuck. Mount the catch pin onto the gear motor shaft. Slide the torque device along the linear ball bearing until the test instrument is located above the rotating pin. By rotating the gear motor in the proper direction in steps, adjust the catch pin until it is lightly touching the test instrument. The torque reading must show zero. Activate the test device. The test will automatically cease when the angular deflection has reached 45°. The torque at 45° shall be recorded for each Hedstrom file tested.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

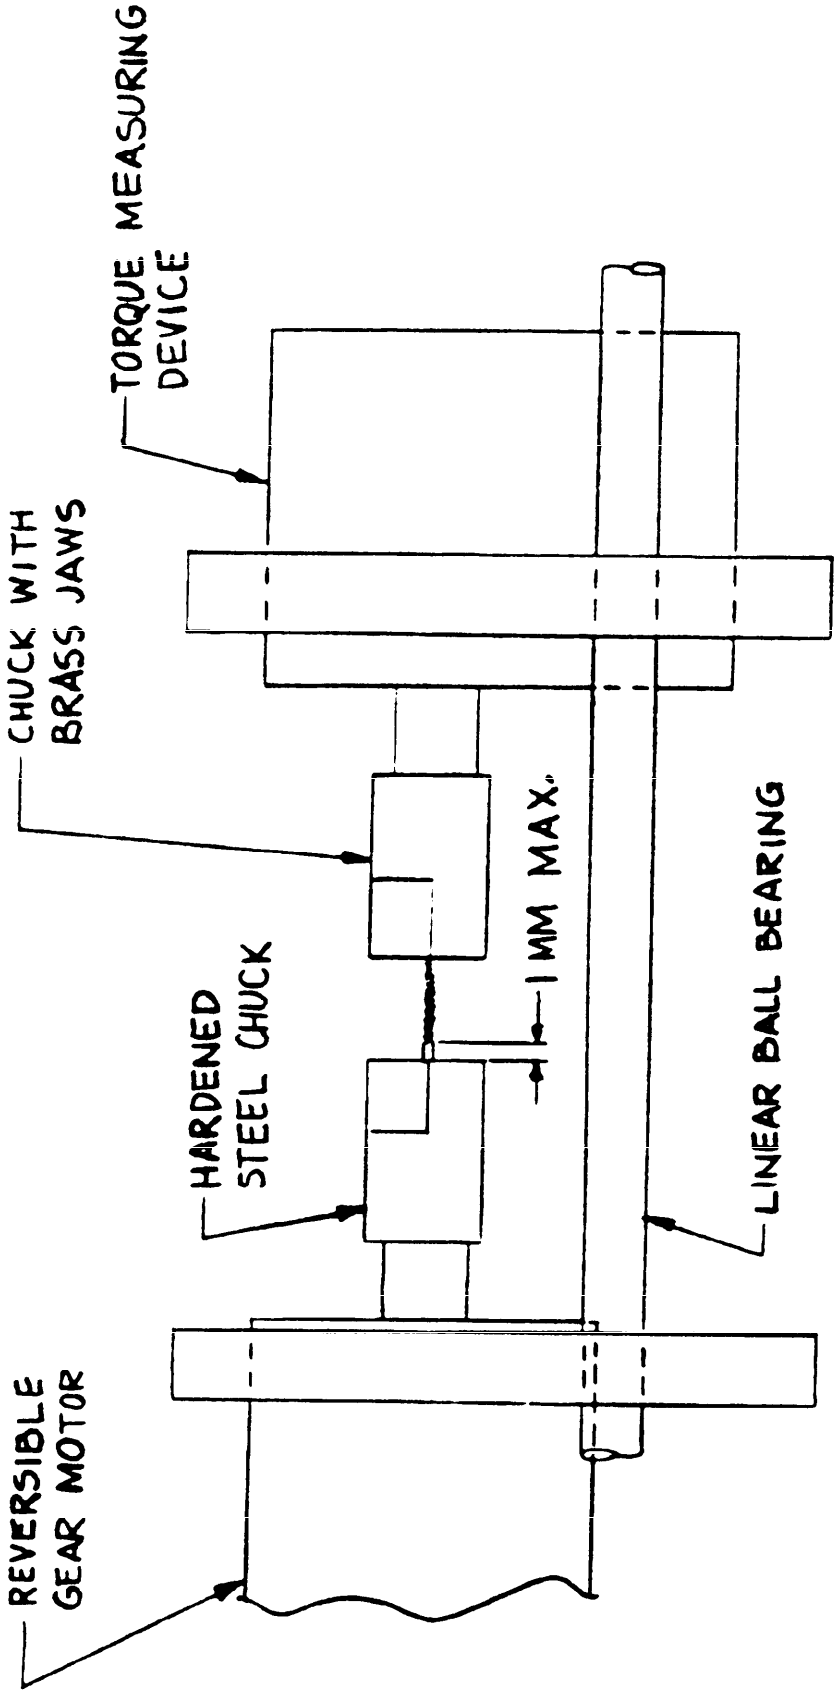


FIG. 2 - TEST EQUIPMENT FOR TORQUE TESTING

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

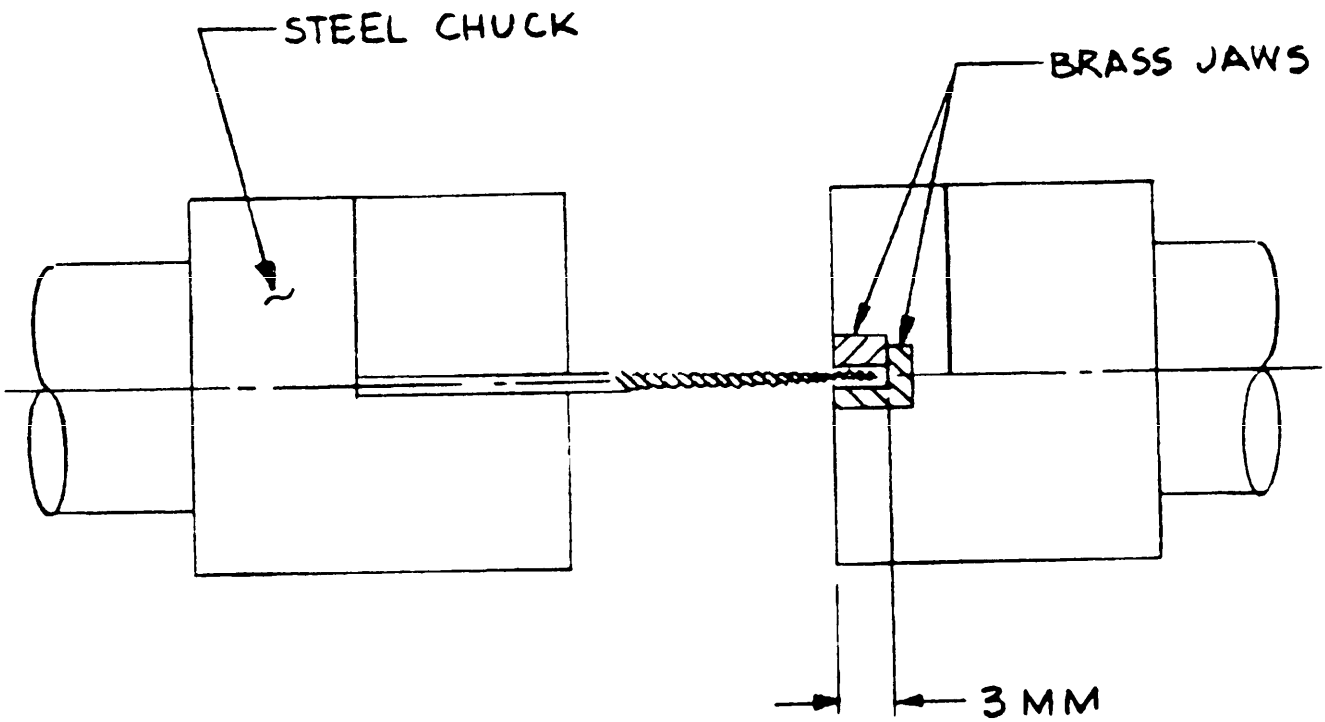


FIG. 3 - TWIST TEST CHUCK DETAIL

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

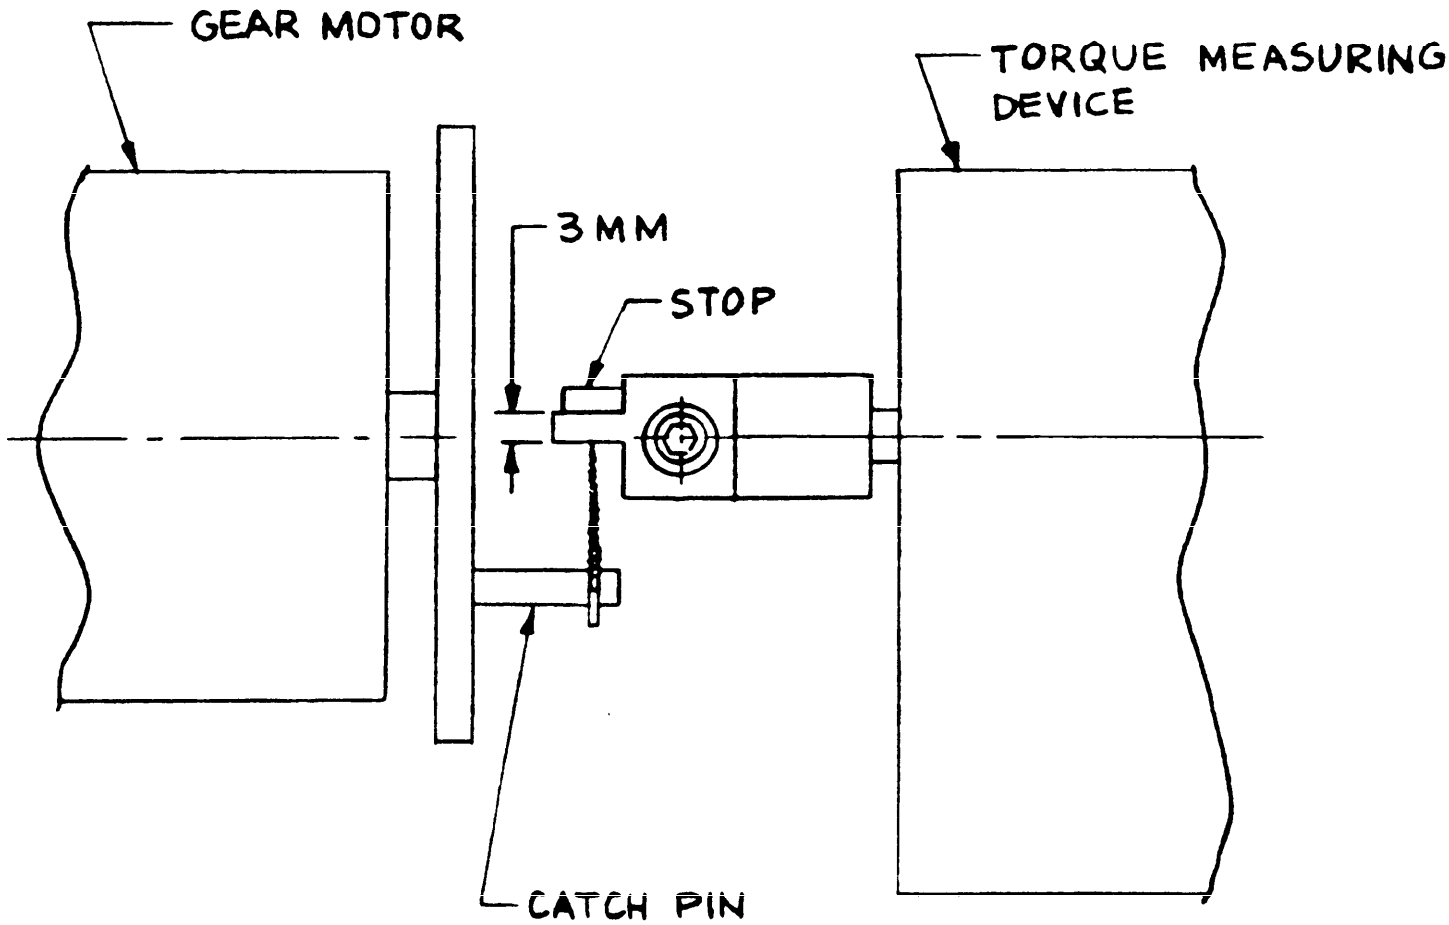


FIG. 4 - STIFFNESS TEST

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

4.4.5 Corrosion test. Files shall be tested for corrosion resistance by one of the following procedures:

4.4.5.1 Sample and preparation. Files of each size shall be scrubbed with soap and water, rinsed in hot water, followed by a dip in ethyl alcohol (95%), or isopropyl alcohol (isopropanol; 2-propanol) National Formulary (NF) and dried at room temperature.

4.4.5.2 Copper sulfate test. A copper sulfate solution is made up as follows: Copper sulfate ($CuSO_4$, 5 H_2O) 4.0 g, Sulfuric acid (H_2SO_4, specific gravity 1.84) 10.0 g, and Water (H_2O) 90.0 milliliters (ml). The instruments selected and prepared shall be immersed in the copper sulfate solution at a temperature of 65° Fahrenheit (F) for 6 minutes and then wiped off with a cloth saturated with fresh water. The instrument shall then be examined under a magnification of at least 5X for the presence of brown stains indicating corrosion.

4.4.5.3 Agar Ion test. An agar ion gel is made up as follows: Potassium ferricyanide ($K_3Fe(CN)_6$) 0.2 g, Sodium chloride (NaCl) 1.0 g, Water (H_2O) 100 ml, Agar-agar 1.5 g. The agar solution shall be poured into a transparent container. The instruments selected and prepared are inserted into the gel (37° ± 2° Celsius (C)) at intervals of not less than 10 mm and at a distance of 10 mm from the periphery of the container. The instruments are inserted to a depth of approximately 20 mm. Visual examination of the instruments while in the gel shall be made for the presence of blue precipitates on the instrument, indicating corrosion.

4.4.6 Sterilization tests. The finished Hedstrom files shall be autoclaved under 27 ± 3 pounds of pressure at 132 ± 5°C (270 ± 9°F) for twenty (20) minutes and dry heat sterilized at 160 ± 5°C (320 ± 9°F) for one hundred and twenty (120) minutes. The handles of the files shall then be examined for compliance with specification requirements.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.1).

5.1.1 Unit of issue. One package containing six files of one class and size, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit packaging. Six files of one class and size shall be packaged in a plastic tray having a clear, slip-over cover or a hinged cover. The tray shall be designed with six cavities or inserts to hold each file in a manner to prevent movement and damage to the operative end. The cover shall be secured with a strip of pressure-sensitive tape. Each plastic container shall be further packaged in a bag as specified in MIL-P-116, method IC-1.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:19Z
Check the source to verify that this is the current version before use.

5.1.2.2 Intermediate package. Twenty-four unit packages containing files of one class and size only shall be packaged in a box constructed in accordance with PPP-B-566 or PPP-B-676. Closure shall be in accordance with the appendix of the applicable box specification.

5.1.3 Level C. Files shall be clean, dry, and packaged in a manner that will afford adequate protection against corrosion, deterioration, and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B, or C, as specified (see 6.1).

5.2.1 Level A. Twenty-four intermediate packages (576 units) containing files of one class and size only shall be packed in a shipping container designed for a type 2 load and constructed in accordance with PPP-B-636, class weather-resistant. Closure, strapping, and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Twenty-four intermediate packages (576 units) containing files of one class and size only shall be packed in a shipping container designed for a type 2 load and constructed in accordance with PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The packaged files shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the carrier's rules and regulations.

5.3 Marking. Each unit package, intermediate package, and shipping container shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Ordering data.

6.1.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number, and date of this specification.
b. Class and size required (see 1.2).
c. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Specification changes. Because of the extensiveness of changes to this document, the margins have not been marked with an asterisk to indicate where changes from the previous issue have been made.

6.3 National Stock Number (NSN) coverage. This specification covers the following items listed in the Federal Supply Catalog:

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

NSN	Item Identification
	FILE, PULP CANAL, DENTAL, 21 MM END LENGTH
6520-00-935-4145	Hedstrom, Standardized, Size 15, 6s
6520-00-935-4146	Hedstrom, Standardized, Size 20, 6s
6520-00-935-4147	Hedstrom, Standardized, Size 25, 6s
6520-00-935-4148	Hedstrom, Standardized, Size 30, 6s
6520-00-935-4149	Hedstrom, Standardized, Size 35, 6s
6520-00-935-4150	Hedstrom, Standardized, Size 40, 6s
6520-00-935-4151	Hedstrom, Standardized, Size 45, 6s
6520-00-935-4152	Hedstrom, Standardized, Size 50, 6s
6520-00-935-4153	Hedstrom, Standardized, Size 55, 6s
6520-00-935-4154	Hedstrom, Standardized, Size 60, 6s
6520-00-935-4155	Hedstrom, Standardized, Size 70, 6s
6520-00-935-4156	Hedstrom, Standardized, Size 80, 6s
6520-00-935-4157	Hedstrom, Standardized, Size 90, 6s
6520-00-935-4158	Hedstrom, Standardized, Size 100, 6s
	FILE, PULP CANAL, DENTAL, 25 MM END LENGTH
6520-00-935-4162	Hedstrom, Standardized, Size 25, 6s
6520-00-935-4163	Hedstrom, Standardized, Size 30, 6s
6520-00-935-4164	Hedstrom, Standardized, Size 35, 6s
6520-00-935-4165	Hedstrom, Standardized, Size 40, 6s
6520-00-935-4166	Hedstrom, Standardized, Size 45, 6s
6520-00-935-4167	Hedstrom, Standardized, Size 50, 6s
6520-00-935-4168	Hedstrom, Standardized, Size 55, 6s

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:19Z
Check the source to verify that this is the current version before use.

6520-00-935-4169	Hedstrom, Standardized, Size 60, 6s
6520-00-935-4170	Hedstrom, Standardized, Size 70, 6s
6520-00-935-4171	Hedstrom, Standardized, Size 80, 6s
6520-00-935-4172	Hedstrom, Standardized, Size 90, 6s
6520-00-935-4173	Hedstrom, Standardized, Size 100, 6s

Military Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DLA-DM

Project No. 6520-1790

Review activity:
DoD-MB

Location S1-2-37-A

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426

PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:19Z
Check the source to verify that this is the current version before use.