MIL-F-36766
27 April 1971

MILITARY SPECIFICATION

FORCEPS, HEMOSTATIC CLIP, APPLYING, LeROY-RANEY

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of hemostatic scalp clip applying forceps suitable for use with plastic LeRoy-Raney scalp clips in surgical procedures.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-up.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The forceps shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The forceps shall be fabricated from Class 5, Type 17-4 PH material.

3.3 Hardness. After proper stress relieving, the Rockwell hardness of the forceps shall be C39 to C44.

3.4 Style, design, and dimensions. Shall be a LeRoy-Raney hemostatic scalp clip applying forceps and shall be of the box lock type in accordance with GG-I-526. The forceps shall be suitable for use with FSN 6515-181-8011 CLIP, HEMOSTATIC, LeRoy-Raney, Disposable, Plastic. The style, design, and dimensions of the forceps shall conform to Figure 1.


3.5 Finish. Shall be satin finish.

3.6 Identification marking. In addition to GG-I-526 requirements, forceps of foreign manufacture shall be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specifications where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:17Z
Check the source to verify that this is the current version before use.

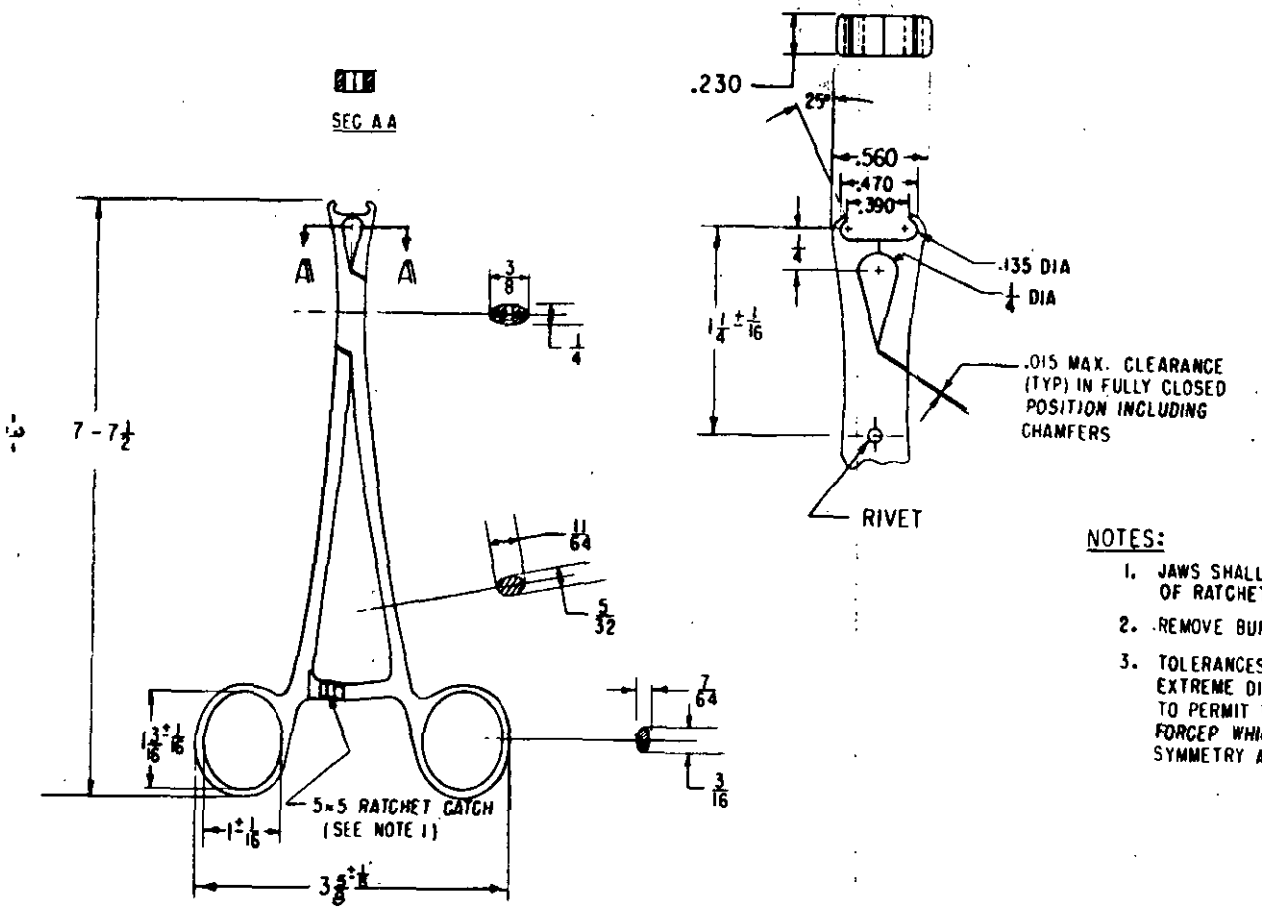

NOTES:

1. JAWS SHALL CLOSE AT FIRST NOTCH OF RATCHET.
2. REMOVE BURRS AND BREAK SHARP EDGES.
3. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE FORCEP WHICH WILL SACRIFICE UNIFORMITY SYMMETRY AND FIRST QUALITY WORKMANSHIP.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Shall be in accordance with GG-I-526.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one forceps.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accorance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.

Table II. Sampling for Tests

Component (unit of product	Characteristic	Require-ment	Test procedure	Inspection level	AQL (percent defective)
1-Forceps	Composition analysis	3.2 and GG-I-526	GG-I-526	**	*
1-Forceps	Hardness	3.3 and GG-I-526	GG-I-526	S-2	*
1-Forceps	Dimensions	3.4	- - -	S-3	*
1-Forceps	Boil test	GG-I-526	GG-I-526	S-2	*
1-Forceps	Distortion	GG-I-526	GG-I-526	S-3	*
1-Forceps	Lock stiffness	GG-I-526	GG-I-526	S-3	2.5

* Acceptance number shall be zero for all sample sizes.

** Sufficient amount from each lot of metal used in the construction of the forceps shall be selected for composition analysis.

4.3 Examination. The forceps shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include, but shall not be limited to, the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Forceps not free from sharp edges, rough areas, burs, cracks, tool marks or pits.
103	Jaws do not close at first notch of ratchet.
104	Locks not accurately fitted or pins not permanently secured.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:17Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects (Cont'd)

Minor	
201	Finish not as specified.
202	Identification marking not present, correct, complete, or legible.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements in accordance with GG-I-526.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One forceps, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	144 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive materials.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IA-8.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to Military Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of Federal Specification PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:17Z
Check the source to verify that this is the current version before use.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The hemostatic clip forceps shall be suitable for use with the LeRoy-Raney plastic scalp clip (see 3.4) for craniotomy procedures, laminectomies, hip surgery, and surgery of the extremities.

6.2 Ordering data. Procurement documents should specifiy the following:

1. Number, title, and date of this specification.
2. Applicable levels of packaging and packing (see 5.1 and 5.2).
3. Federal stock number.

6.3 This specification is intended to cover Federal Stock Number 6515-421-7829 FORCEPS, HEMOSTATIC, CLIP, Applying, LeRoy-Raney, appearing in the Federal Supply Catalog. It does not include all types as indicated by the title nor all types commercially available.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1580

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. *Fold on lines on reverse side, staple in corner, and send to* preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION
MIL-F-36766

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:17Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:17Z
Check the source to verify that this is the current version before use.