A-A-53785
1 February 1989

COMMERCIAL ITEM DESCRIPTION

PLACEMENT KIT, TOOTH DIE PIN

The General Services Administration has authorized the use of this Commercial Item Description in preference to Military Specification MIL-T-36820.

Salient characteristics:

This commercial item description covers a tooth die pin placement kit suitable for use in the placement and positioning of dowel pins in dental elastic impression material during pouring of the stone cast.

Material.

Harness and cap. The harness and cap shall be fabricated of a dark colored vinyl composition.

T-Pin. The T-pins shall be fabricated of nickel-plated steel.


Style, design and dimensions. Tooth die pin placement kit shall consist of the following items:

a) Fifty (50) T-pins (minimum)
b) Fifty (50) elastomeric harness strips with integrated caps (minimum)
c) Plastic immediate container

The kit shall be suitable for use in the placement and positioning of the dowel pins in various types of dental elastic impression material during pouring of the stone cast. All items in the kit shall conform to Figures 1 and 2 for style, design and dimensions.

AMSC N/A FSC 6520
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.


Source: https://assist.dla.mil -- Downloaded: 202610-26T09:24Z
Check the source to verify that this is the current version before use.

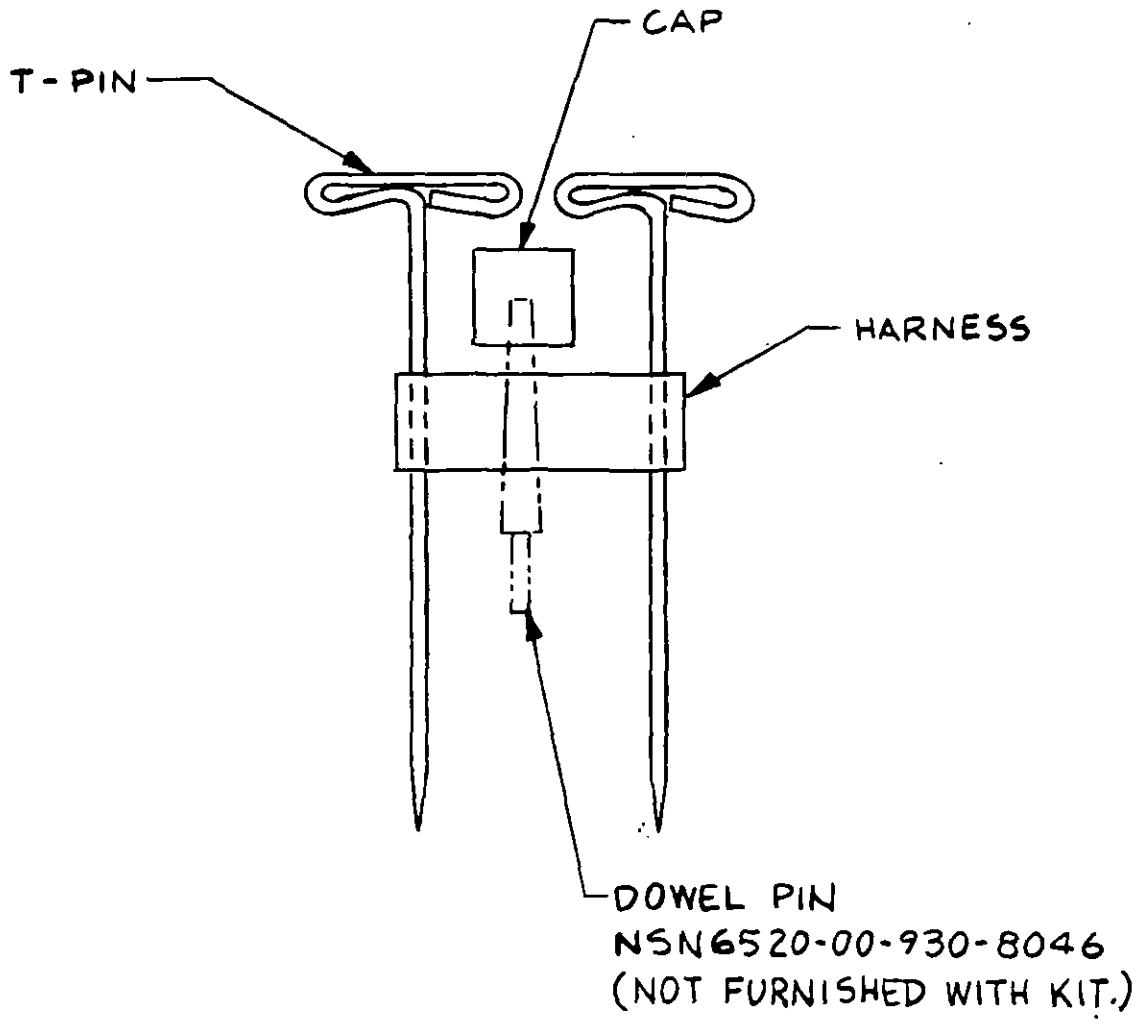


ASSEMBLY

FIGURE 1 TOOTH DIE PIN PLACEMENT KIT


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:24Z
Check the source to verify that this is the current version before use.

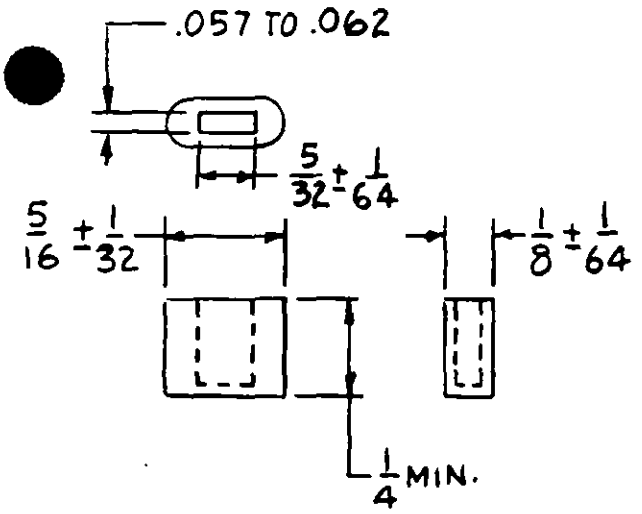

CAP

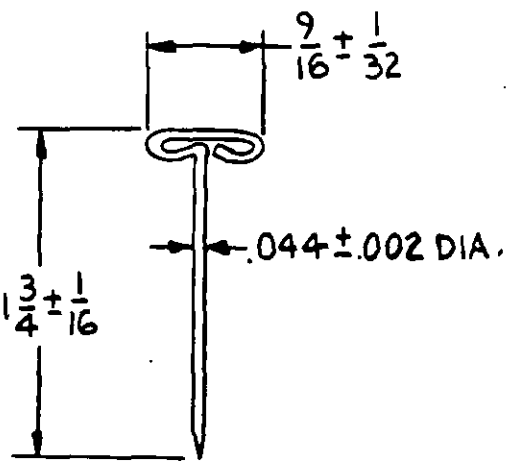

T-PIN

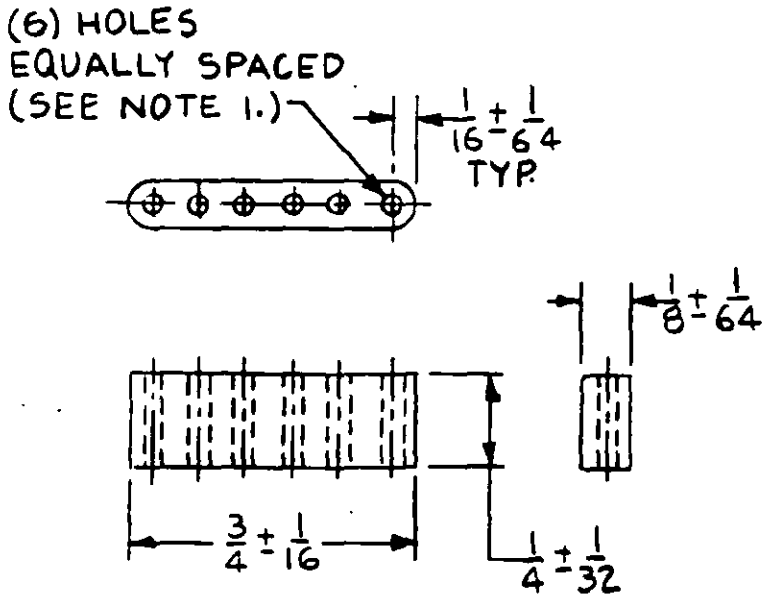

HARNESS

NOTES:

1. INSIDE DIAMETER OF HARNESS TUBES SHOULD BE LESS THAN .042 INCH TO INSURE THAT THE T-PIN WILL FIT SNUGLY IN IT.
2. ALL DIMENSIONS ARE IN INCHES.

FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:24Z
Check the source to verify that this is the current version before use.

T-pin. The T-pin shall be a straight steel pin with a crossbar used to position the harness over the proper area of impression material.

Harness and caps. The harness shall consist of 6 hollow tubes. The cap shall be attached to the harness and shall be easily detachable from the harness. The diameter of the tubes shall be such that each tube shall accommodate the tapered end of the dowel pin. The cap shall be designed to fit onto the non-serrated end of the pin. The cap shall function as a marker for locating the end of the dowel pin in dental stone.

Finish.

Pins. Nickel-plated steel for pins shall have a bright, smooth finish, free of cracks, breaks or burrs.

Harness and cap. The harness and cap shall have a smooth finish and shall be free of tears, cracks or breaks.

Instruction. Instructions for use shall accompany each kit.

Immediate container. The kit, consisting of a minimum of 50 T-pin and 50 harnesses with caps shall be furnished in a suitable, sturdy, plastic compartmented box, having 4 compartments; 3 compartments for the above-mentioned items in the kit, and the fourth compartment as a convenience to hold the dowel pins to be used in this technique.

Workmanship. Tooth die pin placement kit shall be free from defects which may detract from its appearance or its impair function or intended use.

Unit. Each (EA). One placement kit complete with directions for use, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:24Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one kit. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, except for dimensions which shall be conducted at inspection level S-1, AQL 4.0 (percent defective). Sampling for tests (when applicable) shall be conducted at inspection level S-1. For tests, acceptance number shall be zero (0) for all sample sizes.

Examination. Examination shall include but shall not be limited to the following:

Defects.

Cracks, breaks, or burrs present in T-pins.
Cracks, breaks, or tears present in dowel cap or harness.
T-pin does not have a bright smooth surface.
Cap and harness do not have a smooth surface.
Inside diameter of hole in harness not as specified on figure. 1/ 3/
Diameter of hole in cap not as specified. 2/ 3/
Wall thickness of cap not as specified. 3/
Number of tubular elements in harness not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:24Z
Check the source to verify that this is the current version before use.

Defects (continued).

Immediate container not compartmentalized as specified herein.
Dimensions (other than above) not as specified.
Quantity not as specified.

1/ A suitable gage may be used, such as an 0.036 inch T-pin.
2/ A suitable gage may be used, such as a 1.2 mm dowel pin.
3/ Except AQL 1.0 (% defective).

Tests.

Bond strength of harness tubes. A T-pin shall be placed in each of the extreme end cylinders (tubes) of the harness. An 8-oz. load shall be securely attached with a strong thread or string to each end of one pin. The assembly shall then be suspended by holding the free ends of the unloaded pin by hand or in a jig to permit the harness and loaded pin to swing down around the held secured T-pin as a hinge. After 3 minutes under load, the harness shall be examined for breaks or ruptures in the bond between the cylinders.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:24Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

National Stock Number	Item Identification
6520-00-153-8472	PLACEMENT KIT, TOOTH DIE PIN

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:24Z
Check the source to verify that this is the current version before use.

A-A-53785

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

PROJECT NO. 6520-2076

LOCATION: NCR Disk No. 7

47464

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:24Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53785	PLACEMENT KIT, TOOTH DIE PIN

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION (YYMMDD)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:24Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C.

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:24Z
Check the source to verify that this is the current version before use.