

FED. SUP CLASS
6640



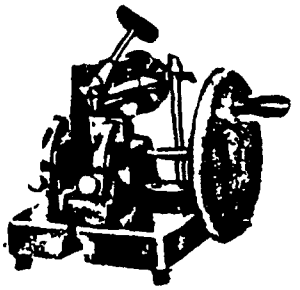

MS36322-1						MS36322-2	
PART NUMBER	DIMENSIONAL DATA in. (mm)						
	LENGTH		WIDTH		HEIGHT		
MS36322-1	15.5	(394)	13.5	(343)	8.75	(222)	
MS36322-2	10	(254)	12	(305)	11	(279)	

MATERIAL: MS36322-1 base shall be cast iron. Cover shall be cast iron or aluminum. All other parts shall be fine grained tool steel in accordance with commercial practice.

MS36322-2 shall be of corrosion-resisting steel in accordance with Federal Specification QQ-S-766 or of nickel-plated bronze in accordance with commercial practice.

FINISH: Cover of MS36322-1 shall be gray epoxy resin.

DESIGN: MS36322-1 shall have a horizontal feed mechanism entirely independent of the vertical movement of the object block. Ratchet wheel rotates a feed screw which advances the cone a measured distance from left to right. Crank at the left of microtome engages the feed screw when the hinged cover is down. Feed indicator is graduated in feed settings from 1 to 50 micrometers in 1 micrometer increments. Lever locks the counterbalanced drive wheel securely which stops the object block at the top of its excursion. A base rigidly supports the mechanism and knife holder and a protective cover, hinged to the base, swings back to completely expose all the interior parts. MS36322-1 shall be furnished with two 120 millimeter microtome knives, a knife handle and back for sharpening, three object disks, one safety razor blade holder, three packages of extra heavy steel single-edge razor blades (10 each), and one can of at least 3 ounces of pike oil.

MS36322-2 shall have a microtome knife rigidly held in the straight edge jaws of a knife holder by tightening two large thumb screws. Lock nuts on two adjusting screws shall maintain the knife angle setting. Ball and socket clamp screw rigidly fixes the specimen holder in place. A micrometer screw feed mechanism provides direct and accurate method of advancing the specimen to the knife. Specimen holder makes one cutting path by the knife for each revolution of the balanced drive wheel. A locking pin on the handwheel holds specimen holder to allow for insertion and adjustment of the specimen. Sections are produced by setting the interchangeable index post from 2 to 16 micrometers in 2 micrometer increments, or 18 to 42 micrometers in 2 micrometer increments. MS36322-2 shall be furnished with one detachable specimen holder, one ball plate specimen holder, one safety razor blade holder with screwdriver and ten blades packed in leather bound box, and one 0.75 ounce bottle of oil.

NOTES:
1. Procurement document for MS36322-1 is Military Specification MIL-M-36314.
2. For knife, microtome used with MS36322-1 see MS36323-2.
3. For object, disk, microtome for MS36322-1 see MS36324-1, -2, and -3.
4. For object, disk, microtome for MS36322-2 see MS36324-4.
5. For holder, safety razor blade, microtome see MS36327-1.
6. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements as specified herein.
7. In the event of a conflict between the text of this standard and the references cited herein, the text of this standard shall take precedence.
8. Referenced Government documents of the issue listed in that issue of the Department of Defense Index of Specifications and Standards (DoDISS) specified in the solicitation form a part of this standard to the extent specified herein.

Ⓑ ENTIRE STANDARD REVISED

P.A.	EA	INTERNATIONAL INTEREST	TITLE
Other Cust	MS 99		MICROTOME, rotary type

PROCUREMENT SPECIFICATION: SEE NOTE 1 | SUPERSEDES:

MILITARY STANDARD
MS 36322
SHEET 1 OF 1

DD FORM 672-1 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1520-01

AMSC N/A
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

DATE
DRAWN BY

Source: https://assist.dla.mil. Downloaded: 2026-10-23T17:19Z
Check the source to verify that this is the current version before use.

USER ACTIVITIES:
ARMY - MD, ME
NAVY - AS, YD
REVIEWER ACTIVITIES:

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

APPROVED 03 SEP 63 REVISED Ⓐ 31 MAR 81 Ⓑ 20 SEP 1988