A-A-53973
9 November 1989

COMMERCIAL ITEM DESCRIPTION

# BAG, BLOOD COLLECTING-DISPENSING-FREEZING

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a sterile, pyrogen-free disposable, plastic, blood collecting/freezing, component processing, and dispensing system.

Salient characteristics:

Shall be a sterile, pyrogen-free, disposable, plastic, blood collecting/freezing component processing and dispensing system. The system shall consist of the components interconnected as shown in Figure 1. The system and anticoagulant shall be in conformance with all requirements of the FDA.

Primary bag. The primary bag shall have an 800 ml capacity and shall contain 63 ml of CPDA-1 anticoagulant for collecting 450 ml of blood. The bag be fabricated of polyvinylchloride (PVC). The bag shall possess two blood outlet ports consisting of externally protruding tubes sealed and closed by an internal transverse puncturable plastic diaphragm within the tube. This diaphragm shall be readily puncturable for connecting to a standard blood recipient set, and Bowl, Washing and Waste Bag Set (See Note 2). Sterility shall be maintained by a tamperproof protective sheath. Design shall be such that the piercing end of the recipient set will make a leakproof connection prior to puncture of diaphragm and provide protection to the bag walls against piercing. The bag shall have a horizontal slot as a means of suspending for infusion approximately 1-1/4 inch (3.2 cm ) long and two circular holes located at the top to permit suspension in the upright position. Donor tube and needle shall be not less than 51 inches (129.54 cm) long and shall bear at least 10 indelibly imprinted identification numbers not more than 3-1/4 inches (8.1 cm) apart. Donor needle shall be 16 gage, thin wall, 1.5- 1.6 inch (3.81- 4 cm) long. Needle shall have a sharp, smoothly expanding ground bevel between 0.203 and 0.318 inch (0.516-0.808 cm long).

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Interior lumen connection to donor tube shall present a smoothly expanding surface to prevent platelet aggregation and clotting needle shall be protected by a tamperproof sheath. During removal only sterile surfaces and edges shall contact the needle cannula. Needle cannula shall be Class 3, austenitic corrosion-resisting steel in accordance with ASTM Designation F899.

Transfer packs. The transfer packs shall each have a 400 ml capacity. The first transfer pack shall be suitable for use in collecting excess glycerol.

The second and third transfer packs are to be used for fresh frozen plasma and 5-7 day platelet concentration, one of which must be polyvinyl choloride (PVC) or polyolefin (including connecting tubing). All transfer packs must possess two standard outlet ports consisting of externally protruding tubes sealed and closed by an internal transverse puncturable plastic diaphragm within the tube. The diaphragm shall be maintained by a tamperproof sheath. Design shall be such that the piercing end of the recipient set will make a leakproof connection prior to puncture of diaphragm and provide protection to the bag walls against piercing.

Outlet port. The standard outlet port shall be suitable for adding 40% glycerol, rejuvinating solutions and other additions. Shall be of the same type port described under primary bag. Sterility shall be maintained by a tamperproof sheath or cap. Shall allow complete acceptance of the stylet end of a transfer set.

Tubing. Tubing from "Y" connector to all transfer packs and donor tubing shall bear indelibly imprinted identification numbers with center-to-center distance being at least 2-7/8 inches (7.2 cm) and not more than 3-1/4 inches (8.1 cm) long. At least 6 numbers shall be provided on the first transfer pack connecting tubing. At least 4 numbers shall be provided on each leg of the second and third transfer pack tubing. Tubing shall have an outer diameter of .158 +/- .003 inches with wall thickness of .020 +/- .002 inches.

Centrifugation. The primary bag and transfer packs shall be shaped to permit centrifugation in the 1000 ml standard trunnion cup of the centrifuge indicated in Note 3. Internal dimensions of the primary bag shall be not less than 8 inches (20 cm) long and 4-3/4 inches (11.8 cm) wide nor more than 9 inches (22.5 cm) long and 5-1/4 inches (13.1 cm) wide.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Commonality label. The primary bag and transfer packs shall bear a single label that is printed according to the latest FDA Guidelines for Uniform Labeling. This is referred to as "Commonality Label" and shall be in conformance with the Food and Drug Administration requirements. This label shall be permanently sealed to the bag. Additional markings to this label shall include manufacturer's name and lot number. The bag shall be made of such material so that applied labels and writing shall remain adhered throughout the useage time (up to 20 years).

The system internal surfaces shall be pyrogen-free, non-toxic and sterile when tested in accordance with the USP. Material of tubing and bags shall be compatible with the blood or blood component stored therein. The sterility assurance level for the system shall be $1x\ 10^{-6}$ in accordance with AAMI guidelines. The system shall meet Class IV biological tests when tested in accordance with the USP.

Expiration dating period of the system shall not be less than 30 months. Not less than 27 months of the expiration dating period shall remain at the time of the delivery to the Government.

Workmanship. The system shall be free from defects which detract from its appearance or impair its serviceability. The system components shall be free from cuts, tears, weak points, discoloration or flash.

Unit. (PG). One package (sealed foil pouch) containing four blood collecting-dispensing-freezing systems, as specified, constitutes one unit. The pouch shall be capable of maintaining sterility of contents. As an alternate, two pouches containing two blood collecting-dispensing-freezing system shall be overwrapped to constitute one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be Level S-4 with acceptance number zero conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one blood warming bag.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Note 1: The following National Stock Number is covered by this document:

| NSN | ITEM IDENTIFICATION |
|---|---|
| 6515-01-234-6831 | BAG, BLOOD COLLECTING-DISPENSING-FREEZING with 63 ml CPDA-1, Anticoagulant, Quadruple Pack, with 5-7 day Platelet Pack, Disposable, 4's |

Note 2: The Blood Collecting-Dispensing-Freezing Bag covered by this specification shall be used with an Indirect Transfusion Blood Recipient Set (NSN 6515-01-128-1407), and a Washing and Waste Bag Set Bowl (NSN 6640-01-234-9582).

Note 3: The Blood Collecting-Dispensing-Freezing Bag covered by this specification shall be used with a Laboratory Centrifuge (NSN 6640-01-139-7457), which is equal to Dupont Model RC-3B.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

A-A-53973

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4594



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

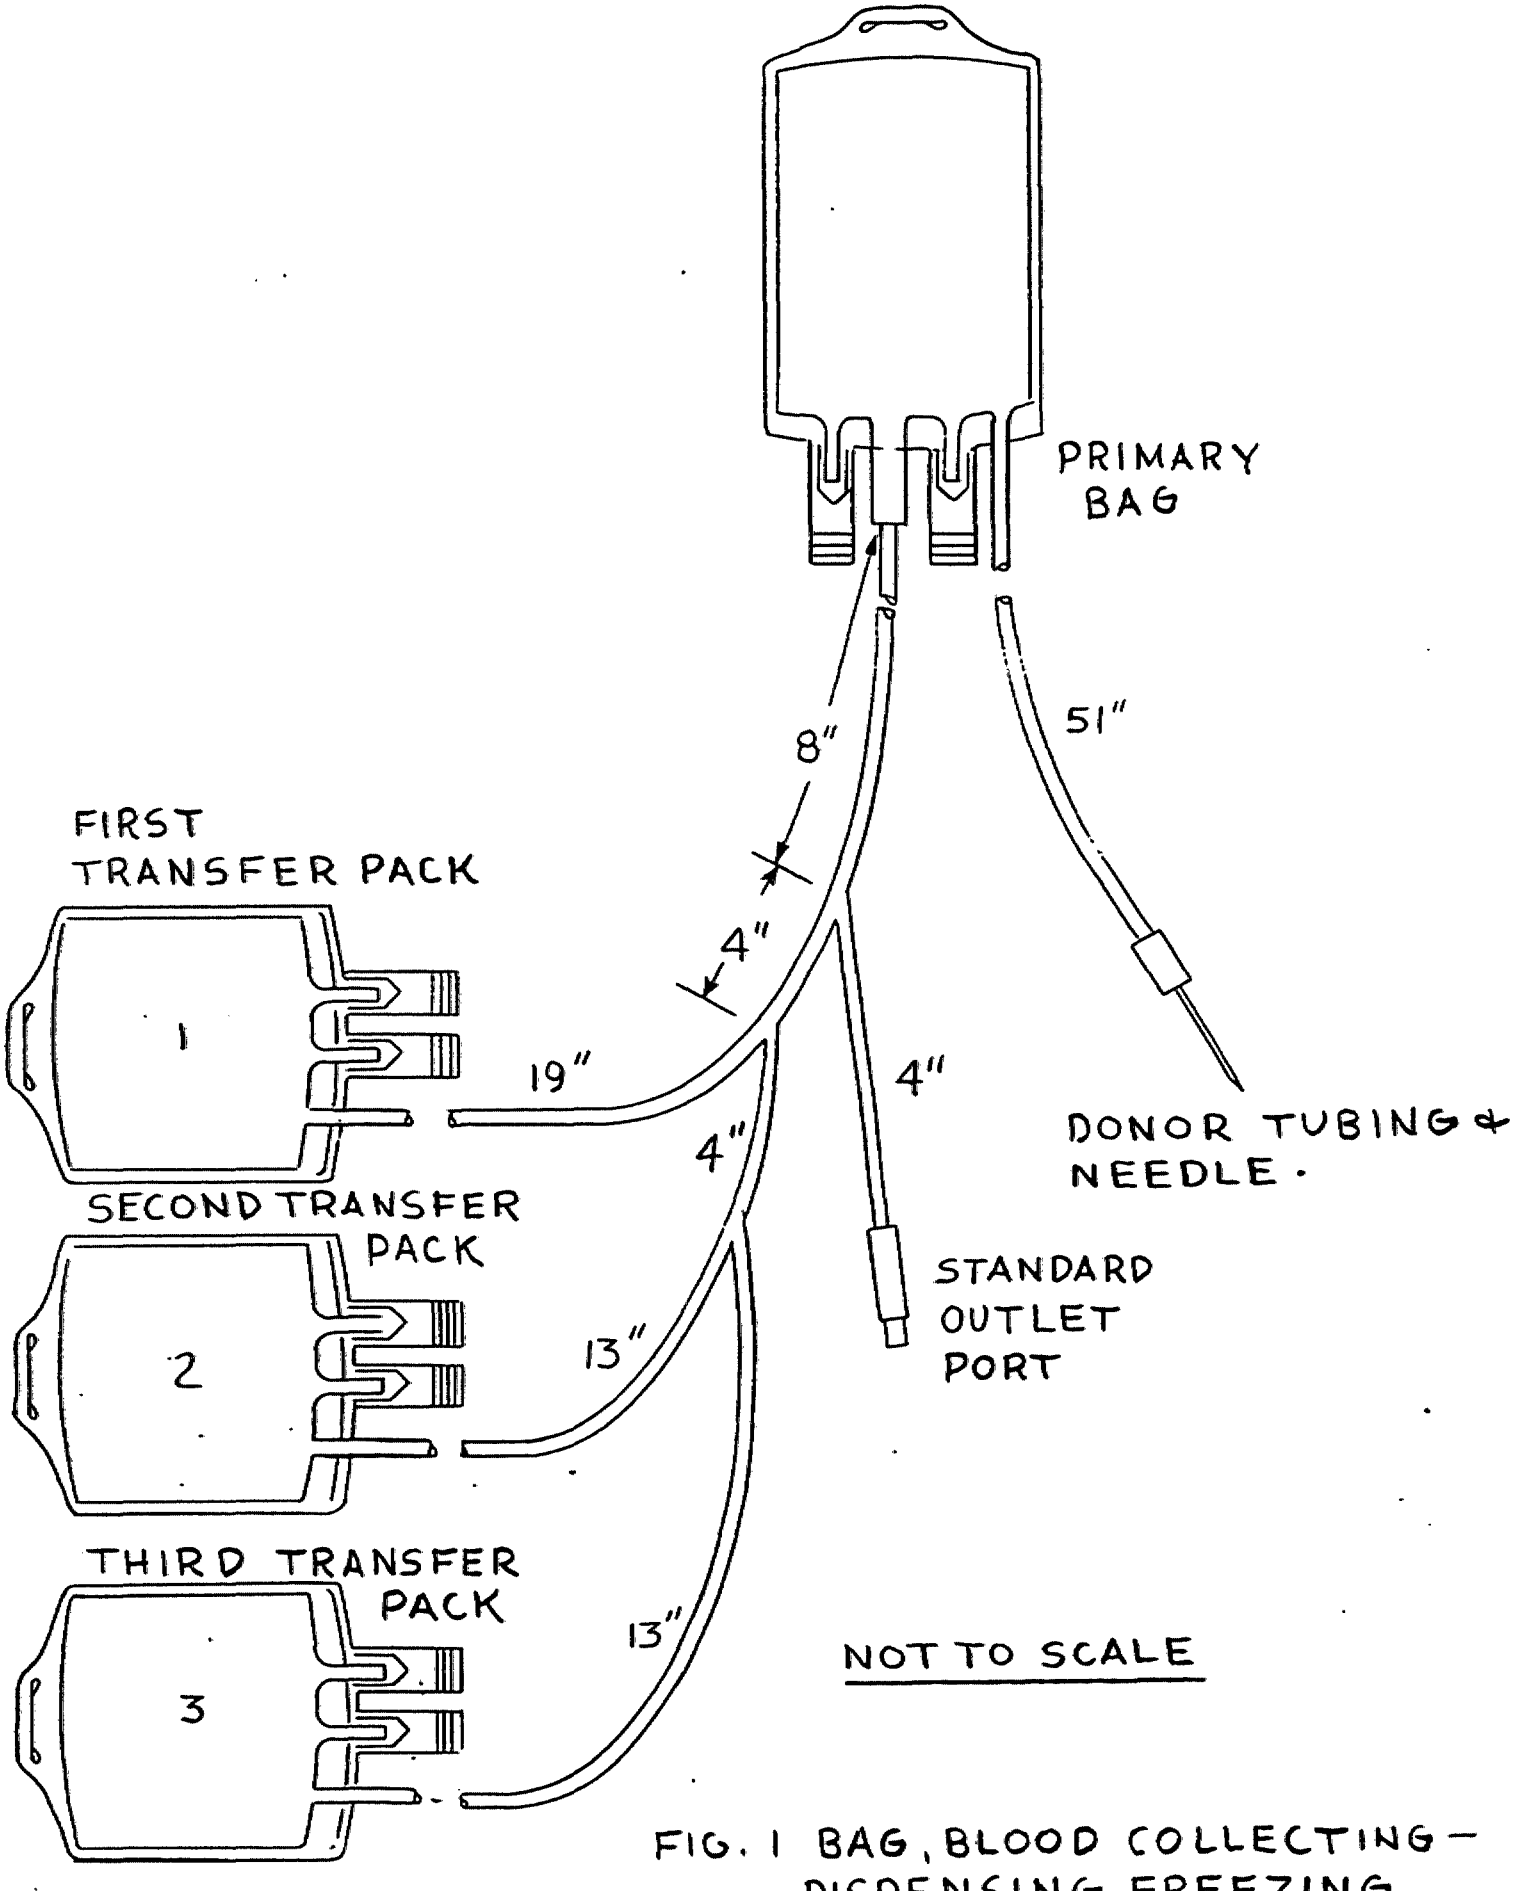



FIG. 1 BAG, BLOOD COLLECTING-DISPENSING, FREEZING

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS:** In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*; and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

*NOTE:* This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

*(Fold along this line)*

*(Fold along this line)*

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 Alexandria, VA.

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions – Reverse Side)*

| 1. DOCUMENT NUMBER | 2. DOCUMENT TITLE |
|---|---|
| A-A-53973 | BAG, BLOOD COLLECTING-DISPENSING-FREEZING |

**3a. NAME OF SUBMITTING ORGANIZATION**

**b. ADDRESS** *(Street, City, State, ZIP Code)*

**4. TYPE OF ORGANIZATION** *(Mark one)*

- ☐ VENDOR
- ☐ USER
- ☐ MANUFACTURER
- ☐ OTHER *(Specify)*: _____

**5. PROBLEM AREAS**

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

**6. REMARKS**

**7a. NAME OF SUBMITTER** *(Last, First, MI)* — Optional

**b. WORK TELEPHONE NUMBER** *(Include Area Code)* — Optional

**c. MAILING ADDRESS** *(Street, City, State, ZIP Code)* — Optional

**8. DATE OF SUBMISSION** *(YYMMDD)*

*(TO DETACH THIS FORM, CUT ALONG THIS LINE.)*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.