FED. SUP CLASS
6640

REVIEW ACTIVITIES: ARMY - AS, CE
AIR FORCE - 82

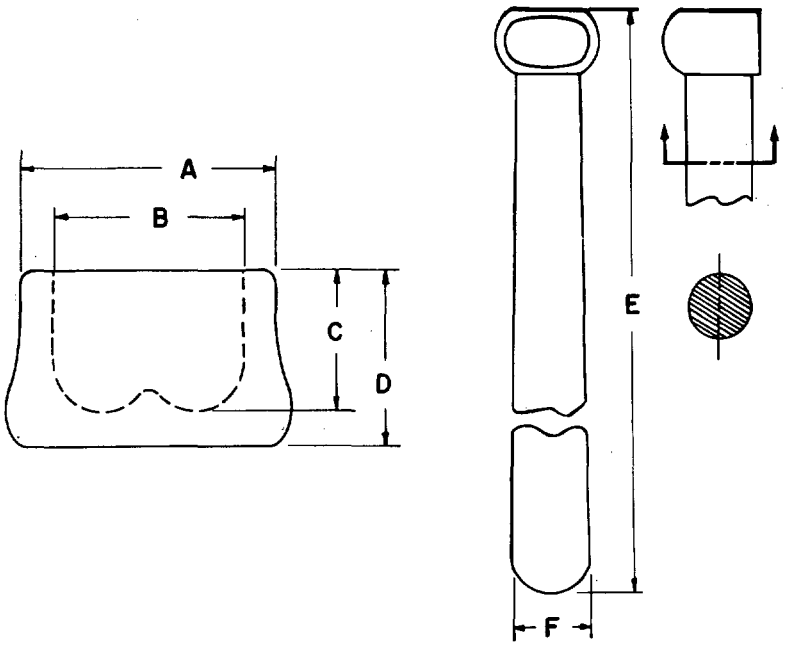

PART NUMBER	DIMENSIONAL DATA (in.)					
	MORTAR				PESTLE	
	A TOP OD	B TOP ID	C INSIDE DEPTH	D HEIGHT	E LENGTH	F BASE DIA
MS36101-1	1-7/8 (± 3/16)	1-3/8 (± 3/16)	1 (± 3/16)	1-1/4 (± 3/16)	4-5/8 (± 1/4)	5/8 (± 1/16)

MATERIAL: Mortar and pestle shall be glass.

(A) DESIGN: Mortar shall have a mound on the inside floor for trituration.

Pestle shall have one flat side.

Mortar and pestle shall be in accordance with Federal Specification NNN-M-560, Type II, Class B, Style I.

FINISH: Inside surfaces of mortar and grinding end of pestle shall be etched and sandblasted. Other surfaces shall be etched or frosted.

NOTES:
1. For design feature purposes, this standard takes precedence over procurement documents referenced herein.
2. Referenced documents shall be of the issue in effect on date of invitations for bid.

APPROVED 22 SEPT 1960 REVISED (A) 31 MAY 1967

This military standard is approved by the Department of Defense and is mandatory on all activities. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A.	MU	TITLE	MILITARY STANDARD
Other Cust	MS 82	MORTAR AND PESTLE, LABORATORY dental	MS36101
Procurement Specification NNN-M-560		SUPERSEDES:	SHEET 1 OF 1

DD FORM 1 SEP 63 672 (Coordinated)

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:34Z
Check the source to verify that this is the current version before use.