MILITARY SPECIFICATION SHEET

CABINET, STORAGE, STEEL: MULTIPLEX LABORATORY SUPPLIES; TYPE IX

The complete requirements for procuring the cabinet described herein shall consist of this document and the issue in effect of MIL-C-40060.

REQUIREMENTS:

Dimensions and configurations shall be as shown on figure 1.

COMPONENTS:

Sliding doors, knobs, and shelves shall be as specified herein and MIL-C-40060, as applicable.

CONSTRUCTION:

Knobs. The knobs shall be of corrosion-resistant metal or of material treated to resist corrosion. The knobs on both doors shall operate latching mechanisms that engage the top and bottom of the cabinet.

Shelves. The three shelves shall be height adjustable at not more than 3-inch intervals.

Custodian:

Army - GL

Review activities:

Army - ME, NS

Preparing activity:

Army - GL

Project No. 7125-A054/9

FSC 7125

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T19:08Z
Check the source to verify that this is the current version before use.

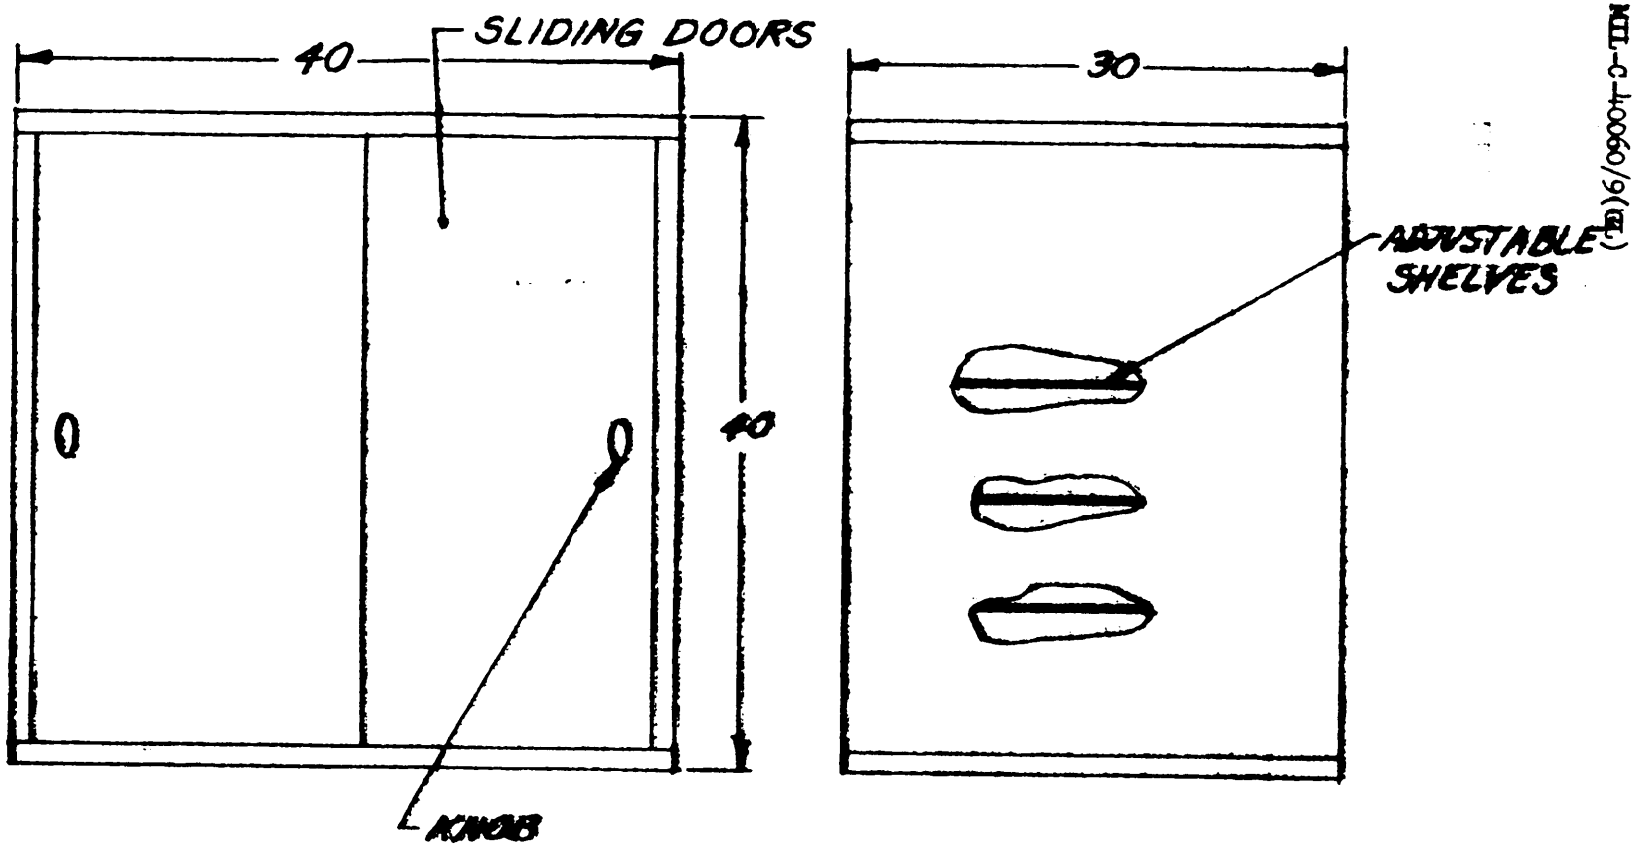


FIGURE 1. CABINET, STORAGE, STEEL, MULTIPLEX LABORATORY SUPPLIES; TYPE II

Source: https://assist.dla.mil -- Downloaded: 2026-02-21T19:08Z
Check the source to verify that this is the current version before use.