|INCH-POUND|
MIL-R-81553B(AS)
17 September 1992
SUPERSEDING
MIL-R-81553A(AS)
30 August 1983

MILITARY SPECIFICATION

REGULATOR, CHEST MOUNTED, OXYGEN, POSITIVE PRESSURE, CRU-79/P

This specification is approved for use by the Naval Air Systems Command, Department of the Navy, and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers oxygen (94 percent and above), positive pressure, chest mounted regulator, type CRU-79/P.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications, standards and handbooks. The following specifications, standards, and handbooks form a part of this document to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation (see 6.2).

SPECIFICATIONS

FEDERAL

BB-N-411	-	Nitrogen, Technical
PPP-B-591	-	Boxes, Shipping, Fiberboard, Wood-Cleated
PPP-B-601	-	Boxes, Wood, Cleated-Plywood
PPP-B-621	-	Box, Wood, Nailed and Lock Corner
PPP-B-636	-	Boxes, Shipping, Fiberboard
PPP-B-640	-	Boxes, Fiberboard, Corrugated, Triple Wall
PPP-T-60	-	Tape, Packaging, Waterproof

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Commanding Officer, Naval Air Warfare Center Aircraft Division Lakehurst, Code SR3, Lakehurst, NJ 08733-5100, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC N/A
FSC 1660
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

MILITARY

MIL-P-116	-	Preservation, Methods of
MIL-C-5541	-	Chemical Conversion Coatings on Aluminum and Aluminum Alloys
MIL-P-7105	-	Pipe Threads, Taper, Aeronautical National Form, Symbol ANPT, General Requirements for
MIL-A-8625	-	Anodic Coatings, for Aluminum and Aluminum Alloys
MIL-B-22191	-	Barrier Material, Transparent, Flexible, Heat Sealable
MIL-O-27210	-	Oxygen, Aviator's Breathing, Liquid and Gas

STANDARDS

FEDERAL

FED-STD-595	-	Colors Used in Government Procurement

MILITARY

MIL-STD-105	-	Sampling Procedures and Tables for Inspection by Attributes
MIL-STD-129	-	Marking for Shipment and Storage
MIL-STD-130	-	Identification Marking of U.S. Military Property
MIL-STD-889	-	Dissimilar Metals
MIL-STD-970	-	Standards and Specifications, Order of Precedence for the Selection of
MIL-STD-1359	-	Cleaning Methods and Procedures for Breathing Oxygen Equipment
MS33658	-	Fitting End, Hose Connections, Standard Dimensions for

HANDBOOKS

MILITARY

MIL-HDBK-695	-	Rubber Products: Recommended Shelf Life

(Unless otherwise indicated, copies of federal and military specifications, standards and handbooks are available from the Standardization Documents Order Desk, Bldg. 4D, 700 Robbins Avenue, Philadelphia, PA 19111-5094.)

2.1.2 Other Government documents, drawings, and publications. The following other Government documents, drawings, and publications form a part of this document to the extent specified herein. Unless otherwise specified, the issues are those cited in the solicitation.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the currentversion before use.

DRAWINGS

Naval Air Systems Command

33C1178	-	Hose Assembly, Oxygen, Disconnect to Chest Mounted Regulator
62A-116-C48	-	Piezometer
62A-116-C49	-	Tube Piezometer
62A-116-C50	-	Ring Piezometer
62A-116-C51	-	Union Piezometer
834-18	-	Tube, Delivery MBU-12/P
62A-116-E1	-	Oxygen Components Test Stand
1172AS100	-	Oxygen Components Test Stand
1316AS100	-	Oxygen Components Test Stand
1964AS100	-	Hose Assembly, Oxygen, Seat Kit to Pilot and Ship's Supply, F/A-18
2004AS100	-	Manifold Body, Oxygen, Seat Survival Kit, SKU-2/A

(Copies of drawings required by manufacturers in connection with specification acquisistion functions should be obtained from the Contracting Activity or as directed by the contracting officer.)

DEFENSE STANDARDIZATION MANUAL

SD-6	-	Provisions Governing Qualification (QPL)

(Unless otherwise indicated, copies of Defense standardization manuals are available from the Standardization Documents Order Desk, Bldg. 4D, 700 Robbins Avenue, Philadelphia, PA 19111-5094.)

2.2 Non-Government publications. The following documents form a part of this document to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DODISS cited in the solicitation. Unless otherwise specified, the issues of documents not listed in the DODISS are the issues of the documents cited in the solicitation (see 6.2).

AMERICAN SOCIETY FOR TESTING MATERIALS (ASTM)

ASTM D 1149-91	Rubber Deterioration - Surface Ozone Cracking in a Chamber (Flat Specimen)

(Application for copies should be addressed to: American Society for Testing Materials, 1916 Race St., Philadelphia, PA 19103).

(Non-Government standards and other publications are normally available from the organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this document, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Qualification. The regulators furnished under this specification shall be products which are authorized by the qualifying activity for listing on the applicable Qualified Products List at the time of award of contract (see 4.3 and 6.3).

3.2 First article. When specified (see 6.2.), a sample shall be subjected to first article inspection (see 6.4) in accordance with 4.4.

3.3 Selection of specifications and standards. Specifications and standards for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-970.

3.4 Materials. Materials shall conform to applicable specifications and shall be as specified herein and on applicable drawings. Materials which are not covered by specifications, or which are not specifically described herein, shall be of the best quality, of the lightest practicable weight, and suitable for the purpose intended. Materials that produce toxic or corrosive substances shall not be used.

3.4.1 Metal parts. All metal parts shall be of a corrosion resistant material or treated in a manner to render them adequately resistant to corrosion.

3.4.1.1 Dissimilar metals. Unless protected against electrolytic corrosion, dissimilar metals shall not be used in intimate contact with each other. Dissimilar metals are defined in MIL-STD-889.

3.4.1.2 Finish. Aluminum and aluminum alloy parts shall be protected in accordance with MIL-A-8625 or MIL-C-5541.

3.4.2 Nonmetallic materials. Any nonmetallic material that is adversely affected by continued use with oxygen shall not be used.

3.4.2.1 Age. Elastomer components except silicone shall not be more than 12 months old from the date of manufacture to the date of delivery to any Government service or to any airframe or accessory manufacturer.

3.4.2.2 Elastomer components. The elastomer components shall be composed of an ozone resistant composition, which shall not bloom, and shall meet the specified ozone resistance performance requirements (3.7.14).

3.4.2.3 Storage life. Elastomeric materials selected shall have an expected shelf storage life of 8 years or more based on the guidelines of MIL-HDBK-695.

3.4.3 Protective treatment. When materials are used in the construction of the unit that are subject to deterioration when exposed to environmental conditions likely to occur during service usage, they shall be protected against such deterioration in a manner that will in no way prevent compliance with the performance requirements of this specification. Protective coating which might crack, chip or scale during normal service life or under extremes of environmental conditions shall not be used.

3.4.4 Adhesives. The regulator shall not contain glue, varnish or other such coatings or adhesives to secure parts (except labels), or to seal leaks.

3.5 Standard parts. Oxygen clean MS and AN Standard parts shall be used where they suit the purpose.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

3.6 Design and construction. The chest mounted oxygen regulator shall be designed in accordance with Figure 1. The regulator size shall not exceed the specified envelope dimensions. The regulator shall be designed so that the aneroid can be adjusted. Aneroid bleed holes shall be visible, accessible, and capable of being blocked. The regulator shall operate in every orientation.

3.6.1 Oxygen inlet. A filter capable of filtering materials 20 microns in size shall be provided in the oxygen inlet to prevent foreign particles from entering the regulator while in service. The filter shall be so installed that it can be easily removed or replaced.

3.6.2 Moisture. The design shall include provisions for preventing moisture from collecting within the regulator.

3.6.3 Plugs. The inlet and outlet of the regulator shall be closed with caps or plugs to prevent foreign matter from entering the regulator during shipping and storage.

3.7 Performance.

3.7.1 Outlet pressure (steady state). The outlet pressures of the regulator, when tested as specified in 4.8.2, shall be in accordance with the requirements of Table I. During test, the regulator shall not vibrate, flutter, chatter, or cause the output flow to fluctuate.

3.7.2 Outlet pressure (dynamic). The outlet pressure of the regulator, when tested as specified in 4.8.3, shall be in accordance with the limits specified in Table II. During test, the regulator shall not vibrate, flutter, or chatter.

3.7.3 Noise level control. The 1/3 octave band analysis of the regulator, measured in accordance with in 4.8.4, shall not exceed the decibel levels (dB) of Table IV.

3.7.4 Overload.

3.7.4.1 Outlet. The regulator, when tested as specified in 4.8.5.1, shall not show any evidence of leakage or damage.

3.7.4.2 Inlet. The regulator, when tested as specified in 4.8.5.2, shall have an outlet pressure that does not exceed 2.5 inches of water.

3.7.5 Leakage.

3.7.5.1 Body leakage. The regulator, when tested as specified in 4.8.6.1 and 4.8.6.2, shall not show any evidence of leakage through the body of the regulator.

3.7.5.2 Designed bleed flow. The designed bleed flow rate, when tested as specified in 4.8.6.3, shall not exceed 900 cubic centimeters per minute (ccm).

3.7.5.3 Demand valve leakage - outward. The outlet pressure of the regulator, when tested as specified in 4.8.6.4, shall be 0.5 to 2.5 inches of water. The outlet pressures after the five-minute period shall be the same as the initial outlet pressures.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the currentversion before use.

3.7.6 Extreme temperature.

3.7.6.1 High temperature. The regulator, when tested as specified in 4.8.7.1, shall show no evidence of mechanical or material failure, and the outlet pressure shall be within ± 0.5 inch of water of the outlet pressure requirements specified in Table I.

3.7.6.2 Low temperature. The regulator, when tested as specified in 4.8.7.2, shall show no evidence of mechanical or material failure, and the outlet pressure shall be within ± 0.5 inch of water of the outlet pressure requirements specified in Table I.

3.7.7 Vibration. The regulator, when tested as specified in 4.8.8, shall show no evidence of mechanical or material failure, and shall operate in accordance with Table I during post-vibration outlet pressure test specified in 4.8.2.

3.7.8 Acceleration. The regulator, when tested as specified in 4.8.9, shall maintain the outlet pressures of Table I for ground level condition at 0, 50, and 100 liter per minute (lpm) flows and shall show no evidence of mechanical or material failure. The 100 lpm flow, established prior to the application of the 7 g force, shall not change as the g force is increased.

3.7.9 Endurance. The regulator, when tested as specified in 4.8.10, shall show no evidence of mechanical or material failure and shall operate in accordance with Table I during the post-endurance outlet pressure test specified in 4.8.2.

3.7.10 Altitude cycling. The regulator, when tested as specified in 4.8.11, shall show no evidence of mechanical or material failure and shall operate in accordance with Table I during the post-cycling outlet pressure test specified in 4.8.2.

3.7.11 Shock. The regulator, when tested as specified in 4.8.12, shall show no evidence of mechanical or material failure and shall operate in accordance with Table I during the post-cycling outlet pressure test specified in 4.8.2.

3.7.12 Repeat of noise level control test. The 1/3 octave band analysis of the regulator, after tests specified in 4.8.13, shall not exceed the decibel levels (dB) of Table IV.

3.7.13 Underwater breathing capabilities. The regulator, when tested as specified in 4.8.14, shall be capable of delivering an adequate supply of oxygen and the subject shall be capable of breathing from the regulator while in the submerged condition.

3.7.14 Ozone resistance. The elastomer test slabs, when tested as specified in 4.8.15, shall not show any evidence of checking, cracking, or other damage.

3.7.15 Oxygen regulator purge. When tested as specified in 4.8.16, the regulator shall not ignite and there shall not be any evidence of charring or deterioration.

3.8 Interchangeability. All parts, subassemblies and assemblies having the same part number shall be dimensionally and mechanically interchangeable.

3.9 Weight. The weight of the oxygen regulator shall not exceed 5 ounces.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

3.10 Color. The color of the regulator shall be black, approximately matching color number 37038 of FED-STD-595.

3.11 Cleanliness.

3.11.1 Degreasing. Prior to assembling the regulator and its sub-assemblies, all internal surfaces shall be degreased in accordance with MIL-STD-1359. The regulator shall be free of grease and other organic materials.

3.12 Identification of product. The regulator shall be identified in accordance with MIL-STD-130, except that the Federal Stock Number shall be omitted from the nameplate.

3.12.1 Serial numbers. The regulators shall be identified by individual serial numbers which shall be assigned by the manufacturer. Serialization shall be by a block of consecutive numbers to cover the entire acquisition quantity (see 4.6.2).

3.13 Workmanship. The regulator shall be uniform in quality and shall be free from irregularities, defects or foreign material which could adversely affect safety, performance, reliability, or durability. The interior of the regulator shall be free from odor.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to ensure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items shall meet all requirements of Section 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of ensuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling inspection, as part of manufacturing operations, is an acceptable practice to ascertain conformance to requirements, however, this does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to acceptance of defective material.

4.2 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. Qualification inspection (see 4.3).
b. First article inspection (see 4.4).
c. Quality conformance inspection (4.5).
d. Quality conformance verification inspection (see 4.6).

4.3 Qualification inspection. Qualification inspection shall be as specified in Table V (listed sequence mandatory).

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

4.3.1 Qualification samples. Qualification samples shall consist of four regulators, three elastomer test slabs, 6 by 6 by 0.075 inch, composed of the identical ozone-resistant composition and cure that was used in manufacturing the elastomer components and two sets of manufacturer's drawings for the samples submitted (see 6.3.1). Samples shall be forwarded to a test facility set forth in the letter of authorization to submit samples (see 6.3). The samples shall be plainly identified by securely attached durable tags marked with the following information:

> Sample submitted by (name) (date) for qualification inspection in accordance with the requirements of MIL-R-81553B(AS) and number under authorization (reference authorizing letter and number) (see 6.3).

4.3.2 Retention of qualification. The retention of qualification shall consist of periodic verification to determine compliance of the qualified regulator with the requirements of this specification. The time and method of periodic verification shall be specified by the activity responsible for the Qualified Products List and shall be included in the Notice of Qualification letter.

4.4 First article.

4.4.1 First article inspection. First article inspection shall be as specified in Table VI (listed sequence mandatory).

4.4.2 First article samples. Unless otherwise specified, as soon as practicable, after the award of the contract or order, the manufacturer shall submit four complete regulators and three elastomer test slabs, 6 by 6 by 0.075 inch, composed of the identical ozone-resistant composition and cure that was used in manufacturing the elastomer components. The samples shall be representative of the construction, workmanship, components and materials to be used during production. When a manufacturer is in continuous production of these units from contract to contract, submission of further first article samples on a new contract may be waived at the discretion of the acquiring activity (see 6.2). Approval of the first article samples or the waiving of the first article inspection does not eliminate the requirements of submitting to the quality conformance inspection and the quality conformance verification inspection. The first article inspection samples shall be furnished to the Government as directed by the contracting officer (see 6.2).

4.4.2.1 First article information. Upon completion of the first article inspection program, pertinent comments and recommendations will be forwarded by the Government activity responsible for the inspection program (see 6.2) to the contracting officer. Disposition of samples will be as follows:

a. One approved sample will be initially returned to the contractor for use in monitoring production.

b. One approved sample will be retained by the test facility for reference during quality conformance verification inspection and will be returned to the contractor with the samples from the final production lot.

c. The remaining samples will be consumed or destroyed during the inspection program and shall not be considered as part of the quantity to be delivered under the acquisition document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:35Z
Check the source to verify that this is the current version before use.

4.5 Quality conformance inspection. The sampling and inspection levels and acceptance criteria shall conform to MIL-STD-105 and Table VII. Quality conformance inspection shall be as specified in Table VII (listed sequence mandatory).

4.5.1 Sampling.

4.5.1.1 Inspection lot.

4.5.1.1.1 Regulator. An inspection lot size shall be expressed in units of one regulator made under essentially the same conditions and from the same materials and components. The sample unit shall be one regulator.

4.5.1.1.2 Packaging. An inspection lot size shall be expressed in units of fully prepared shipping containers, containing regulators, fully prepared for delivery just prior to closure, made from essentially the same materials and components. The sample unit shall be one shipping container, containing regulators, fully prepared for delivery with the exception that it need not be sealed.

4.6 Quality conformance verification.

4.6.1 Quality conformance verification inspection. The quality conformance verification inspection shall be as specified in Table VIII (listed sequence mandatory).

4.6.2 Quality conformance verification samples. Upon completion of the tests and examinations specified in Table VII, a random sample shall be selected from each lot in accordance with MIL-STD-105, Inspection Level I. The tests and examinations required for the regulators shall be as specified in Table VIII. The sample size and acceptance criteria shall be in accordance with MIL-STD-105 for single sampling plans for normal inspections. Each regulator, selected as a sample unit, shall be identified by its assigned serial number (see 3.12.1) and shall be forwarded to the inspection facility specified in the acquisition document (see 6.2). Additionally, the serial numbers of the units within the lot, represented by the sample units, shall be furnished to the inspection facility.

4.6.3 Quality conformance verification approval. Upon completion of the quality conformance verification inspection, the Government activity responsible for conducting the inspection program (see 6.2) shall report the results of tests, with recommendations, to the contracting officer of the procuring activity specified in the acquisition document. Final acceptance of the lot from which the samples were selected shall be based upon completion of the inspection program by the Government Quality Assurance Representative/Specialist.

4.7 Test conditions.

4.7.1 Gas. Unless otherwise specified, the gas used in testing the regulator shall be oil-free nitrogen, 99.95 percent pure, conforming to Type I, Grade A, Class 1 of BB-N-411 or oxygen conforming to Type I of MIL-O-27210. The gas used in the oxygen regulator purge shall be oxygen in accordance with MIL-O-27210, Type I.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

4.7.2 Temperature and pressure. Unless otherwise specified, tests shall be conducted at local ambient temperature and barometric pressure. Test instruments shall be calibrated or adjusted according to their required usage in conducting individual tests. Temperature and pressure shall be recorded at the time of inspection and, when required, the test results shall be corrected to normal temperature and pressure (NTP) conditions. NTP conditions are 29.92 inches of mercury (101.3 kPa) and 70°F (21.1°C). In the case of pressure drop measurements, the flow setting for conducting the test shall be corrected to NTP conditions before the test in conducted.

4.7.3 Adjustment of inlet supply pressure. At the start of the operational tests, the initial static test inlet pressure of 40, 50, 70 or 120 psig applies only to zero flow conditions. When the pressure reducing regulator device is not in the same ambient conditions as the oxygen breathing regulator, means shall be provided to determine the above noted pressure at the ambient conditions of the breathing regulator. When flow is started, the inlet supply pressure shall not be allowed to drop more than 8 psig at 100 lpm ambient flow for inlet pressures of 50, 70 or 120 psig. Under no condition shall the inlet supply pressure be allowed to drop below 40 psig.

4.7.4 Orientation. Unless otherwise specified, the regulator may be mounted in any position while conducting the tests specified herein.

4.7.5 Piezometer assembly. Unless otherwise specified, the regulator shall be operated with a test gas (see 4.7.1) at an inlet supply pressure of 40 to 120 psig. The outlet pressure shall be measured using a piezometer assembly conforming to drawings 62A-116-C48, 62A-116-C49, 62A-116-C50 and 62A-116-C51. The piezometer shall be connected to the outlet of the regulator as shown on Figure 2. The regulator outlet pressures shall be measured at the piezometer union shown in drawing 62A-116-C48.

4.7.6 Vibratory control. Flutter dampers may not be used to control or eliminate the output flow fluctuation.

4.7.7 Test equipment.

4.7.7.1 Test equipment. All flow and pressure tests should be performed on test stands in accordance with Drawings 62A-116-E1, 1172AS100, or 1316AS100. Oxygen shall not be used as a test gas on these stands. Regulators, when tested on other stands, shall be capable of fulfilling all flow and pressure test requirements of this specification when tested on test stands in accordance with Drawings 62A-116-E1, 1172AS100 or 1316AS100.

4.7.7.2 Noise level control test set-up. Noise level control test set-up shall be in accordance with Figure 4 and the test shall be conducted in accordance with 4.8.4. The noise analysis equipment shall consist of Bruel & Kjaer test equipment, or equivalent, and shall include the following:

Description	Model No.
Digital Frequency Analyzer	2131
Condenser Microphone 1" Free Field	4145

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:35Z
Check the source to verify that this is the current version before use.

Condenser Microphone Preamplifier	2619S
Graphic Level Recorder, With Voltage Control Paper Drive	2307A
Operation 2120 and 1614-10 Synchronous or Charge Cable	AQ-0035

4.7.7.3 Breathing Simulator. All dynamic breathing tests shall be performed on a KRUG INTERNATIONAL breathing simulator model TS8225-PC or equivalent. Regulators, when tested on other simulators, shall be capable of fulfilling all flow and pressure test requirements of this specification when tested on the specified breathing simulator. The simulator shall breathe through an MBU-14/P oxygen mask secured to a head form with an airtight mask seal and connected to the regulator by an oxygen hose conforming to drawing number 834-18. Inlet pressure to the regulator shall be supplied through the regulator-to-seat kit hose (drawing No. 33C1178-1), seat kit hose (drawing No. 1964AS100-1), seat kit manifold assembly (drawing No. 2004AS100-1), and check valve (part No. 30941/EW63003) from a reservoir held at constant pressure. Regulators, when tested by an equivalent method, shall be capable of fulfilling all flow and pressure test requirements.

4.8 Inspection methods.

4.8.1 Visual examinations.

4.8.1.1 Regulator. Every regulator shall be examined visually for the critical defects listed in Table IX to determine conformance to this specification and applicable drawings.

4.8.1.2 Packaging. Each of the fully prepared shipping containers, containing regulators, selected as a sample unit from the lot, shall be examined to determine that the packaging, packing and marking conform to this specification. The list of defects, Table X, shall be used to enumerate the defects found.

4.8.2 Outlet pressure (steady state). The regulator shall be connected to a pressure source capable of providing the inlet pressures indicated in Table I. The regulator shall then be subjected to the pressures and conditions specified in 4.8.2.1 or 4.8.2.2, as applicable. The outlet pressure shall be measured as specified in 4.7.5, with the use of a piezometer assembly, and shall pass the requirements specified in 3.7.1.

4.8.2.1 Outlet pressure - qualification and first article inspections. Qualification and first article inspections shall be performed utilizing the altitudes, inlet supply pressures and flows delineated in Table I.

4.8.2.2 Outlet pressure - quality conformance and quality conformance verification inspections. Quality conformance and quality conformance verification inspections shall be performed in accordance with Table I except that the test shall be conducted using ambient air flows of 0, 50, and 100 lpm with inlet pressures of 40 and 120 psig at altitudes of ground level, 10,000, and 30,000 feet. In the pressure breathing range, tests shall be conducted utilizing ambient flows of 0 and 100 lpm with inlet pressures of 40 and 120 psig at altitudes of 34,000, 40,000, 45,000, and 50,000 feet.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

4.8.3 Outlet pressure (dynamic). The regulator shall be connected to a pressure source to provide inlet pressures as specified in Table II. A breathing regulator shall be connected to the regulator outlet as described in 4.7.7.3. The breathing simulator shall be set to the flowrates specified in Table II and the regulator outlet pressures shall be recorded in accordance with Figure 3. The regulator shall pass the requirements specified in 3.7.2.

4.8.4 Noise level control. The regulator shall be installed as shown on Figure 4. The regulator shall then be subjected to an ambient flow of 100 lpm at an inlet pressure of 70 and 120 psig. The noise level shall be measured and shall pass the requirements specified in 3.7.3.

4.8.5 Overload.

4.8.5.1 Outlet. The inlet and all bleed openings of the regulator shall be capped and a pressure of 25 inches of water shall be applied to the outlet of the regulator and maintained for 2 minutes. The regulator shall pass the requirements specified in 3.7.4.1.

4.8.5.2 Inlet. While maintaining a zero flow condition at ground level, a pressure of 150 psig shall be applied to the inlet of the regulator and shall be maintained for a minimum of 3 minutes. The regulator shall pass the requirements specified in 3.7.4.2.

4.8.6 Leakage.

4.8.6.1 Body leakage (outlet pressure). The inlet and all bleed openings of the regulator shall be capped and a pressure of 10 inches of water shall be applied to the outlet of the regulator for a period of 3 minutes. The regulator shall pass the requirements specified in 3.7.5.1.

4.8.6.2 Body leakage (inlet pressure). The inlet of the regulator shall be subjected to a pressure of 120 psig while maintaining a flow of 100 lpm at ground level. The regulator shall pass the requirements specified in 3.7.5.1.

4.8.6.3 Designed bleed flow. The inlet of the regulator shall be capped and a pressure of 25 inches of water shall be applied to the outlet of the regulator. The regulator shall pass the requirements specified in 3.7.5.2.

4.8.6.4 Demand valve leakage - outward. The inlet of the regulator shall be subjected to a pressure of 40 and 120 psig while maintaining zero flow conditions at ground level. After a five-minute period, the outlet pressure of the regulator shall be measured and shall pass the requirements specified in 3.7.5.3.

4.8.7 Extreme temperatures.

4.8.7.1 High temperature. The regulator shall be conditioned at a temperature of 160 ± 5°F (71° ± 3°C) for 3 hours. After conditioning and while still at this temperature, the regulator shall be subjected to the outlet pressure test, 4.8.2, and shall pass the requirements specified in 3.7.6.1. Upon completion of this test procedure, the regulator shall be returned to normal temperature conditions (4.7.2) and shall then be subjected to and pass the outlet pressure and leakage tests, 4.8.2 and 4.8.6.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the currentversion before use.

4.8.7.2 Low temperature. The regulator shall be conditioned at a temperature of -65 ± 5°F (-54° ± 3°C) for 3 hours. After conditioning and while still at this temperature, the regulator shall be subjected to the outlet pressure test, 4.8.2, and shall pass the requirements specified in 3.7.6.2. Upon completion of this test procedure, the regulator shall be returned to normal temperature conditions (4.7.2) and shall then be subjected to and pass the outlet pressure and leakage tests, 4.8.2 and 4.8.6.

4.8.8 Vibration. The regulator outlet shall be capped with an end cap containing a minute bleed hole to relieve the buildup of pressure. A pressure of 80 ± 10 psig shall be applied to the inlet of the regulator. The regulator shall be vibrated for a total of 9 hours (3 hours in each major axis) at a frequency of 500 to 2500 to 500 cycles at a sweep rate of 15 minutes, and a double amplitude of 0.018 to 0.020 inch. The regulator shall pass the requirements specified in 3.7.7. After vibration, the regulator shall be subjected to and pass the outlet pressure and leakage tests, 4.8.2 and 4.8.6.

4.8.9 Acceleration. A pressure of 80 psig shall be applied to the inlet of the regulator, and an acceleration force of 7g shall be applied to the regulator in six different directions. The force shall be applied in one direction at a time, and the forces shall be in the directions shown on Figure 5. A 100 lpm flow shall be maintained as the g force is increased to 7g in each direction. Prior to, during, and after the application of each acceleration force, the regulator shall pass the requirements specified in 3.7.8.

4.8.10 Endurance. The regulator shall be subjected to 250,000 breathing cycles of endurance testing at the cycles per minute, peak delivery rates, and number of cycles specified in Table III. The regulator shall then be subjected to and pass the outlet pressure and leakage tests, 4.8.2 and 4.8.6.

4.8.11 Altitude cycling. A pressure of 80 psig shall be applied to the inlet of the regulator and the regulator shall be exposed to simulated altitudes of ground level to 50,000 feet for a total of 50 cycles. One cycle shall constitute ground level to 50,000 feet to ground level. The ascent rate shall be 500 feet per second (ft./sec.) and the descent rate shall be 1000 ft./sec. The regulator shall pass the requirements specified in 3.7.10. The regulator shall then be subjected to and pass the outlet pressure and leakage tests, 4.8.2 and 4.8.6.

4.8.12 Shock. The regulator shall be subjected to the following shock testing. The height of the drop shall be 29.0 ± 1.0 inches. The regulator shall be released from a quick-release hook or drop tester. The floor or barrier receiving the impact shall be of two-inch plywood backed by concrete. The regulator shall be randomly dropped 10 times on various faces, edges, and corners. The regulator shall pass the requirements specified in 3.7.11. The regulator shall then be subjected to and pass the outlet pressure and leakage tests, 4.8.2 and 4.8.6.

4.8.13 Repeat of noise level control test. At the completion of the tests described in 4.8.7 through 4.8.12 the regulator shall be subjected to the noise level control test, 4.8.4, and shall pass the requirements specified in 3.7.12.

4.8.14 Underwater breathing capabilities. The regulator shall be connected to a hose conforming to drawing number 834-18, and the hose shall be connected to an MBU-14/P oxygen mask and fitted to a subject. The regulator shall be

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

positioned 2 inches to 4 inches below the subject's suprasternal notch. The inlet oxygen pressure shall be maintained at 50 psig. The subject shall be submerged under 16 feet of water, for a minimum of 3 minutes, in both the upright and inverted positions. Under these conditions, the regulator shall pass the requirements specified in 3.7.13.

4.8.15 Ozone resistance (elastomer components). The three elastomer test slabs submitted for qualification and first article inspection shall be tested for ozone resistance. The test apparatus shall be in accordance with ASTM D1149. The test slabs shall be elongated 20 percent, placed in an ozone-free atmosphere for 24 hours, then placed in the ozone chamber. The chamber shall be adjusted to 100 ± 2°F (38° ± 3°C) and to give an exposure of ozone concentration of 120 ± 10 parts by volume of ozone per million parts by volume of air. The air-ozone velocity in the chamber shall be at least 2 ft/sec. The material shall be exposed to these conditions for 60 minutes. The test slabs shall be examined under a 10X magnification and pass the requirements specified in 3.7.14.

4.8.16 Oxygen regulator purge. The regulator inlet shall be connected to a regulated source of oxygen (4.7.1). An inlet pressure of 120 psig shall be applied and the regulator shall free flow for 1 to 3 minutes. The regulator shall pass the requirements specified in 3.7.15.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C, as specified (see 6.2).

5.1.1 Level A. Each breathing regulator shall be preserved in accordance with MIL-P-116, method IC-4. No contact preservation is required. Each breathing regulator shall be sealed within a snug fitting bag of 0.0015 inch gage material conforming to MIL-B-22191, Type III. The sealed breathing egulator shall be cushioned and packaged within a waterproof fiber can with sealed metal ends. The breathing regulator shall be cushioned in such a manner as to prevent damage to itself. Ten unit packages shall be packaged within a fiberboard container conforming to PPP-B-636, Type I, Class 2, Grade 3. The manufacturer's seam shall be adhesive sealed. All seams and joints shall be sealed with tape conforming to PPP-T-60.

5.1.2 Level C. The breathing regulator shall be packaged to afford the minimum degree of protection necessary to prevent deterioration or damage during shipment under normal environmental conditions and commercial modes of transportation.

5.2 Packing. Packing shall be level A, B, or C, as specified (see 6.2.1e).

5.2.1 Level A. One hundred breathing regulators, packaged as specified in 5.1.1, shall be packed in overseas type exterior containers conforming to PPP-B-601, PPP-B-621, PPP-B-591, PPP-B-636, or PPP-B-640, Class 2. Packages for Southeast Asia shall be packed in PPP-B-621 boxes, constructed from wood which has been sprayed with a solution of 2 percent copper naphthenate in mineral spirits. Closure and strapping of the containers shall be in accordance with the applicable container specification or appendix thereto. The gross weight of the packed shipping container shall not exceed the weight limitations of the applicable container specification.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. One hundred breathing regulators, packaged as specified in 5.1.1, shall be packed in domestic type exterior containers conforming to PPP-B-601, PPP-B-621, PPP-B-591, PPP-B-636, or PPP-B-640, Class 1. Closure and strapping of the containers shall be in accordance with the applicable container specification or appendix thereto. The gross weight of the packed shipping container shall not exceed the weight limitations of the applicable container specification.

5.2.3 Level C. The packaged breathing regulators, which the carrier requires to be packed, shall be packed within exterior type shipping containers in a manner that shall ensure safe transportation at the lowest rate to the point of delivery. The shipment shall conform to the minimum requirements of the rules and regulations applicable to the mode of transportation selected.

5.3 Marking. Nomenclature tags shall be inserted in each bag showing title, part number or other data as required by acquiring activity. In addition, interior and exterior containers shall be marked in accordance with MIL-STD-129.

5.3.1 Precautionary marking. The following precautionary marking shall appear on each package:

"CAUTION: DO NOT ALLOW CONTAMINANTS OF ANY KIND TO BE USED ON OR ABOUT THE OXYGEN REGULATORS."

6. NOTES

(This section contains information of a general or explanatory nature that may be helpful, but is not mandatory.)

6.1 Intended use. The regulator covered by this specification is intended for use in supplying breathing oxygen.

6.2 Acquisition requirements. Acquisition documents must specify the following:

a. Title, number and date of this specification.

b. Applicable QPL, Government designation and manufacturer designation required.

c. Issue of DODISS to be cited in the solicitation, and if required, specific issue of individual documents referenced (see 2.1.1 and 2.2).

d. Whether first article inspection is required (see 3.2 and 4.4.2).

e. Name and address of the first article inspection facility and the name and address of the Government activity responsible for conducting the first article inspection program (see 4.4.2 and 4.4.2.1).

f. Selection of applicable levels of preservation, packaging and packing required (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the currentversion before use.

g. Name and address of the quality conformance verification inspection facility and the name and address of the Government activity responsible for conducting the quality conformance verification inspection program (see 4.6 and 6.5).

h. Items of data required (see 6.2.1).

6.2.1 Consideration of data requirements. The following data requirements should be considered when this specification is applied on a contract. The applicable Data Item Descriptions (DID's) should be reviewed in conjunction with the specific acquisition to ensure that only essential data are requested/provided and that the DID's are tailored to reflect the requirements of the specific acquisition. To ensure correct contractual application of the data requirements, a Contract Data Requirements List (DD Form 1423) Must be prepared to obtain the data, except where DOD FAR Supplement 27-4,75-1 exempts the requirement for a DD Form 1423.

Reference Para.	DID Number	DID Title	Suggested Tailoring
4.4.2.1	NDTI-80809A	Test/Inspection Report	

The above DID's were those cleared as of the date of this specification. The current issue of DOD 5010.12-L, Acquisition Management Systems and Data Requirements Control List (AMSDL), must be researched to ensure that only current, cleared DID's are cited on the DD Form 1423.

6.3 Qualification. With respect to products requiring qualification, awards will be made only for products which are, at the time of award of contract, qualified for inclusion in the applicable Qualified Products List (QPL-81553) not such products have actually been so listed by that date. The attention of the contractors is called to these requirements, and manufacturers are urged to arrange to have the products that they propose to offer to the Federal Government tested for qualification in order that they may be eligible to be awarded contracts or purchase orders for the products covered by this specification. The activity responsible for the Qualified Products List is the Commander, Naval Air Systems Command, Department of the Navy, Washington, DC 20361; however, authorization for qualification of products may be obtained from the Commander, Naval Air Warfare Center Aircraft Division Warminster, (Code 6031), Warminster, PA 18974-5000.

6.3.1 Drawings. When requested, the manufacturer shall submit engineering drawings and inspection reports in accordance with SD-6 (see 4.3.1).

6.4 First article. When a first article inspection is required, the item will be tested and should be a first article sample. The contracting officer should include specific instructions in acquisition documents regarding arrangements for examinations, test and approval of the first article.

6.5 Laboratory information. The successful bidder will be furnished with the name of the quality conformance verification inspection laboratory and the Government activity responsible for conducting the inspection program at the time of award. The costs of the tests and examinations on samples initially submitted from a lot, as required by 4.6, shall be borne by the Government whether the test and examinations are conducted by a Government laboratory or by a laboratory selected by the cognizant Government activity. Samples from a rejected lot shall

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the currentversion before use.

not be resubmitted for tests and examinations, as required by 4.6, without the approval of the contracting officer. The costs of the tests and examinations on samples resubmitted from a reworked lot or from a new lot which is necessitated by the rejection of a previous lot shall be borne by the contractor whether the tests and examinations are conducted by a Government laboratory or by a laboratory selected by the cognizant Government activity.

6.6 Changes from previous issue. Marginal notations are not used in this revision to identify changes with respect to the previous issue due to the extensiveness of the changes.

6.7 Subject term (keyword) listings.

Altitude operation
Breathing gas
Oxygen system
Pressure breathing
Sea level operation

Preparing activity:
Navy - AS
(Project No. 1660-N626)

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

TABLE I. Outlet pressures (steady state) (see 4.8.2).

Altitude (feet)	Inlet supply pressure (psig)	Outlet pressure @ 0.0 lpm flow (in. H2O)	Outlet pressure @ 50.0 lpm flow (in. H2O)	Outlet pressure @ 100.0 lpm flow (in. H2O)
Ground level	40, 80, 120	0.5 to 2.5	0.5 to 2.5	1.0 to 2.5
10,000	40, 80, 120	0.5 to 2.5	0.5 to 2.5	1.0 to 2.5
30,000	40, 80, 120	0.5 to 2.5	0.5 to 2.5	1.0 to 2.5
34,000	40, 80, 120	1.0 to 3.7	1.0 to 3.7	1.0 to 3.7
40,000	40, 80, 120	8.0 to 10.5	8.0 to 10.5	8.0 to 10.5
45,000	40, 80, 120	13.0 to 16.0	13.0 to 16.0	13.0 to 16.0
50,000	40, 80, 120	16.0 to 20.0	16.0 to 20.0	16.0 to 20.0

TABLE II. Outlet pressures (dynamic) (see 4.8.3) 1/.

Tidal Volume (L)	Inlet Pressure	Flow Rate (Liters/Min, NTP 2/)		Cycling Rate 3/ Cycles/Minute	Oxygen Regulator (Inch/H_2O)
		Average	Peak		
2.0	40	15.9	50	8.0	0.5 to + 2.5
2.0	40	31.8	100	15.9	1.0 to + 2.5
2.0	50	47.8	150	23.9	1.0 to + 3.0
2.0	60	57.3	180	28.7	1.5 to 5.0
2.0	70	63.7	200	31.8	2.0 to 6.0

1/ This test shall be run for a period of 10 minutes at each inlet pressure.

2/ 70°F, 14.7 psia

3/ A complete cycle includes the flow period during breathing simulator inhalation and the no flow period during breathing simulator exhalation.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the current version before use.

TABLE III. Endurance (see 4.8.10) 1/.

Number of Cycles	Flow Rate (Liters/Min, NTP 2/)		Cycling Rate 3/
	Average	Peak	Cycles/Min
25,000	57.3	180	28.7
50,000	15.9	50	8.0
175,000	31.8	100	15.9

1/ This test shall be run for a total of 250,000 cycles.

2/ 70°F, 14.7 psia

3/ A complete cycle includes the flow period during breathing simulator inhalation and the no flow period during breathing simulator exhalation.

TABLE IV. Noise level (see 4.8.4).

1/3 Octave Band Center Frequency	dB (Referred To) 0.0002 dynes/cm^2
315	95 max
400	95 max
500	95 max
630	95 max
800	95 max
1000	95 max
1250	95 max
1600	95 max
2000	95 max
2500	95 max
3150	95 max
4000	95 max
5000	95 max
6300	95 max

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

TABLE V. Qualification inspection (see 4.3).

Inspection	Requirement Paragraph	Paragraph Test Method	Sample Number
Visual examination	-	4.8.1	Every Regulator
Overload	3.7.4	4.8.5	Every Regulator
Leakage	3.7.5	4.8.6	Every Regulator
Outlet pressures (steady state)	3.7.1	4.8.2	Every Regulator
Outlet pressures (dynamic)	3.7.2	4.8.3	Every Regulator
Noise level control	3.7.3	4.8.4	Every Regulator
High temperature	3.7.6.1	4.8.7.1	1,2
Low temperature	3.7.6.2	4.8.7.2	1,2
Vibration	3.7.7	4.8.8	3,4
Acceleration	3.7.8	4.8.9	3,4
Endurance	3.7.9	4.8.10	1
Altitude cycling	3.7.10	4.8.11	3,4
Shock	3.7.11	4.8.12	3,4
Repeat of noise level control	3.7.12	4.8.13	Every Regulator
Underwater breathing capabilities	3.7.13	4.8.14	2
Ozone resistance (elastomer components)	3.7.14	4.8.15	-

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the currenversion before use.

TABLE VI. First article inspection (see 4.4).

Inspection	Requirement Paragraph	Test Method Paragraph
Visual examination	-	4.8.1
Overload	3.7.4	4.8.5
Leakage	3.7.5	4.8.6
Outlet pressures (steady state)	3.7.1	4.8.2
Leakage	3.7.5	4.8.6
Altitude cycling	3.7.10	4.8.11
Noise level control	3.7.3	4.8.4
Outlet pressures (dynamic)	3.7.2	4.8.3
Ozone resistance (elastomer components)	3.7.14	4.8.15

TABLE VII. Criteria for quality conformance inspection (see 4.5.).

Inspection 1/	Requirement Para.	Test Method Para.	Sample Size	Acceptance Criteria 2/
Visual	-	4.8.1.1	Every regulator for critical defects. Inspection Level II for minor defects	Reject all units with any critical defects. An AQL of 2.5 defects per 100 units for minor defects.
Overload	3.7.4	4.8.5	Every regulator	Reject all defective units.
Leakage	3.7.5	4.8.6	Every regulator	Reject all defective units.
Outlet Pressures (Steady State)	3.7.1	4.8.2	Every regulator	Reject all defective units.
Noise level control	3.7.3	4.8.4	Every regulator	Reject all defective units.
Packaging	-	4.8.1.2	Inspection level S-2	An acceptable quality level of 4.0 defects per hundred units.

1/ The results of all inspections shall be identifiable by the assigned serial numbers (see 3.12.1).

2/ The sample size and acceptance criteria shall be in accordance with MIL-STD-105.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:35Z
Check the source to verify that this is the current version before use.

TABLE VIII. Criteria for Quality Conformance Verification Inspection (see 4.6).

Inspection	Requirement Paragraph	Test Method Paragraph	Sample Size
Visual	-	4.8.1.1	Every Regulator
Overload	3.7.4	4.8.5	Every Regulator
Leakage	3.7.5	4.8.6	Every Regulator
Outlet pressure (steady state)	3.7.1	4.8.2	Every regulator
Noise Level Control	3.7.3	4.8.4	Every Regulator

TABLE IX. Classification of defects for visual examination of the regulator (see 4.8.1.1).

CRITICAL
1. Material imperfections - foreign matter embedded.
2. Surface - unclean, rough, misaligned, or containing cracks, nicks, or other flaws.
3. Any component missing, malformed, fractured, or otherwise damaged.
4. Gaps between surfaces that should be sealed.
5. Any component loose or otherwise not securely retained.
6. Gasket or seal improperly positioned or unevenly compressed.
7. Incorrect assembling or improper positioning of components.
8. Any functioning part that works with difficulty.
9. Faulty workmanship or other irregularities.
10. Evidence of adhesives other than to secure labels.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the currentversion before use.


TABLE IX. Classification of defects for visual examination of the regulator (see 4.8.1.1). (Continued)

CRITICAL
11. Marking - missing, insufficient, incorrect, illegible, or not permanent.
12. Evidence of excessive use of lubricants.
13. Missing inlet/outlet caps or plugs
MINOR
1. Color not as specified.

TABLE X. List of defects for packaging (see 4.8.1.2).

Item	Defects
Exterior and interior markings	Missing, incorrect, incomplete, illegible; of improper size, location, sequence; method of application; markings not the same on the interior and exterior containers.
Packaging and packing materials	Any nonconforming component; any component missing, damaged, or otherwise defective.
Workmanship	Inadequate application of the components such as incomplete closure of the unit package, intermediate package, case liners, container flaps, loose strappings, etc.; bulging or distortion of the containers.
Exterior and interior weight or content	Number per container is more or less than required; gross or net weight exceeds the requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

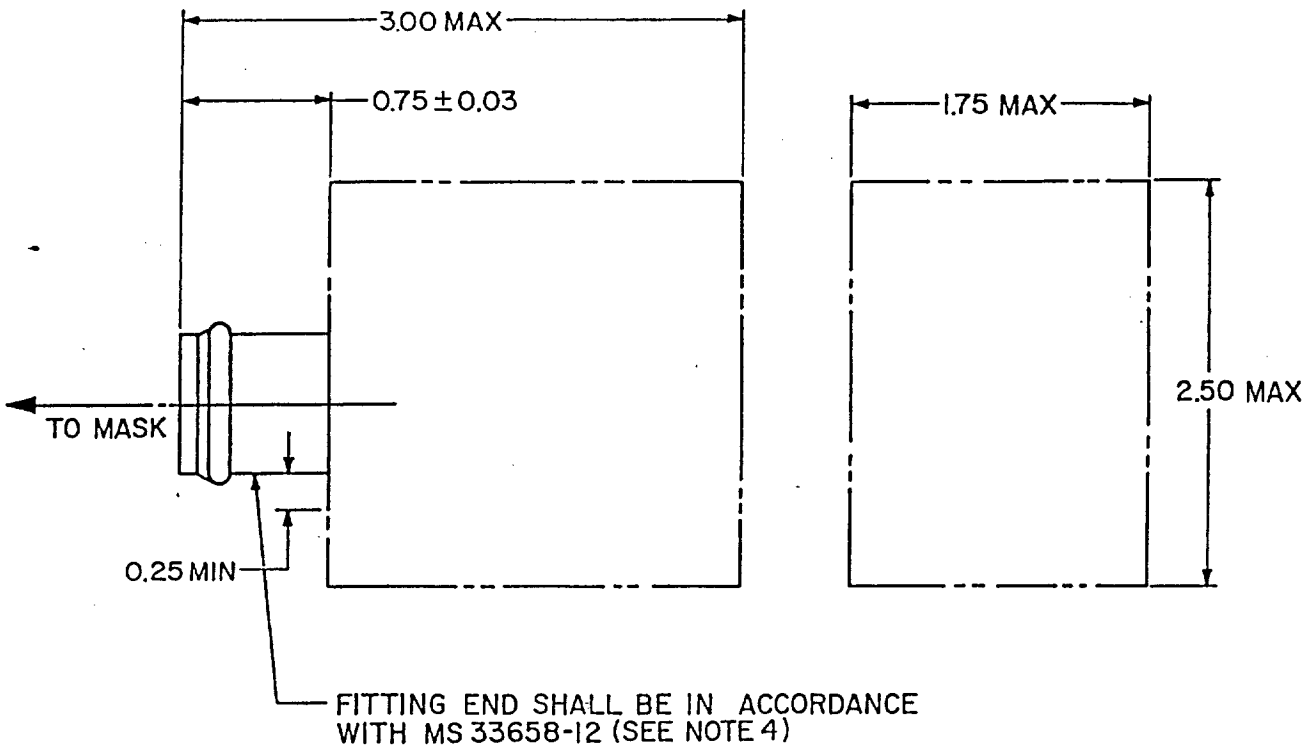

DIMENSIONS IN INCHES

NOTES:

1. THE INLET SHALL NOT BE LOCATED ON THE SAME SIDE AS THE OUTLET.
2. THE INLET OF THE REGULATOR SHALL HAVE FEMALE THREADS AND MATE WITH A 1/8 - 27 ANPT INLET FITTING FOR 40 - 120 PSIG OXYGEN.
3. ANPT SHALL BE IN ACCORDANCE WITH MIL-P-7105.
4. ENVELOPE DIMENSIONS INCLUDE ALL HOSE CONNECTING PARTS.
5. INTERNAL DIMENSION NOT APPLICABLE.

FIGURE 1. Chest mounted regulator (envelope dimensions.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:35Z
Check the source to verify that this is the currenversion before use.


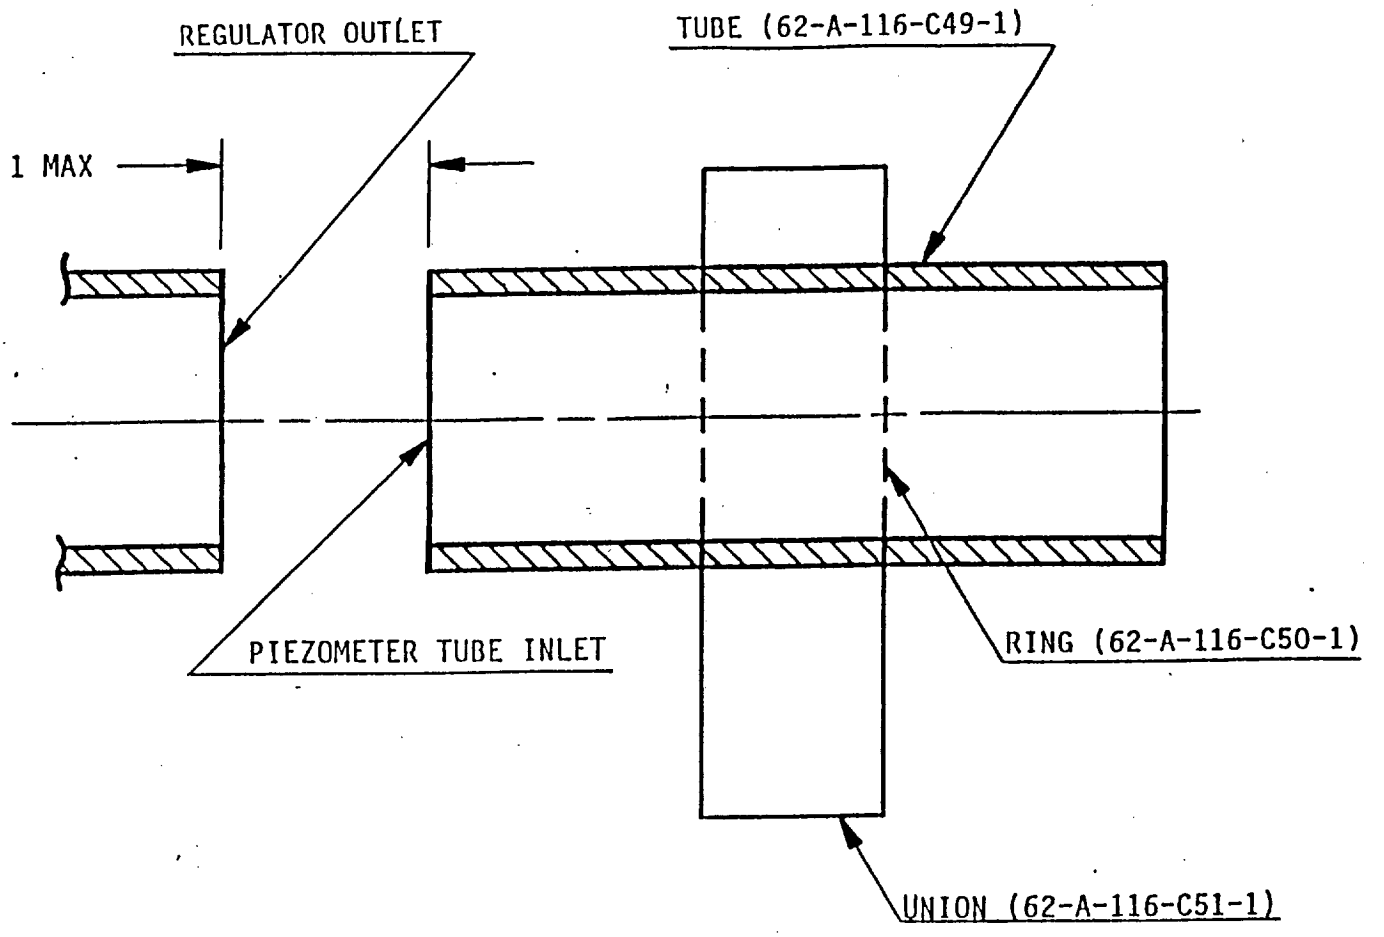


FIGURE 2. Location of regulator outlet of piezometer (62-A-116-C48)

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the currentversion before use.

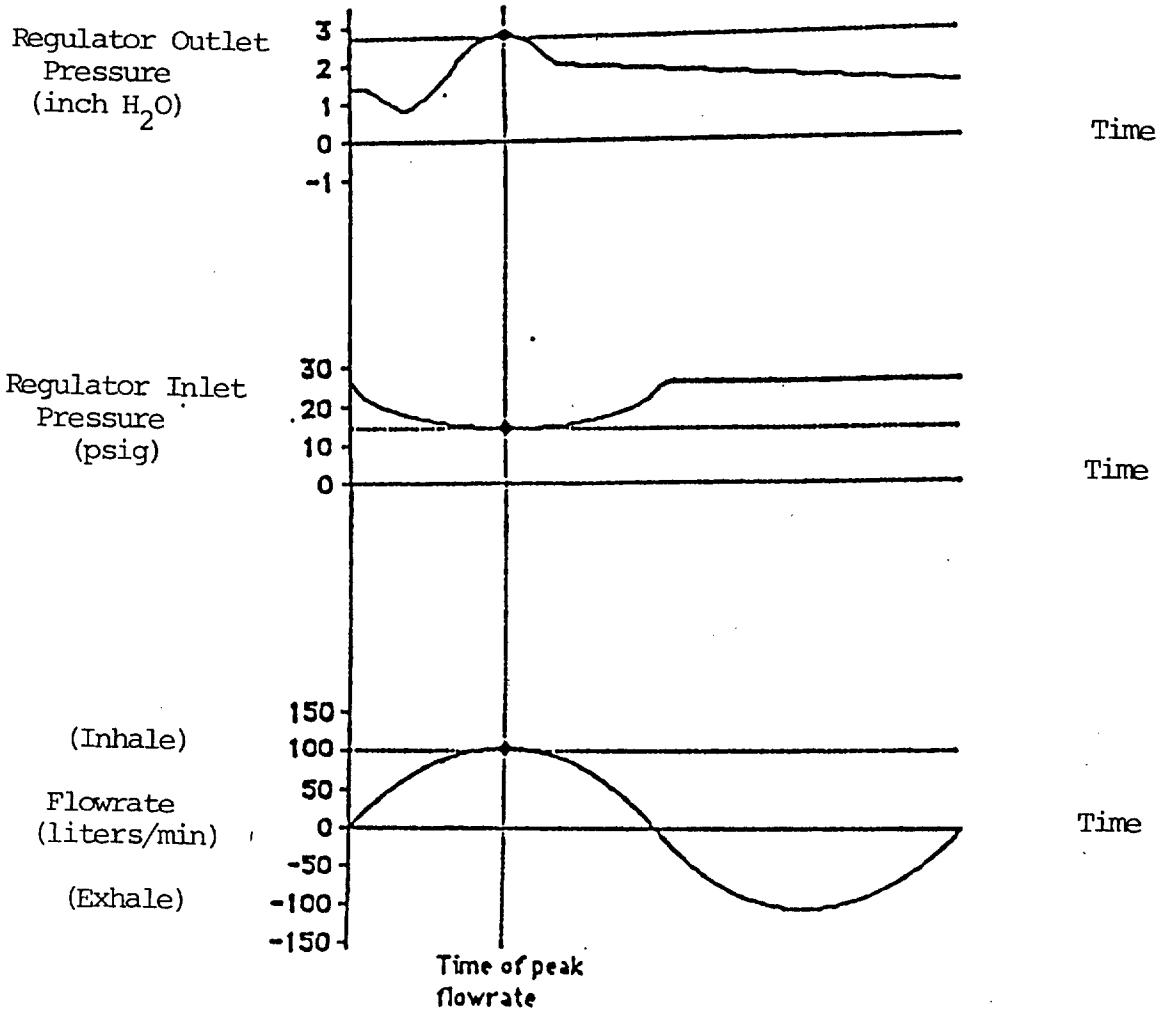

NOTES:

1. MINIMUM REGULATOR INLET PRESSURE SHALL BE SET TO +2 / -0 PSID OF THE SPECIFIED VALUE AT THE TIME OF PEAK FLOWRATE.
2. REGULATOR OUTLET SHALL BE RECORDED AT THE TIME OF PEAK FLOWRATE.

FIGURE 3. Dynamic test measurements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.


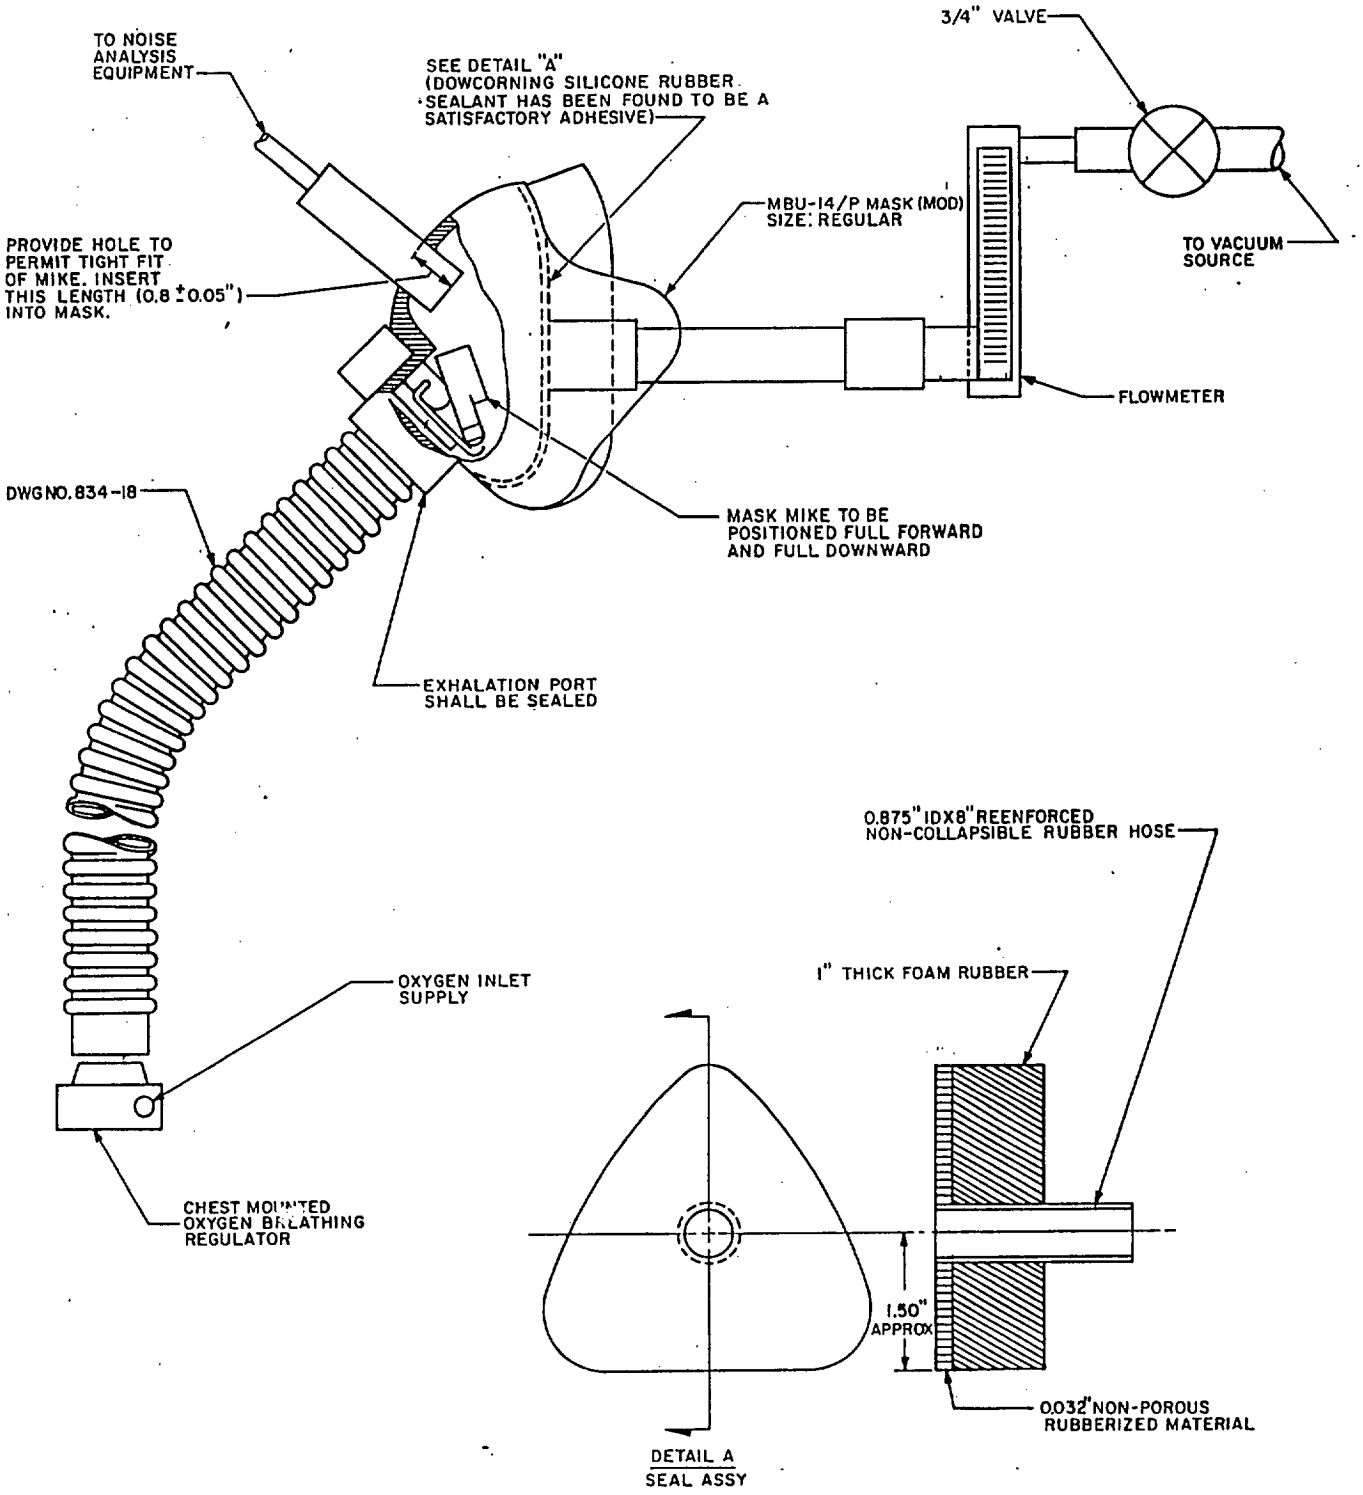


Figure 4. Noise level control test set-up.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:35Z
Check the source to verify that this is the current version before use.

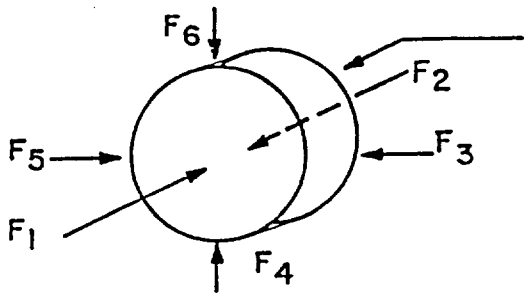

NOTE:

1. F_1 AND F_2 ARE PERPENDICULAR TO THE PLANE OF THE DEMAND DIAPHRAGM. F_3, F_4, F_5 AND F_6 ARE PARALLEL TO THE PLANE OF THE DEMAND DIAPHRAGM.

FIGURE 5. Direction of applied forces.

Source: https://assist.dla.mil - Downloaded: 2026-10-26T04:35Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	MIL-R-81553B(AS)	92/09/17

3. DOCUMENT TITLE
REGULATOR, CHEST MOUNTED, OXYGEN, POSITIVE PRESSURE, CRU-79/P

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME COMMANDING OFFICER, NAVAL AIR WARFARE CENTER AIRCRAFT DIVISION LAKEHURST SYSTEMS REQUIREMENTS DEPARTMENT	b. TELEPHONE (Include Area Code) (1) Commercial: (908) 323-7488 (2) AUTOVON: 624-7488
c. ADDRESS (Include Zip Code) CODE SR3 LAKEHURST, NJ 08733-5100	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

Source: https://assist.dla.mil -- Downloaded: 2025-Jan-26 10:04 EST
Check the source to verify that this is the current version before use.