A-A-51756A
15 August 1988
SUPERSEDING
A-A-0051756(DM)
1 December 1986

COMMERCIAL ITEM DESCRIPTION

GUIDE, ANGLE (Adjustable)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an adjustable angle guide used for determining and stabilizing the proper angle of pin insertion during hip nailing and plating surgical procedures.

Salient characteristics:

Style and design. Style and design shall be in accordance with Figure 1.

Components. Components of the angle guide shall be in accordance with the following:

Handle. The handle shall be between 2.75 and 5 inches in length. Diameter of the handle shall be 0.75 inch (nominal) and shall be fully cannulated to accept guide pins up to 3/32 inch in diameter. The handle shall be able to be removed from body of angle guide for cleaning purposes. The handle shall be knurled along its length for a minimum of 2 inches, adjustable, and able to be secured at any angle on the 90 to 180 degree scale so as to provide stabilization of the angle for pin insertion.

Indicator. Indicator shall be at base of handle and shall clearly indicate the angle on the scale.

Angle scale. Angle scale shall be easily visible and permanent and shall range from 90 to 180 degrees. The 180 degree line shall be parallel to shaft of guide.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Shaft. Shaft shall be of one-piece construction or shall be permanently secured to the angle scale proper and shall have a length of 2.5 ± .5 inches. Width shall be .62 ± .13 inch. Thickness shall be .19 ± .06 inch. Shaft may include a screw hole to allow for temporary fixation of shaft to femur.

Material. Angle guide shall be fabricated of Class 3 austenitic corrosion resistant steel in accordance with ASTM Designation F899. The angle guide shall have a Rockwell Hardness B Scale (HRB) 90, minimum. Instrument components shall be properly passivated.

Sterilization. The angle guide shall be capable of withstanding repeated sterilization via steam, ethylene oxide, or long-term, 10 hour soaking in cold sterilization solution. The hand drill shall show no evidence of corrosion when autoclaved as follows:

The guide shall be cleaned and placed in an autoclave. The guide shall then be autoclaved at 270 ± 5 degrees F and 27 ± 1 psi for a minimum of 20 minutes. Upon removal of guide from autoclave, the entire surface area of the guide shall be examined for evidence of corrosion.

Workmanship. The angle guide shall be free from defects which detract from its appearance or impair its serviceability.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One angle guide, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The acceptable quality level (AQL) shall be 1.0 for an inspection level of S-2. The unit of product for test purposes shall be one angle guide.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8026	GUIDE, ANGLE, Adjustable 90° to 180° Scale, 5 Inch (12.7 cm) Long

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4282

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

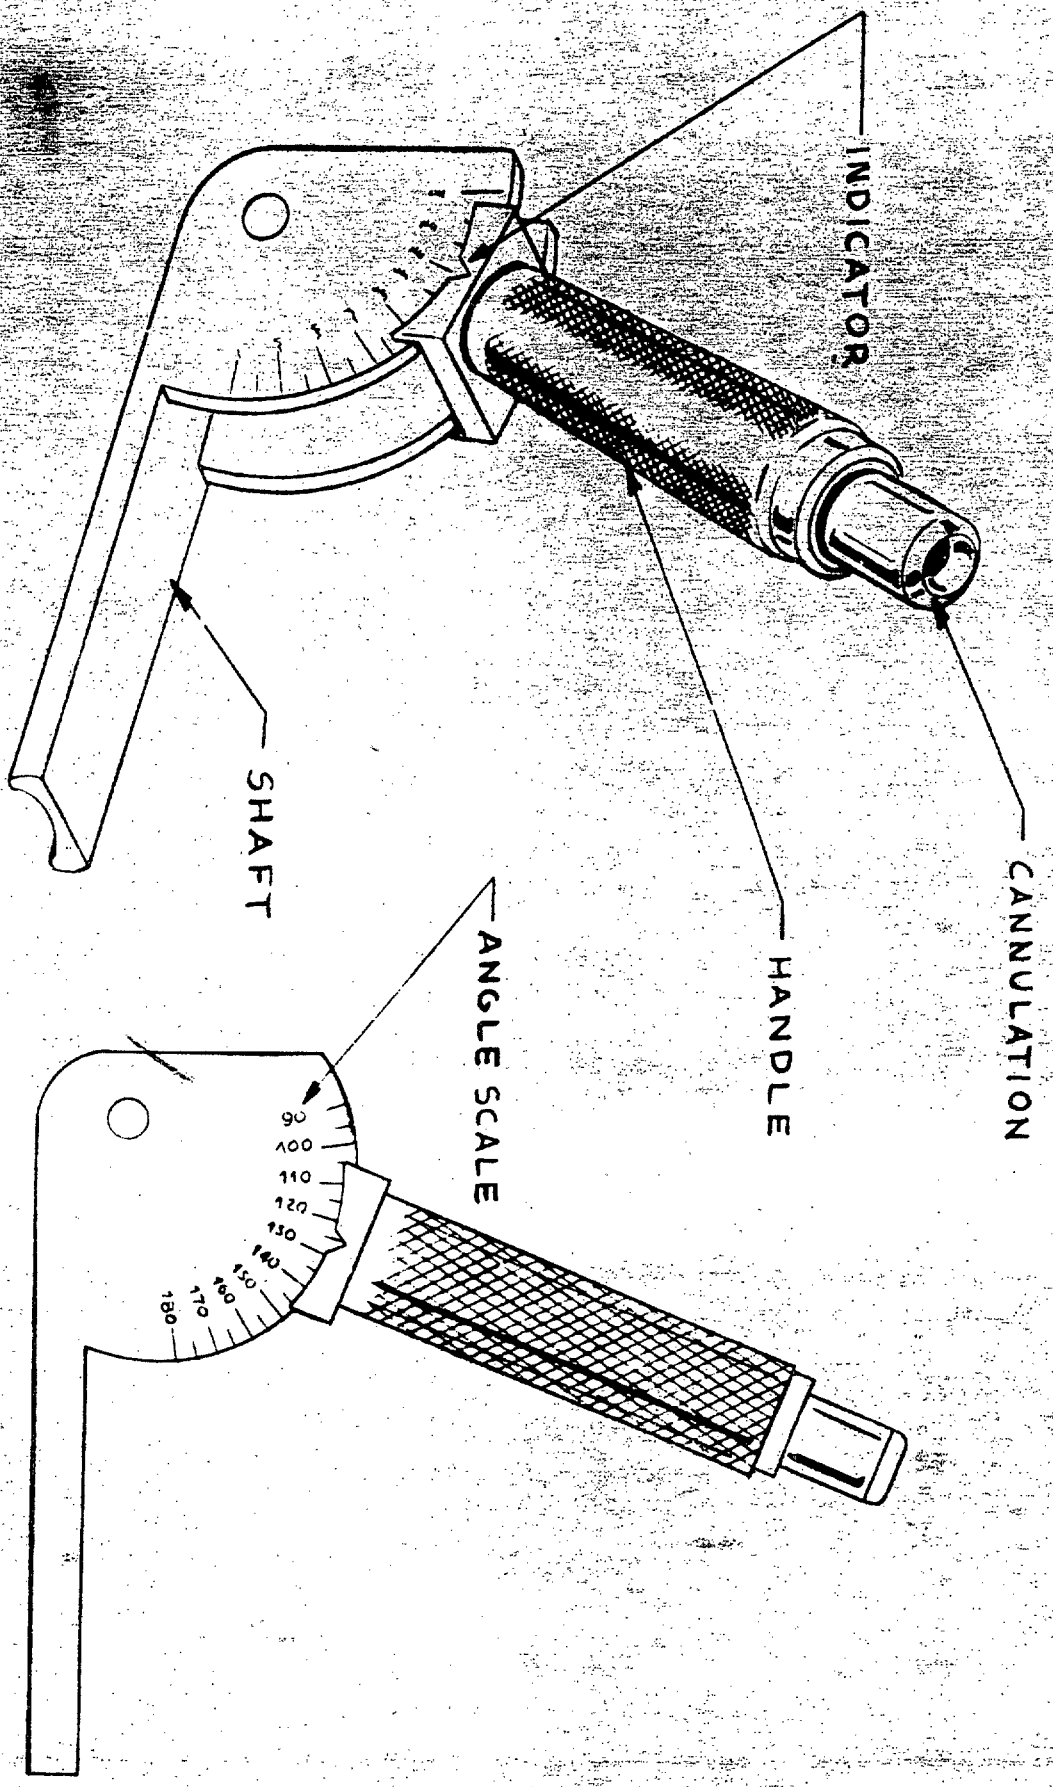


FIGURE 1. GUIDE, ANGLE, ADJUSTABLE 90° TO 180° SCALE

NOTE: FOR STYLE AND DESIGN PURPOSES ONLY.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.