# COMMERCIAL ITEM DESCRIPTION

## STAPLER, SURGICAL (INTRALUMINAL)

The General Services Administration has approved the use of this commercial item description.

This commercial item description covers an intraluminal surgical stapler suitable for use in colo-rectal, intestinal, and esophageal surgery.

Salient characteristics:

Style and design. Style and design of the stapler shall be in accordance with Figures 1,2 and 3. The stapler shall consist of a center-rod assembly and instrument-body assembly.

The center-rod assembly shall contain all of the moving parts of the stapler, except for the bayonet-sleeve mechanism. The instrument body assembly shall contain of all stationary stapler parts, bayonet-sleeve mechanism, and moveable handle. The design of the moveable handle and its pivot screw shall permit the user to remove and attach the handle without loss of pivot screw. Stapler design shall permit disassembly, cleaning and re-assembly.

Materials. The stapler shall be fabricated from suitable corrosion-resistant steels that conform to ASTM Designation F899.

Performance. The stapler shall perform the following functions:

1) The safety latch shall prevent stapler operation until manually unlocked.

2) The drive shaft shall advance when the user turns the wing nut counterclockwise. The drive shaft shall retract when the user turns the wing nut clockwise.

3) The drive tube shall advance when the user gives a firm squeeze on the instrument handles. The drive tube shall retract when the user releases the handle.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

4) The bayonet-sleeve mechanism shall accept a compatible staple-unit cartridge and lock it in place when the user gives the bayonet-sleeve a 1/8 turn clockwise. It shall stay in position until manually unlocked by the user.

5) When loaded with a compatible staple unit, the stapler shall effect a circular anastomosis on the tissues to be joined and resect all excess tissues from the joint provided the user has followed the instruction manual.

Workmanship. The surgical stapler shall be free from any defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One surgical stapler, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at level S-2, AQL 1.0%. The unit of product shall be one stapler.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers is covered by this document:

| NSN | Item Identification |
|---|---|
| 6515-01-205-2379 | STAPLER, SURGICIAL, INTRALUMINAL |

NOTE: The following are compatible with the stapler covered by this document:

| NSN | Item Identification |
|---|---|
| 6515-01-151-1835 | STAPLE UNIT, SURGICAL, Intraluminal 31.6 mm, Disposable, 12s |



Source: https://assist.dla.mil -- Downloaded: 202640-26T09:20Z
Check the source to verify that this is the current version before use.

| | |
|---|---|
| 6515-01-151-1836 | STAPLE UNIT, SURGICAL, Intraluminal, 28.6 mm, Disposable, 12s. |
| 6515-01-151-1837 | STAPLE UNIT, SURGICAL, Intraluminal, 25 mm, Disposable, 12s. |

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPOAS

Project No. 6515-4133



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

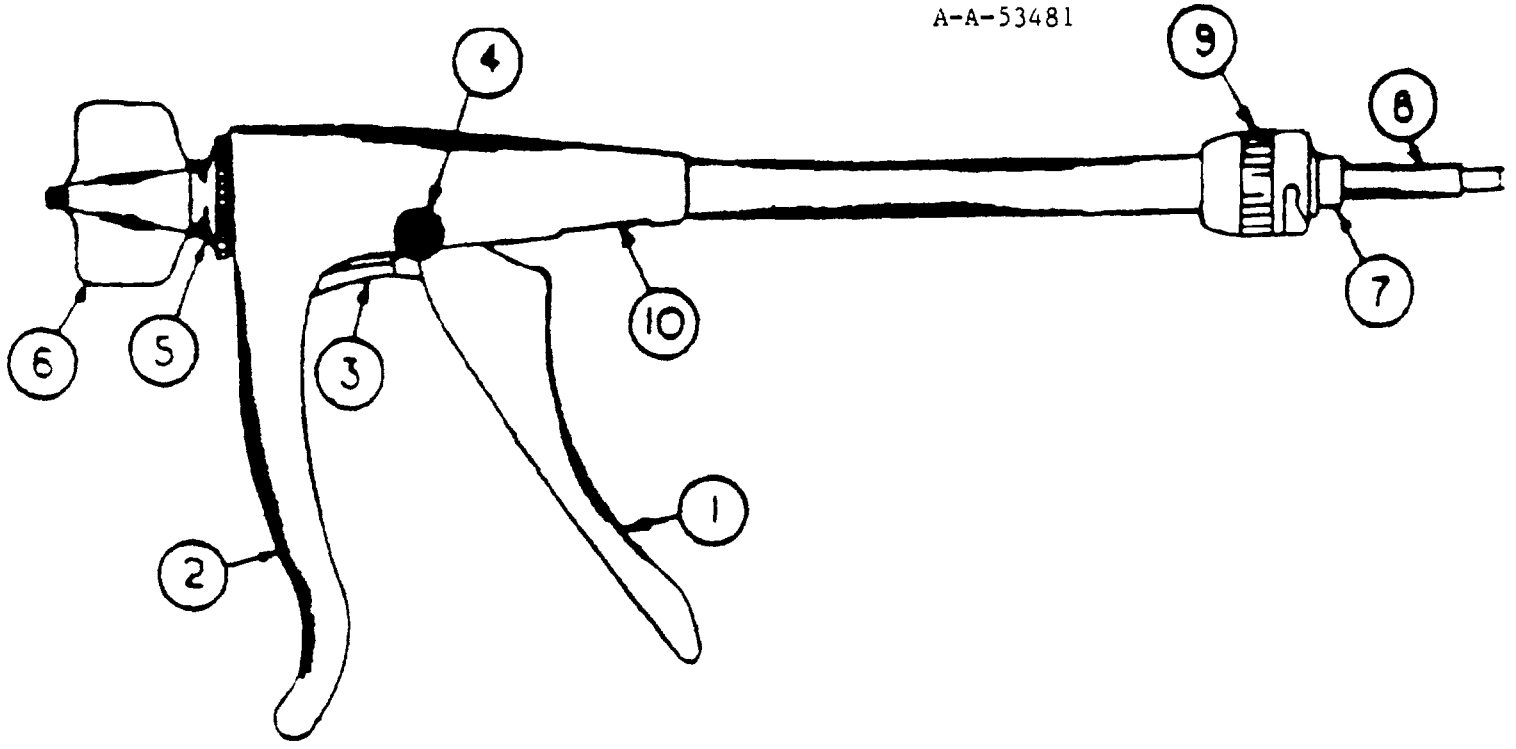



FIGURE 1
STAPLER, SURGICAL, INTRALUMINAL

1) Movable Handle
2) Fixed Handle
3) Safety Latch
4) Pivot Screw
5) Mounting Collar
6) Wing Nut
7) Drive Tube
8) Drive Shaft
9) Bayonet-Sleeve Mechanism
(See Figure 3)
10) Viewing Window
(See Figure 2)



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

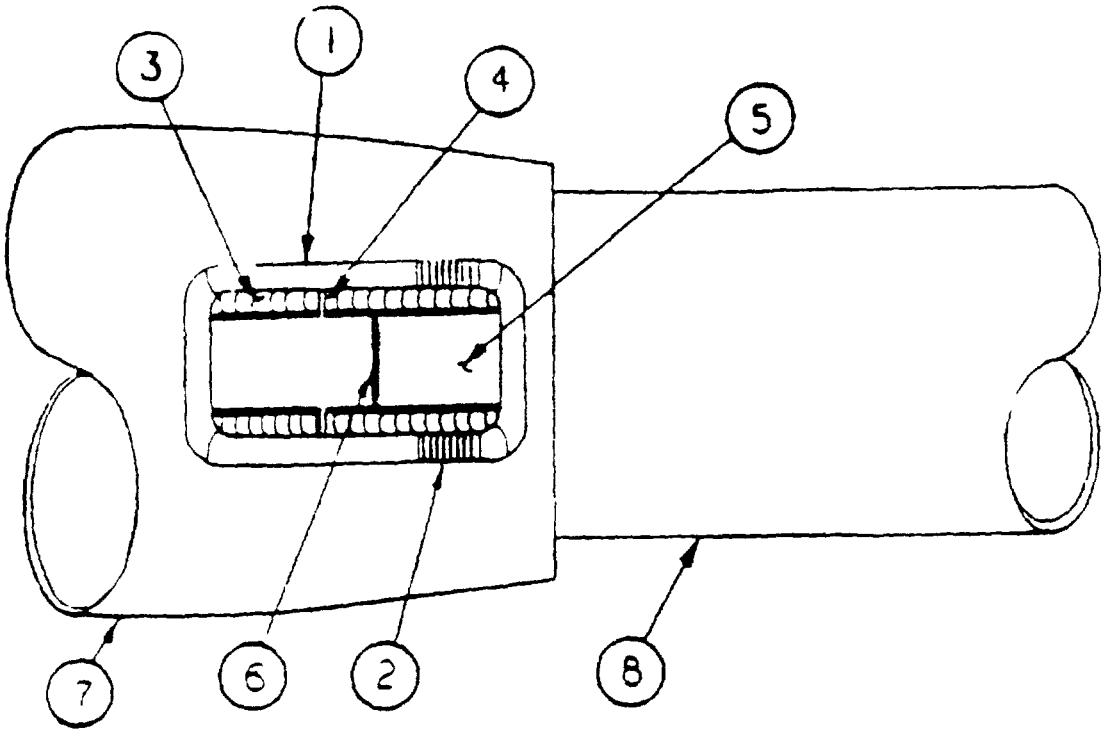



FIGURE 2
VIEWING WINDOW, SURGICAL STAPLER

1) View Port
2) Wide Alignment Marks
3) Drive Tube
4) Alignment Notches
5) Drive Shaft
6) Narrow Alignment Mark
7) Instrument Body Housing
8) Body Tube



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

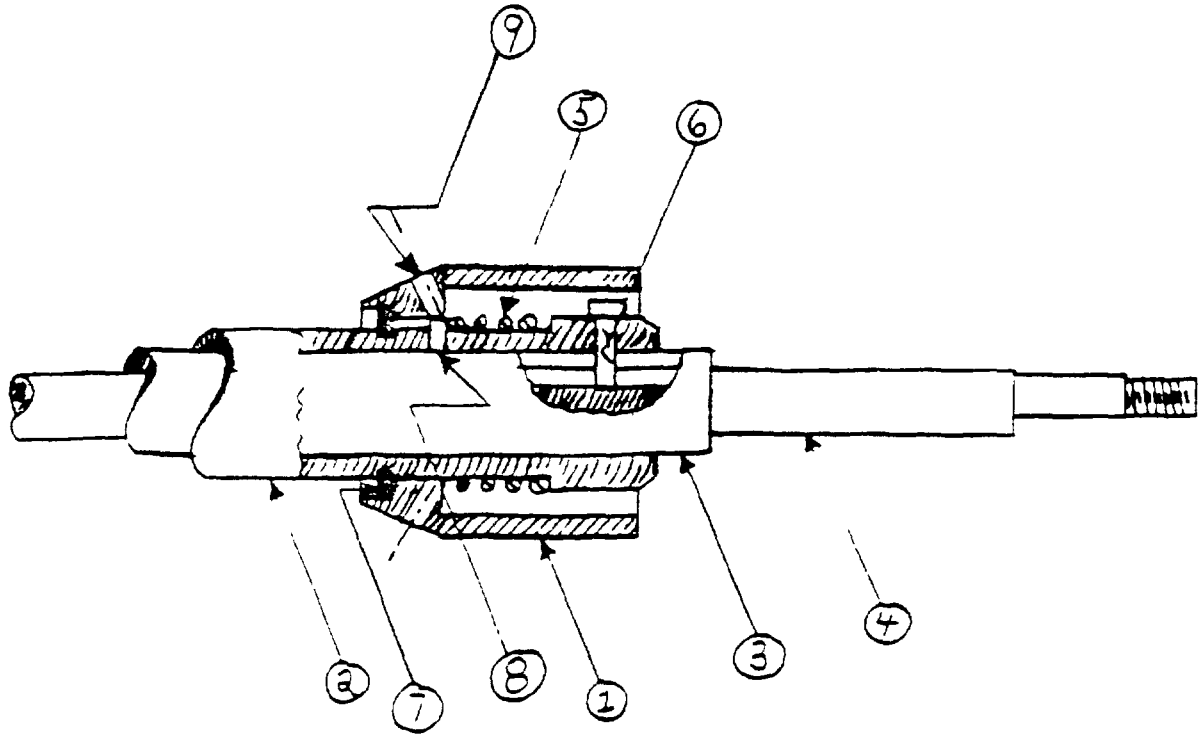



FIGURE 3
BAYONET-SLEEVE MECHANISM.

1) Bayonet-Sleeve
2) Body Tube
3) Drive Tube
4) Drive Shaft
5) Retaining Spring
6) Cartridge Key
7) Snap Ring
8) Retaining Pin
9) Vent (Typical)



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS** In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

*NOTE* This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

*(Fold along this line)*

*(Fold along this line)*

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions – Reverse Side)*

| 1 DOCUMENT NUMBER | 2 DOCUMENT TITLE |
|---|---|
| A-A-53481 | STAPLER, SURGICAL (NTRALUMINAL) |

| 3a NAME OF SUBMITTING ORGANIZATION | 4 TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR |
| b ADDRESS *(Street City State ZIP Code)* | ☐ USER |
| | ☐ MANUFACTURER |
| | ☐ OTHER *(Specify)* |

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason Rationale for Recommendation

6 REMARKS

| 7a NAME OF SUBMITTER *Last First MI* – Optional | b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional |
|---|---|
| c MAILING ADDRESS *(Street City State ZIP Code)* – Optional | 8 DATE OF SUBMISSION *(YYMMDD)* |

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:20Z
Check the source to verify that this is the current version before use.

DD FORM 1426 PREVIOUS EDITION