A-A-53482
31 May 1988

COMMERCIAL ITEM DESCRIPTION

STAPLE UNIT, SURGICAL (Gastro-intestinal)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one type of sterile, disposable, gastro-intestinal staple unit suitable for use in various surgical procedures.

Salient characteristics:

Style and design. Style and design of staple unit shall conform to Figure 1. Staple units shall consist of staple cartridge, push-bar/knife assembly, handle, alignment tabs, tip, and locking tabs.

The staple cartridge shall contain fifty-two (52) staple channels arranged in two (2) parallel, double-staggered rows. The minimum distance between the rows shall be 3.5 mm. Each staple channel shall be loaded with a surgical staple.

The push-bar/knife assembly shall contain a push-bar mechanism and a central knife blade. The knife blade shall be able to move down the center of the cartridge, between the two double-staggered rows of staple channels. The push-bar mechanism shall be suitable for driving the staples towards the anvil of the compatible surgical stapler. The proximal end of the mechanism and the knife-blade shall be permanently attached to the handle.

The tip of the staple unit shall act as a stop for the knife-blade. The alignment tabs shall ensure proper orientation between the staple unit and the cartridge half of the compatible stapler. The locking tabs shall secure the staple unit to the stapler until manually removed.

Dimensions. Dimensions of the surgical staples shall be as follows: 3.85 ± 0.005 mm leg length, 3.0 ± 0.05 mm width, 0.20 ± 0.005 mm wire diameter. The length of the staple pattern shall be 53 ± 0.5 mm.

Performance. The staple unit shall be compatible with Stapler, Surgical, Gastrointestinal, 53 mm (Note 2). The staple unit shall be suitable for use in abdominal, gynecological, pediatric, and thoracic surgical procedures.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Materials. The staple unit shall be fabricated from corrosion-resisting steel and rigid plastic. Corrosion resisting steel shall conform to ASTM Designation F899.

The staples shall be fabricated from austenitic corrosion-resisting steel that conforms to Grade 1 or Grade 2 of ASTM Designation F55.

All materials shall be suitable for their intended purpose.

Sterility. The staple unit shall be sterile in accordance with the latest edition of the United States Pharmacopeia (USP).

Workmanship. The staple unit shall be free from defects that detract from their appearance or impair their serviceability.

Unit. Package (PG). One package containing twelve individually packaged sterile staple unit, as specified, constitutes one unit. The individual package shall be a sealed peel-open type container capable of maintaining sterility of contents unless the package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at level S-2, AQL 0.65%. The unit of product for inspection purposes shall be one staple unit.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

NOTE 1: This document covers the following National Stock Number:

NSN	ITEM IDENTIFICATION
6515-01-207-8226	Staple Unit, Surgical, Gastrointestinal, 53 mm, Disposable, 12s: Sterile, Individually Wrapped. Includes Built-In Knife-Blade

NOTE 2: The above listed NSN is compatible with the following:

NSN	ITEM IDENTIFICATION
6515-01-204-5363	Stapler, Surgical, Gastrointestinal, 53 mm

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL COORDINATING ACTIVITIES:

VA-OSS
PBS
FDA-MPQAS

Project No. 6515-3981

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

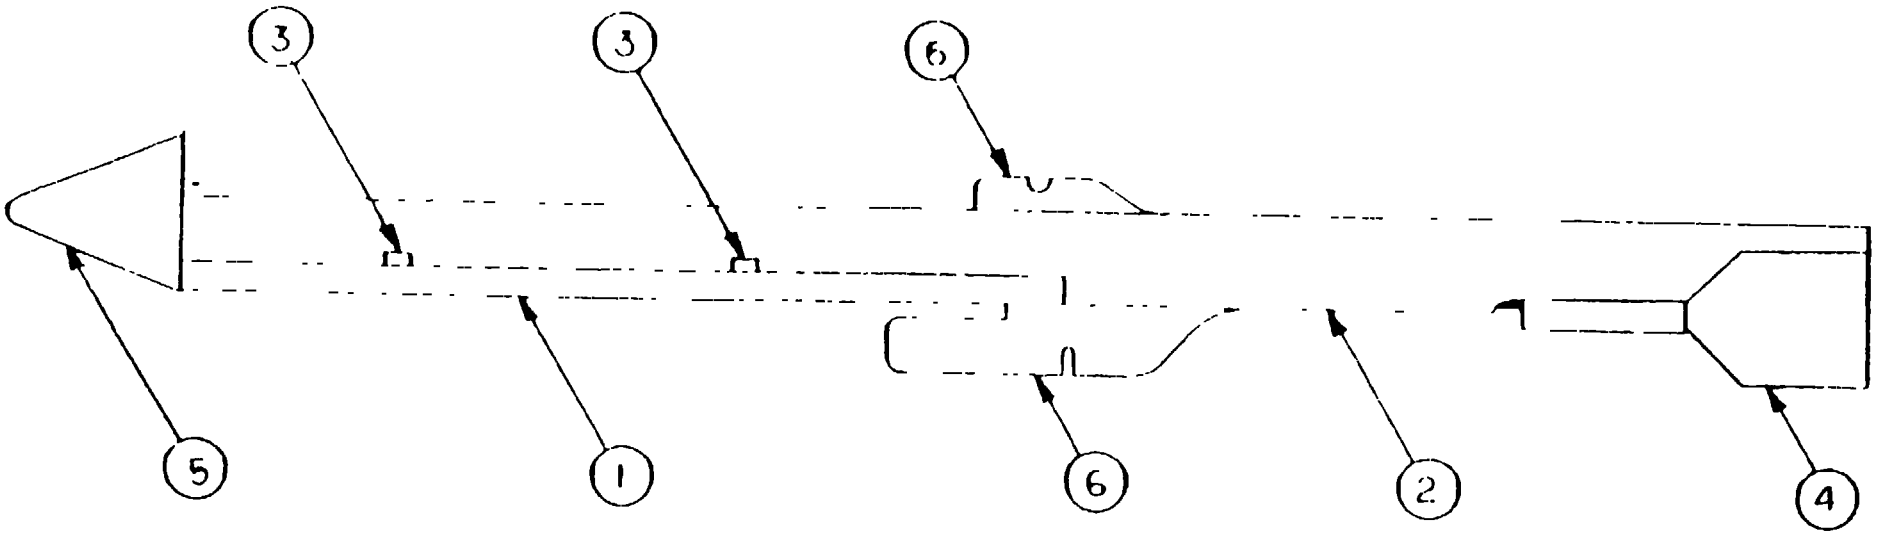

A-A-53482

(1) STAPLE CARTRIDGE

(2) PUSH-BAR/KNIFE ASSEMBLY

(3) ALIGNMENT TABS

(4) HANDLE

(5) TIP

(6) LOCKING TABS

FIGURE 1 STAPLE UNIT, SURGICAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS. In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s), or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 0000 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-RSTE
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions - Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53482	STAPLE UNIT, SURGICAL (Gastro-intestinal)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION (Mark one)
	☐ VENDOR
	☐ USER
3b. ADDRESS (Street, City, State, ZIP Code)	☐ MANUFACTURER
	☐ OTHER (Specify)

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER (Last, First, MI) - Optional	b. WORK TELEPHONE NUMBER (Include Area Code) - Optional
c. MAILING ADDRESS (Street, City, State, ZIP Code) - Optional	8. DATE OF SUBMISSION (YYMMDD)

DD FORM 12 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.