A-A-53483
8 May 1988

COMMERCIAL ITEM DESCRIPTION

STAPLER, SURGICAL (Gastro-intestinal)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a gastro-intestinal surgical stapler.

Salient characteristics:

Style and design. Shall be a gastro-intestinal surgical stapler. The stapler shall consist of a cartridge half and an anvil half.

Style and design of the cartridge half shall be in accordance with Figure 1. The cartridge half shall consist of a handle and channeled cartridge fork. Both components shall be attached by means of a distal pivot (see Figure 1). The handle shall have a proximal snap-anchor and transverse bar. The snap-anchor shall be designed to hold the cartridge fork in place until manually detached.

The cartridge fork shall contain four alignment slots; two on each side, identically spaced on both sides of the fork. This arrangement shall permit the fork to accept a compatible staple unit.

Style and design of the anvil half shall be in accordance with Figure 2. The anvil half shall consist of an anvil fork and lock lever. The proximal end of the lock lever shall be joined to the mid-point of the anvil by means of the lock-lever pivot. The anvil fork shall have a distal engagement hook and a proximal anvil. The anvil shall contain 52 staple-clinching pockets arranged in two double-staggered rows. The pocket pattern shall match the staple-channel pattern contained in the compatible staple unit.

Performance. The stapler shall be capable of undergoing repeated assembly and disassembly cycles without jamming or breakage.

When the user loads a compatible staple unit and follows the operating manual, the stapler shall place 52 surgical staples, arranged in two double-staggered rows, into tissue and split the tissue between the staples.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Materials. The stapler shall be fabricated from rigid plastic and corrosion-resisting steel. Corrosion-resisting steel shall conform to ASTM Designation F899. All materials shall be suitable for the purpose intended.

Instructions. The stapler shall be supplied with a "Directions for Use" Manual.

Workmanship. The stapler shall be free from defects that detract from its appearance or impair its serviceability.

Unit. Each (EA). One stapler, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at level S-2, AQL 1.0%. The unit of product for inspection purposes shall be one surgical stapler. As an alternate, staplers may be 100% inspected for compliance with this specification and the manufacturer's own blueprints and performance specifications.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

NOTE 1: This document covers the following National Stock Number:

NSN	ITEM IDENTIFICATION
6515-01-204-5363	STAPLER, SURGICAL, Gastrointestinal, 53 mm

NOTE 2: The following NSN is for use with the NSN listed above:

NSN	ITEM IDENTIFICATION
6515-01-207-8226	STAPLE UNIT, SURGICAL, Gastrointestinal, 53 mm, Disposable, 12s: Sterile, Individually Wrapped. Includes: Built-In Knife Blade

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4036

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

A-A-53483

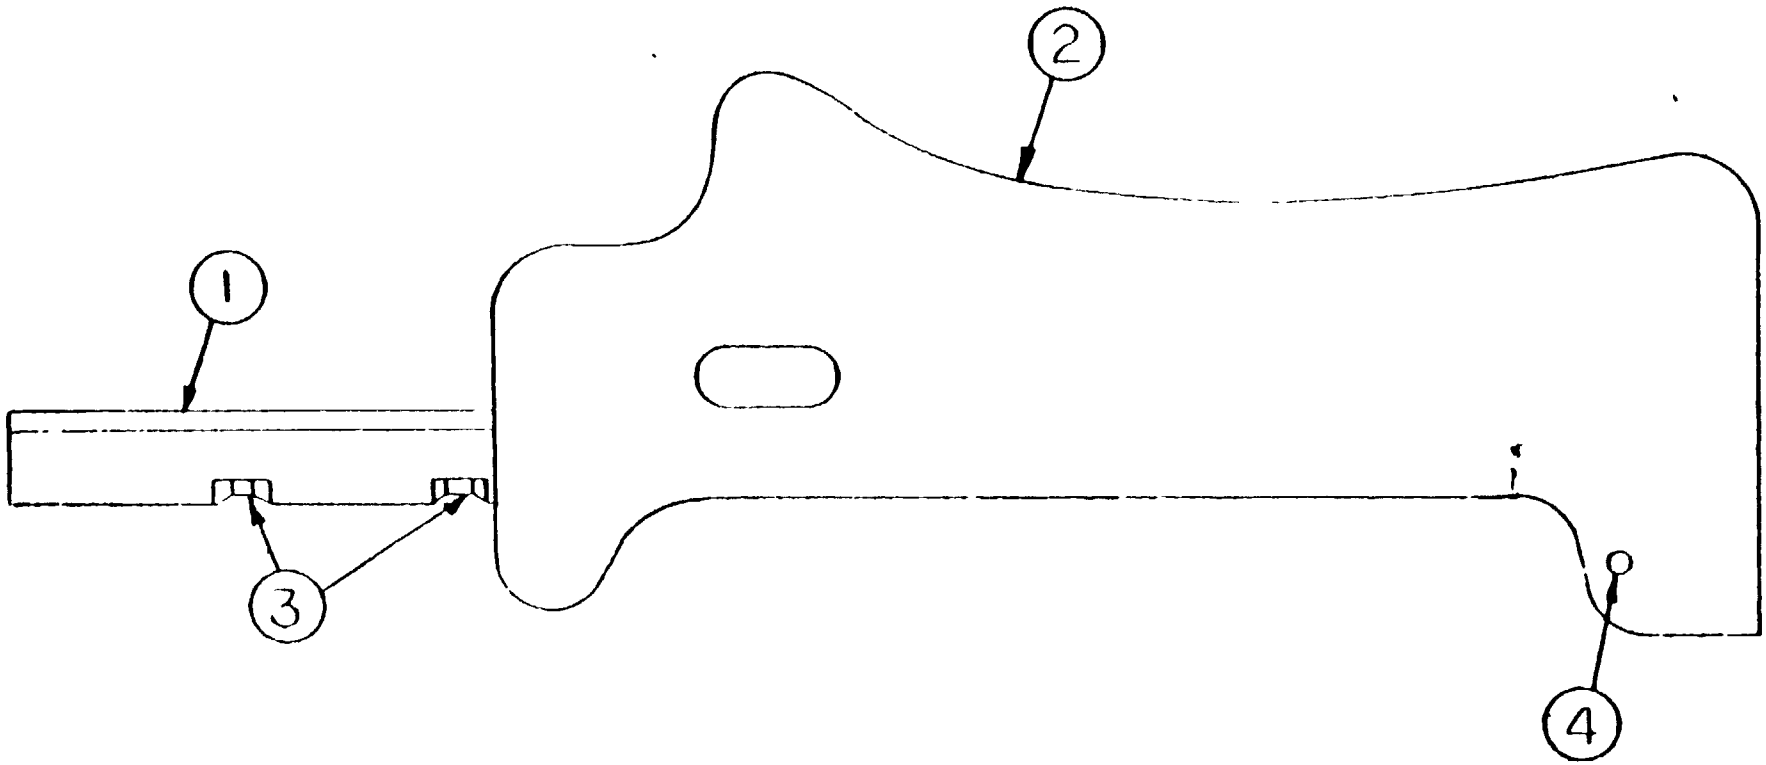

(1) CARTRIDGE FORK

(2) HANDLE

(3) ALIGNMENT SLOTS

(4) INSTRUMENT PIVOT

NOTE:
FOR GENERAL STYLE AND DESIGN

FIGURE 1 SURGICAL STAPLER, CARTRIDGE HALF

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

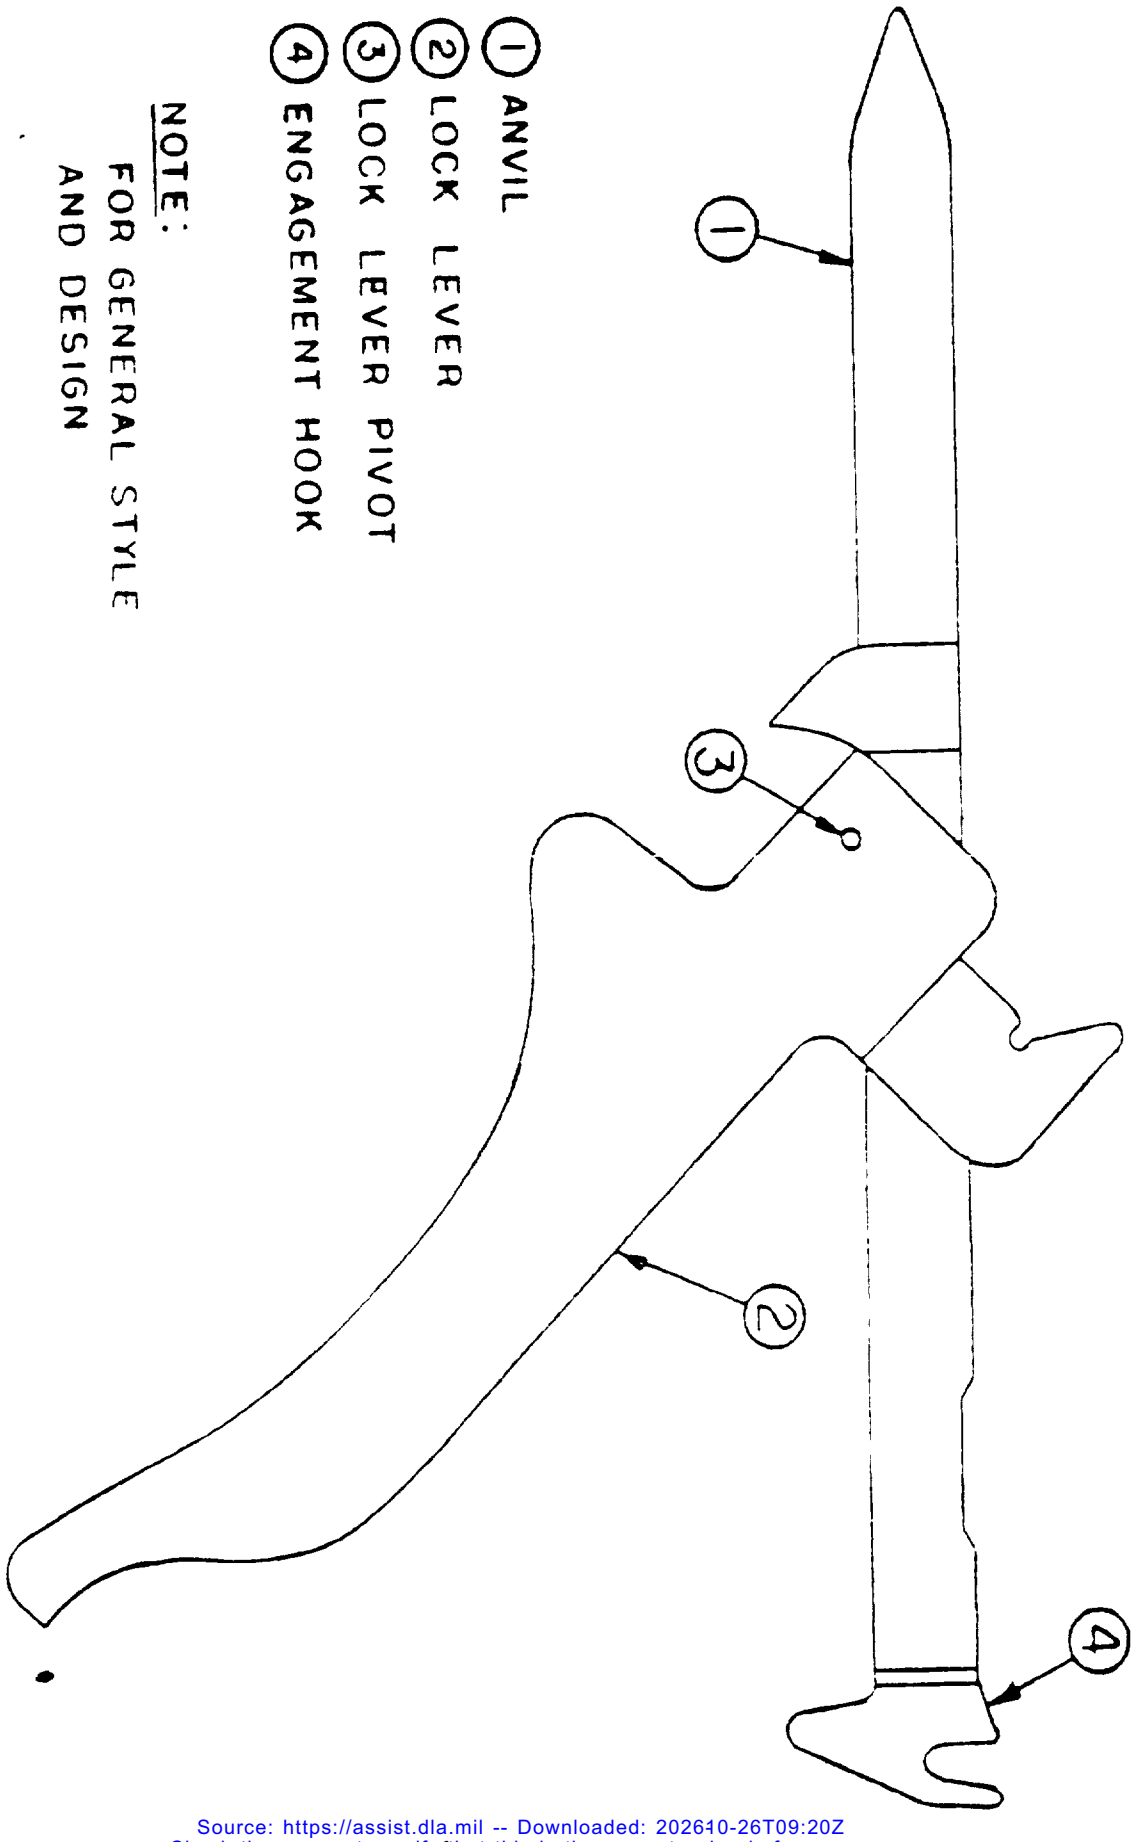


FIGURE 2 SURGICAL STAPLER, ANVIL HALF

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4066 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-RSTE
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53483	STAPLER, SURGICAL (Gastro-intestinal)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION (Mark one)
	☐ VENDOR
	☐ USER
3b. ADDRESS (Street, City, State, ZIP Code)	☐ MANUFACTURER
	☐ OTHER (Specify) _____

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER (Last, First, MI) – Optional	b. WORK TELEPHONE NUMBER (Include Area Code) – Optional
c. MAILING ADDRESS (Street, City, State, ZIP Code) – Optional	8. DATE OF SUBMISSION (YYMMDD)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil - Downloaded: 2025-10-26T09:20Z
Check the source to verify that this is the current version before use.