COMMERCIAL ITEM DESCRIPTION

STAPLER, SURGICAL, THORACIC-ABDOMINAL

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one type of reusable surgical stapler.

Salient characteristics:

Style and design. Style and design of surgical staplers shall be in accordance with Figure 1. Staplers shall consist of seven major components.

(1) Frame. The frame shall hold and align the stapler components via a suitable internal mounting system. The frame shall be slotted to permit cleaning. The frame's proximal end shall contain an integral, fixed handle. Its distal end shall contain jaws suitable for housing a compatible staple unit.

(2) Moveable handle. The moveable handle shall be spring-biasd and mounted inside the stapler frame. The moveable handle shall engage the approximating lever assembly by means of a "Tongue and Groove arrangement.

(3) Safety latch. The safety latch shall be mounted inside the stapler frame.

(4) Release lever. The release lever shall be mounted inside the stapler frame.

(5) Actuator assembly. The actuator assembly shall consist of a spring-biased actuator rod and a housing with an integral lift-plate and a set of distal guide lugs. The proximal end of the actuator assembly shall be mounted on the mechanical linkage (See #7). The distal end of the assembly shall be supported by the guide lugs which ride in extended slots in the stapler frame.

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

(6) Approximating lever assembly. The approximating lever assembly shall contain a housing and a spring-biased approximating rod. The distal end of the assembly shall be mounted on the mechanical linkage. The mid-point of the assembly shall be mounted inside the stapler frame.

(7) Mechanical linkage. The mechanical linkage shall be spring-biased and suitable for transmitting force between the approximating lever and actuator assemblies.

Materials. Surgical staplers shall be fabricated from corrosion-resisting steels, properly tempered and passivated. All materials shall be suitable for the purpose intended.

Performance. Staplers shall be compatible with the surgical staple units as indicated in Table I.

TABLE I.
Stapler - Staple Unit Compatibility

NSN: Stapler	NSN: Stapling Unit
6515-01-204-5362	6515-01-207-8222
6515-01-204-5362	6515-01-207-8223
6515-01-204-5364	6515-01-207-8224
6515-01-204-5364	6515-01-207-8225
6515-01-204-5365	6515-01-207-8219
6515-01-204-5365	6515-01-207-8220
6515-01-204-5365	6515-01-207-8221

Staplers shall place a linear, double-staggered row of surgical staples when loaded with a compatible staple unit. Staplers shall perform the following functions:

(1) The safety latch shall prevent stapler operation until manually unlocked.

(2) The actuator assembly shall pivot out of the stapler to facilitate cleaning.

(3) As the approximating lever is being closed, the actuator assembly shall advance and close the compatible staple unit. The approximating rod shall engage the moveable handle.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

(4) When the moveable handle is squeezed, the approximating and actuator rods shall simultaneously advance. The distal tip of the actuator rod shall actuate the compatible staple unit. When the handle is released, both rods shall simultaneously retract.

(5) The release lever shall unlock the stapler. When this lever is applied, the approximating assembly shall pivot up to a vertical position and the actuator assembly shall retract and allow the staple unit to open.

Instructions. Each stapler shall be supplied with a "Directions for Use" manual.

Workmanship. Surgical staplers shall be free from defects that detract from their appearance or impair their serviceability.

Unit. Each (EA). One surgical stapler, together with directions for use, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at Level S-2, AQL 1.0%. The unit of product for inspection purposes shall be one surgical stapler. As an alternate, staplers may be 100% inspected for compliance with this specification and the manufacturer's own blueprints and performance specifications.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

NSN	ITEM IDENTIFICATION
6515-01-204-5362	STAPLER, SURGICAL, Thoracic-Abdominal, 90 mm.
6515-01-204-5364	STAPLER, SURGICAL, Thoracic-Abdominal, 55 mm.
6515-01-204-5365	STAPLER, SURGICAL, Thoracic-Abdominal, 30 mm.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-3973

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

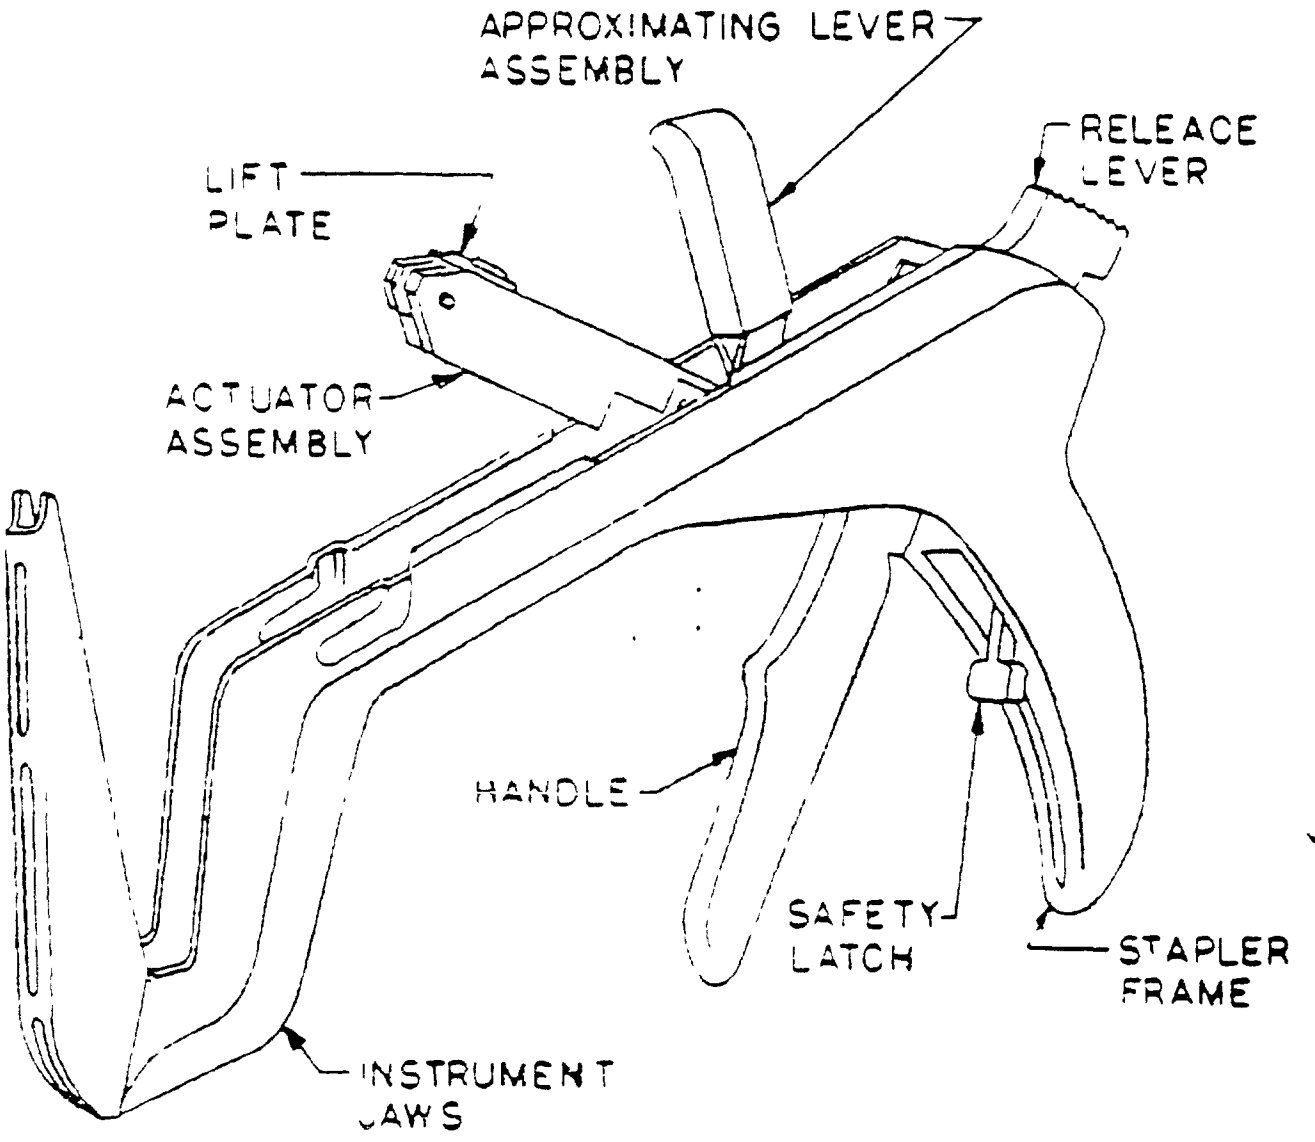


FIGURE 1 STAPLER, SURGICAL SUTURE, AUTOMATIC

(FOR GENERAL STYLE AND DESIGN)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53500	STAPLER, SURGICAL, THORACIC-ABDOMINAL

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.