COMMERCIAL ITEM DESCRIPTION

STAPLE UNIT, SURGICAL, THORACIC-ABDOMINAL

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers seven styles of Thoracic -abdominal surgical staple units.

Salient characteristics:

Style and design. Style and design of staple units shall conform to Figure 1. Staple units shall consist of the following:

Staple cartridge. The staple cartridge shall contain staple channels, a drive mecnanism designed to engage tne compatible stapler and drive the staples toward the anvil, a spring-loaded alignment pin, and a slotted alignment pin spring. The number of staple cnannels (staples) shall be as specified in Table II. Except as specified in tne "Notes" section, the channels shall be arranged in a double-staggered row (See Figure 1). Eacn cnannel shall be loaded with a surgical staple.

Anvil. The anvil shall contain a mated set of staple-clinching pockets and an engagement nook and detent stop, as snown in Figure 1.

Hinge. The ninge shall be a spring-loaded hinge connecting tne anvil and cartridge.

Dimensions. For eacn NSN, staple dimensions snall be as indicated in Table I. Tne lengtn of tne staple-cnannel pattern and tne number of cnannels snall be as indicated in Table II.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Table I.
Surgical Staple Dimensions

NSN (a)	Staple (1) Leg Length	Staple (1) Width	Staple (2) Wire Diameter
6515-01-207-8219	2.5	3.0	0.21
6515-01-207-8220	4.8	4.0	0.28
6515-01-207-8221	3.5	4.0	0.23
6515-01-207-8222	4.8	4.0	0.28
6515-01-207-8223	3.5	4.0	0.23
6515-01-207-8224	3.5	4.0	0.23
6515-01-207-8225	4.8	4.0	0.28

(a) All dimensions in mm.
(1) Tolerance: ± 0.05 mm.
(2) Tolerance: ± 0.005 mm.

Table II.
Staple Unit Dimensions

NSN	No. of Staples	Staple-Pattern (1), (2) Length
6515-01-207-8219	23	31
6515-01-207-8220	11	31.5
6515-01-207-8221	11	31.5
6515-01-207-8222	33	91.5
6515-01-207-8223	33	91.5
6515-01-207-8224	19	53
6515-01-207-8225	19	53

(1) Length in mm.
(2) Tolerance: ± 0.05 mm.

Materials. Staples shall be fabricated from corrosion-resisting steel wire that conforms to ASTM Designation F138, Grade 1 or ASTM Designation F55, Grade 1. Staple units shall be fabricated from a suitable corrosion-resisting steel and a suitable rigid plastic.

Performance. Staple unit shall be compatible with the stapler indicated in Table III. Staple units shall be suitable for use in abdominal, gynecological, pediatric, and thoracic surgical procedures.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

TABLE III.
Stapler - Staple Unit Compatibility

NSN: Staple Unit	NSN: Stapler
6515-01-207-8219	6515-01-204-5365
6515-01-207-8220	6515-01-204-5365
6515-01-207-8221	6515-01-204-5365
6515-01-207-8222	6515-01-204-5362
6515-01-207-8223	6515-01-204-5362
6515-01-207-8224	6515-01-204-5364
6515-01-207-8224	6515-01-204-5364

Sterility. Staple units shall be sterile in accordance with the latest edition of the United States Pharmacopiea (USP).

Workmanship. Staple units shall be free from defects that detract from their appearance or impair their serviceability.

Unit. Each (PG). One package containing twelve individually packaged sterile stapling units, as specified, constitutes one unit. The individual package shall be a sealed peel-open type container capable of maintaining sterility of contents unless the package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one package of staple units. As an alternate, staplers may be inspected for compliance with this specification and the manufacturer's own blueprints and performance specifications.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-207-8219	Staple Unit, Surgical, Thoracic-Abdominal, 31 mm, Disposable, 12s Sterile, Individually Wrapped
6515-01-207-8220	Staple Unit, Surgical, Thoracic-Abdominal, 31.5 mm, Disposable, 12s Sterile, Individually Wrapped
6515-01-207-8221	Staple Unit, Surgical, Thoracic-4.0 mm Wide, 31.5 mm, Disposable, 12s Sterile, Individually Wrapped
6515-01-207-8222	Staple Unit, Surgical, Thoracic-4.0 mm Wide, 91.5 mm, Disposable, 12s Sterile, Individually Wrapped
6515-01-207-8223	Staple Unit, Surgical, Thoracic-4.0 mm Wide, 91.5 mm, Disposable, 12s Sterile, Individually Wrapped
6515-01-207-8224	Staple Unit, Surgical, Thoracic-4.0 mm Wide, 53 mm, Disposable, 12s Sterile, Individually Wrapped
6515-01-207-8225	Staple Unit, Surgical, Thoracic-4.0 mm Wide, 53 mm, Disposable, 12s Sterile, Individually Wrapped

NOTE: NSN 6515-01-207-8219 shall have 23 staple-channels arranged in a triple-staggered row. All other staple units covered by this document shall conform to the requirements specified herein.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-3979

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

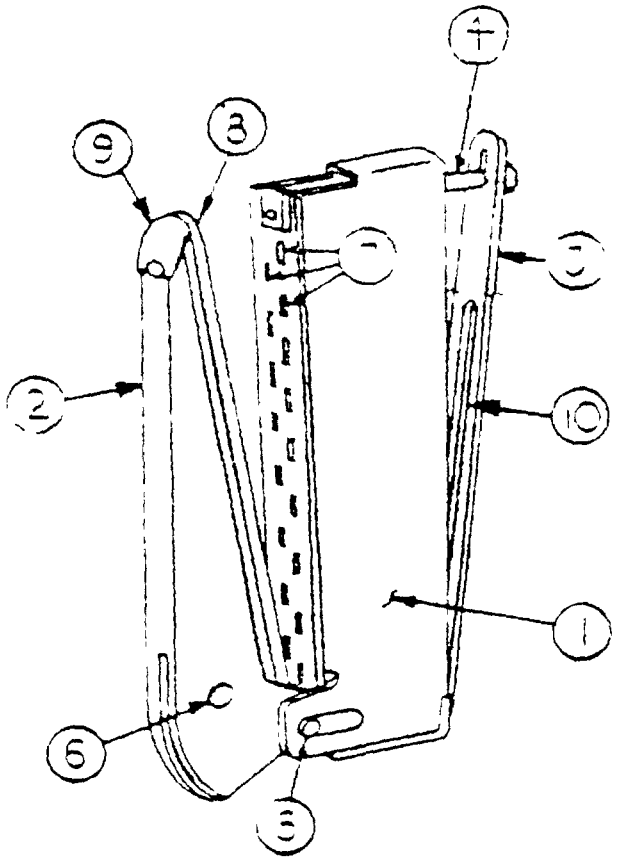


FIGURE 1

STAPLE UNIT, SURGICAL

1 STAPLE CARTRIDGE ASSEMBLY
2 ANVIL ASSEMBLY
3 ALIGNMENT PIN SPRING
4 ALIGNMENT PIN
5 SPRING-LOADED HINGE
6 DETENT STOP
7 STAPLE CHANNELS
8 ANVIL
9 ENGAGEMENT HOOK
10 ACTUATOR ROD SLOT

(FOR GENERAL STYLE AND DESIGN)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

RUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in itting comments and suggestions for improvements All users of military standardization documents are invited to provide as This form may be detached, folded along the lines indicated taped along the loose edge (*DO NOT STAPLE*), and In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was ngid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the dems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out, an owledgement will be mailed to you within 30 days to let you know that your comments were received and are being adered

TE This form may not be used to request copies of documents nor to request waivers, deviations, or clarification of ification requirements on current contracts Comments submitted on this form do not constitute or imply authorization waive any portion of the referenced document(s) or to amend contractual requirements

(Fold along this line)

(Fold along this line)

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO [illegible] ALEXANDRIA VA
POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

NO POSTAGE
NECESSARY
IF MAILED
IN THE
UNITED STATES

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions - Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53501	STAPLE UNIT, SURGICAL, THORACIC-ABDOMINAL

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION (Mark one)
	☐ VENDOR
b ADDRESS (Street, City, State, ZIP Code)	☐ USER
	☐ MANUFACTURER
	☐ OTHER (Specify) _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER (Last, First, MI) - Optional	b WORK TELEPHONE NUMBER (Include Area Code) - Optional
c MAILING ADDRESS (Street, City, State, ZIP Code) - Optional	8 DATE OF SUBMISSION (YYMMDD)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

(TO DETACH THIS FORM CUT ALONG THIS LINE.)