MIL-T-25620C(USAF)
23 JULY 1987
SUPERSEDING
MIL-T-25620B(USAF)
21 October 1958

MILITARY SPECIFICATION

TESTER, OXYGEN MASK, HEADSET AND MICROPHONE, TYPE MQ-1A

This specification is approved for use by the Department of the Air Force, and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers the requirements for a portable tester for pre-flight check of pressure demand oxygen masks and personal intercom equipment and EEU-2P goggles. The tester is designated type MQ-1A.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

FEDERAL

BB-O-925	Oxygen, Technical, Gas and Liquid.
QQ-S-781	Strapping, Steel, and Seals.
PPP-B-601	Boxes, Wood, Cleated Plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Shipping, Fiberboard.

MILITARY

MIL-P-116	Preservation, Method of.
DOD-D-1000	Drawings, Engineering and Associated Lists.
MIL-R-6371	Regulator, Diluter, Demand Oxygen, Pressure Breathing, Type A-14.
MIL-T-28800	Test Equipment for use with Electrical and Electronic Equipment, General Specification for.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: the Engineering Division, San Antonio ALC/MMEDO, Kelly AFB, TX 78241 by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC F4128 FSC 6695
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

STANDARDS

MILITARY

FED-STD-151	Metal, Test Methods.
FED-STD-595	Color (Requirements for Individual Color Chips (3 X 5 Supplements) (Should be submitted to the Naval Publication, and Forms Center,Philadelphia, citing FED-STD-595 together with Appropriate Chip Number as shown therein).

MILITARY

MIL-STD-129	Marking for Shipment and Storage.
MIL-STD-130	Identification Marking of U.S. Military Property.
MIL-STD-143	Standards and Specifications, Order of Precedence for the Selection of.
MIL-STD-147	Palletized Unit Loads.
MIL-STD-454	Standard General Requirements for Electronic Equipment.
MIL-STD-794	Part and Equipment, Procedures for Packaging and Packing of.
MIL-STD-810	Environmental Test Methods and Engineering Guidelines.
MIL-STD-831	Test Reports, Preparation of.
MIL-STD-889	Dissimilar Metals.
MIL-STD-1472	Human Engineering Design Criteria for Military Systems, Equipment and Facilities.
MS22055	Hose Assemblies-Oxygen Breathing, Connector to Regulator.

2.1.2 Other Government documents. The following other Government document forms a part of this specification to the extent specified herein. Unless otherwise specified, the issues shall be those in effect on the date of the solicitation.

AIR FORCE - AERONAUTICAL STANDARDS

AN804	Tee, Flared Tube with Bulkhead on Run.
AN924	Nut, Tube, Bulkhead and Universal Fitting.
AN929	Cap Assembly, Tube, Pressure Seal.
AN6021	Gage, Panel Mounting Low Pressure Oxygen.
AN6029	Indicator - Oxygen Flow.

(Copies of specifications, standards, and other Government documents required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting officer.)

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise specified, the issues of the documents which are DOD adopted shall be those listed in the issue of the DODISS specified in the solicitation. Unless otherwise specified, the issues of documents not listed in the DODISS shall be the issue of the non-government documents which is current on the date of the solicitation.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

AMERICAN SOCIETY FOR TESTING AND MATERIAL (ASTM)

ASTM D-3951 Packaging, Commercial.

(Application for copies of ASTM publications should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

(Nongovernment standards and other publications are normally available from the organizations which prepare or which distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein (except for associated detail specifications, specification sheets or MS standards), the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 First article. When specified in the contract or purchase order, a sample shall be subjected to first article inspection (see 4.4 and 6.4).

3.2 Materials.

3.2.1 Metals. Metals shall be of the corrosion-resistant type or suitably treated to resist corrosion due to fuels, salt spray, or atmospheric conditions likely to be met in storage or normal service. Non-ferrous materials shall be used for all parts of the tester except where ferrous materials are essential and do not come into contact with the oxygen. Nonmagnetic materials shall be used for all parts of the tester except where magnetic materials are essential.

3.2.1.1 Dissimilar metals. Unless protected against electrolytic corrosion, dissimilar metals shall not be used in intimate contact with each other. Dissimilar metals are defined in MIL-STD-889.

3.2.2 Protective treatment. When materials are used in construction of the tester that are subject to corrosion in oxygen, salt, or other atmospheric conditions likely to occur during service usage, they shall be protected against such corrosion in a manner that will in no way prevent compliance with the performance requirements of this specification. The use of any protective coating that will crack, chip, or scale with age or extremes of atmospheric conditions shall be avoided.

3.3 Design. The tester shall conform to figure 1. The components shall be enclosed in a case, provided with a carrying handle, hinges, and latches. Combination captive catch and hinge assemblies shall be provided at rear of case, and the case design shall include provisions for stacking.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

3.3.1 Components. The tester shall consist of the following major components:

Case

Oxygen equipment

Flow indicator

Pressure gage

Oxygen regulator

Mask hose

Inlet fitting

Communications and goggle equipment

Power unit

Headset and microphone and goggle equipment test circuit

3.3.1.1 Case. The case shall be made of fiberglass, aluminum, or fiberboard material, and finished in a durable black color, lusterless, no. 33538 of FED-STD-595. The panel shall be recessed so that the accessible components are completely enclosed when the tester is not in use. Case dimensions shall be in accordance with figure 1.

3.3.1.2 Oxygen equipment. The oxygen equipment shall be connected as specified in figure 2.

3.3.1.2.1 Flow indicator. The oxygen flow indicator shall conform to AN6021.

3.3.1.2.2 Pressure gage. The oxygen pressure gage shall conform to AN6021-1B.

3.3.1.2.3 Oxygen regulator. The oxygen regulator shall conform to MIL-R-6371.

3.3.1.2.4 Mask hose. The regulator end of the hose shall be permanently attached below the panel.

3.3.1.2.5 Inlet fitting. The inlet fitting shall be a T-fitting. The fitting shall be attached to the panel of the tester with a check-nut conforming to AN924D5. A cap conforming to AN929 shall be provided for each of the two inlets. The caps shall be attached to the case by means of suitable chains.

3.3.1.2.6 Fuse. Protection fuse shall be provided with the tester to prevent electrical hazard during operation. The fuse shall locate between the input power and the internal circuit. The fuse and fuse holder shall be in accordance with requirement 39 of MIL-STD-454.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

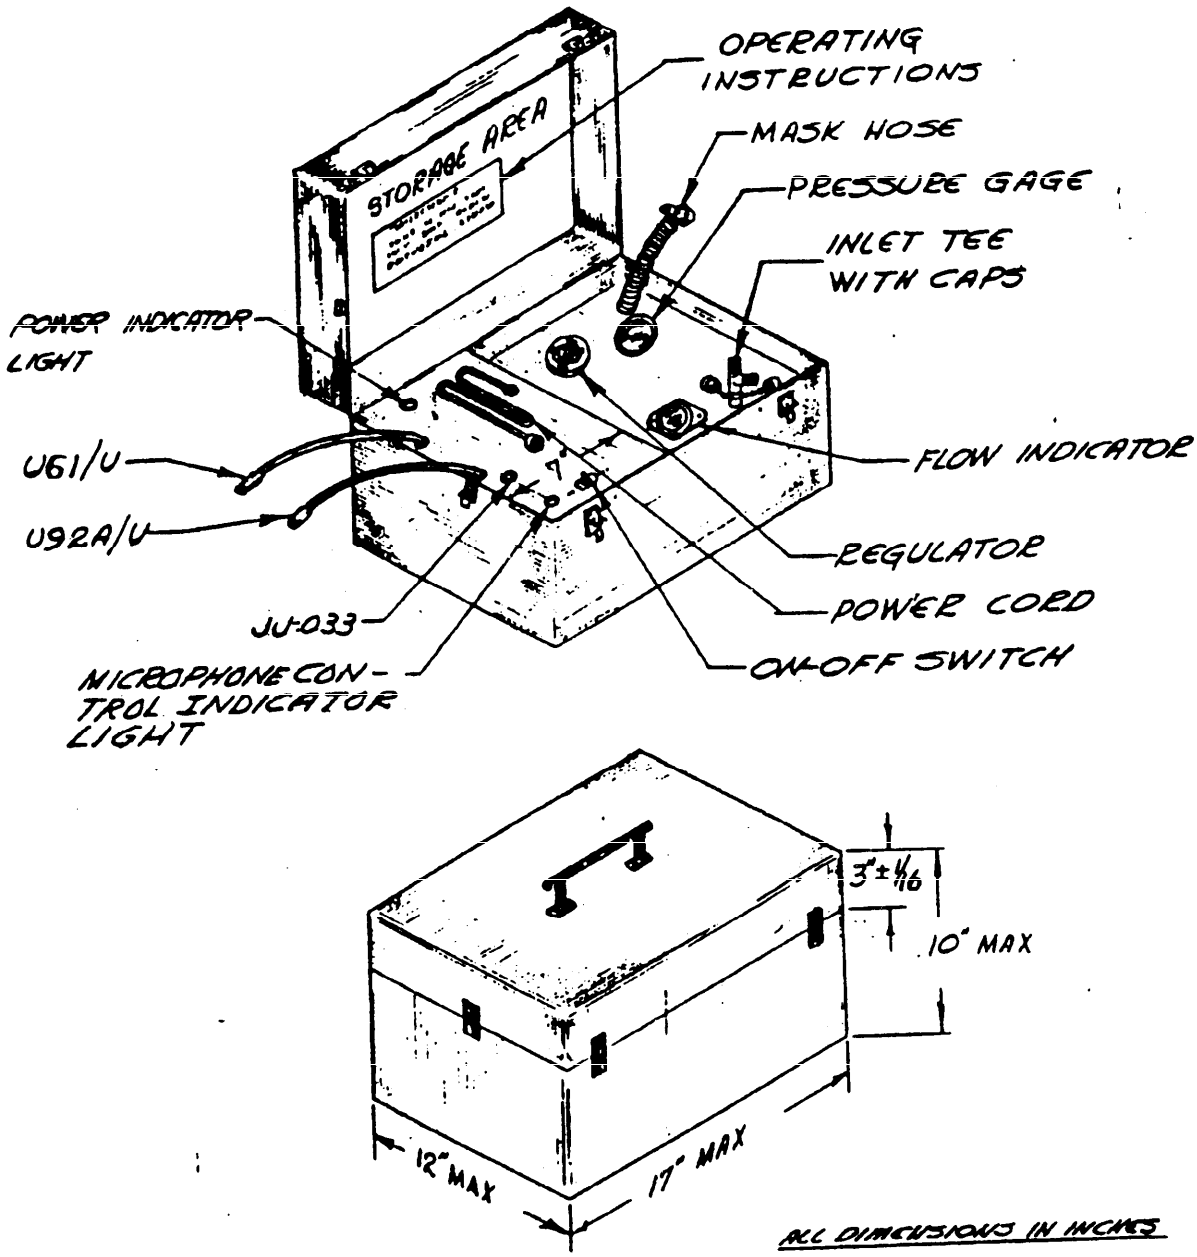


FIGURE 1. Tester.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

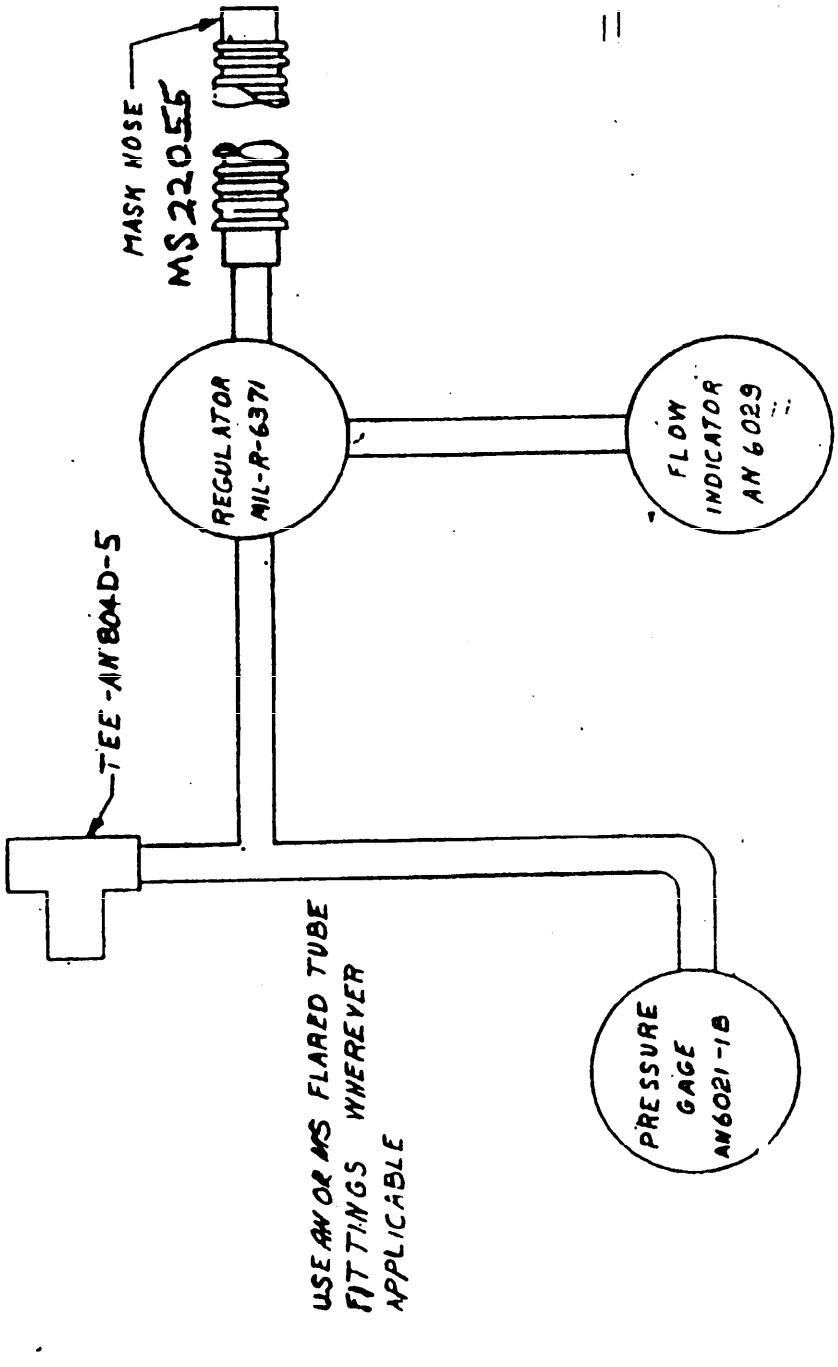


FIGURE 2. Oxygen equipment.

Source: https://assist.dla.mil -- Downloaded: 202610-20T06:49Z
Check the source to verify that this is the current version before use.

3.3.1.3 Communications and goggle equipment. Communications equipment shall be provided to allow a "talk-out" check of headsets and mask microphones currently in use. The equipment shall consist of necessary circuitry for headset, microphones (carbon and dynamic) and functionally test EEU-2P goggles. The equipment shall conform to MIL-T-28800.

3.3.1.3.1 Power unit. A power unit shall be provided in the test set case to convert 115 volts (v) alternating current (AC), 60 cycles (Hz). The output of the power unit shall supply power to amplifier and goggle circuit of 28VDC 200 milliampere (ma): A power conditioner unit is required between tester and goggles. An isolation transformer, "ON" "OFF" power switch, 115V line fuse, 115V power indicator light, and a 6-foot(ft) heavy duty commercial rubber electrical cord shall be provided.

3.3.2 Control panel. All electrical connections and control components shall be located on the top panel of the tester. Arrangement and location of the connectors, control knobs, indicator, gage and accessories shall be in accordance with MIL-STD-454 requirement 28.

3.4 Maintainability. The equipment shall be designed as to facilitate maintenance. It shall require a minimum number and types of tools and test equipment to perform maintenance. The tester shall provide optimum accessibility and replaceability of all components requiring maintenance in accordance with MIL-STD-1472, section 5.9. Maintenance procedures shall be provided with the equipment.

3.5 Performance characteristics.

3.5.1 Operation. With the tester connected to a 450 pounds per square inch (psi) breathing oxygen cylinder and the communications unit to a 115 V outlet, an oxygen mask (see 3.10) shall be tested for leakage while the microphone and headset are being tested for correct operation.

3.5.2 Oxygen leakage. The oxygen system shall not leak more than 7 psi under a pressure of 450 psi with source removed.

3.5.3 Load. The case shall be able to withstand a static load as specified in 4.5.4 without damage.

3.5.4 Water-tightness. The case shall be designed so that no water will enter the case when tested as specified in 4.5.5.

3.5.5 Salt spray. The case and case accessories (hinges, handle, locks, and reinforcements) shall withstand the salt spray test as specified in 4.5.6.

3.5.6 Handle. The case handle shall be designed and constructed to withstand the test specified in 4.5.7.

3.5.7 Drop. The case shall be able to withstand the free fall drop test specified in 4.5.8.

Source: https://assist.dla.mil -- Downloaded: 202610-20T06:49Z
Check the source to verify that this is the current version before use.

3.6 Interchangeability. All parts of the tester having the same manufacturer's part number shall be functionally and dimensionally interchangeable. Interchangeability shall be in accordance with MIL-STD-454, requirement 7. The drawing number requirements of DOD-D-1000 shall govern changes in the manufacturer's part numbers.

3.7 Finish. Finish shall be in accordance with high-grade manufacturing practice covering this class of work and shall be consistent with material employed in the fabrication of the case.

3.8 Operating instructions. Instructions for operating the tester shall be permanently attached to the inside of the case cover as shown on figure 1. The instructions shall be as follows:

Preliminary instructions.

a. Connect external oxygen supply to one inlet of the test unit with the other inlet capped (450 psi).

b. Set A-14 regulator to "normal" oxygen position.

c. Open cylinder valve. Allow pressures up to 450 psi (maximum).

d. Plug input into 110 V, 60 Hz power source, and turn "ON"-"OFF" switch to "ON" position.

Operating instructions.

a. Don headgear and mask.

b. Set regulator to "normal" position.

c. Connect mask delivery tube to mask hose.

d. Turn regulator to 43M (M=1000).

e. Exhale slowly.

(1) If blinker opens - no leak.

(2) If blinker remains closed - mask leaks and needs adjustment.

f. Turn regulator to 45M.

g. Exhale slowly.

(1) If no resistance to exhalation, inhalation valve is satisfactory.

(2) If resistance to exhalation, inhalation valve needs cleaning or replacing in accordance with applicable technical order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

h. Plug in headset and microphone. Headset and microphone are functioning properly when the voice is transmitted from the microphone to the headset through the amplifier. (NOTE: When a hand-held microphone is tested, the handle switch must be pressed to talk. The microphone control indicator light should light up when the microphone switch is depressed).

i. Plug EEU-2P goggles into goggle power cord after donning the helmet. Pull the goggles forward and downward to engage the side latches. The lenses should immediately change to the open, transparent mode.

(1) Wait 10 seconds, then press the press to test (PTT) actuator (located above the left front lens), the goggles should rapidly darken to the closed mode. They should rapidly return to the open mode when the PTT Actuator is released.

(2) Use a fast strobe lite (SDU-5/E) to illuminate the forward side of the goggles. The goggles should rapidly darken to the closed mode, and then return to the open mode.

(3) Raise the goggles to remove electrical power, the goggles should darken to the closed mode in approximately 5 seconds.

j. Set A-14 regulator back to "Normal" and disconnect the mask, microphone-headset and EEU-2P goggles from the test unit.

3.9 Identification of product. Each tester shall be marked in accordance with MIL-STD-130. This marking shall be on the outside of the case.

3.9.1 There shall be suitable markings on the face of the tester to differentiate between the power indicator light and the microphone control indicator light.

3.10 Government loaned property. The Government will loan the following equipment to the contractor upon his request (see 6.5).

ITEM	NSN	QUANTITY
Mask	1660-01-073-7596	1
Goggles	8475-01-017-4473	1
Cable	8475-01-081-1349	1
Cable	8475-01-081-1350	1
Toplatch Assy	8475-01-098-0881	1
Cord assy	5995-01-006-1836	1
Microphone	5965-00-843-9957	1
Headset assy	5965-00-069-2723	1

EEU-2P Operational Manual will be provided to contractor for reference material.

Source: https://assist.dla.mil -- Downloaded: 202610-20T06:49Z
Check the source to verify that this is the current version before use.

3.11 Workmanship. The tester shall be constructed in accordance with high-grade aircraft instrument manufacturing practice. The tester shall be thoroughly cleaned of all oil and foreign matter and free from any defects that might affect its operation or functionability.

3.12 Selection of specifications and standards. Specifications and standards for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-143.

3.13 Reclaimed materials. The use of reclaimed materials shall be encouraged to the maximum extent possible.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirement specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items must meet all requirements of sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of assuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling in quality conformance does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to acceptance of defective material.

4.2 Classification of tests. The inspection and testing of testers shall be classified as follows:

First article testing (see 4.4).

4.2.1 Defects in items already accepted. The investigation of a test failure could indicate that defects may exist in items already accepted. If so, the contractor shall fully advise the procuring activity of all defects likely to be found and methods of correcting them.

4.3 Test conditions.

4.3.1 Atmospheric conditions. Unless otherwise specified, all tests required by this specification shall be made at an atmospheric pressure of 28 to 32 inches of mercury and at a temperature of 77 degrees Fahrenheit, (25 degrees Celsius) plus or minus 18 degrees ($\pm$ 7°C), and a relative humidity of 80 percent or less. Where tests are made with atmospheric pressure or temperature substantially different from the above values, proper allowance shall be made for the change in instrument reading.

4.3.2 Oxygen. Oxygen used for test purposes shall conform to type I, grade A of BB-O-925.

Source: https://assist.dla.mil -- Downloaded: 202610-20T06:49Z
Check the source to verify that this is the current version before use.

4.4 First article testing.

4.4.1 First article test sample tested by the contractor. The contractor shall subject one tester to the first article tests specified in 4.4.3.

4.4.2 First article test report. When specified in the contract or order, a first article test report shall be prepared (see 6.2.2).

4.4.3 First article tests. First article tests shall consist of all tests described under test methods (see 4.5).

4.5 Test methods.

4.5.1 Examination of product. Each tester shall be examined to determine conformance with the requirements of this specification with respect to general construction, finish, workmanship, and marking.

4.5.2 Operation. The operating instructions listed in 3.8 shall be accomplished on each tester. Prior to plugging in EEU-2P goggles and checking for proper voltage and current output, the following tests should be performed on the power conditioner PC board:

a. With 32VDC± 1 to input and the output short circuited, the output current shall be 70 ma (min) to 100 ma (max).

b. With 28VDC± 4 to input and a load of 20 ma ± 1 using a 1400 ohm resistor to output, the output voltage shall be 27V (MIN).

4.5.3 Oxygen leakage. Rate of leakage shall be determined by applying 450 psi pressure to the tester with the regulator in "normal" position. The rate of leakage shall be determined by pressure drop within the system. The tester shall not leak more than 0.5 liter per minute standard temperature and pressure based on the volume of the system. Testers which leak more than 0.5 liter per minute shall be rejected.

4.5.4 Load. The case shall withstand an evenly distributed static load of 2.5 psi on all case surface areas. Any cracking, or permanent deformation or damage to the case, lock, or hinges caused by this load shall be cause for rejection.

4.5.5 Water-tightness. The case shall be rain-tested in accordance with procedure I, "RAIN TESTS" of MIL-STD-810.

4.5.6 Salt spray. The case and case accessories (hinges, handle, locks, and reinforcements) shall be subjected to a 30-hour salt spray test in conformance with FED-STD-151. Any evidence of corrosion in the case accessories (hinges, handle, locks, and reinforcements); or any distortion of dimensions, or displacement of fittings of more than 0.067 inch (17 millimeter) of the case subsequent to drying, shall be cause for rejection.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

4.5.7 Handle. Any empty case shall be loaded with dead weight equal to five times the weight of the complete tester to give even interior loading. The case shall be lifted and rotated through 360 degrees 10 times. Cause for rejection shall be any residual distortion at completion of the lifting test which exceeds 0.067 in linear and angular dimensions or linear or angular dimensions from the original design specifications. Opening or springing of the case locks, hinges, reinforcements, or handle, or permanent distortion of the case during the lifting tests shall be cause for rejection.

4.5.8 Drop. The case shall be subjected to 18 inches free fall drop on a concrete surface, on each of eight corners. A dummy load (15 pounds, plus or minus 1 pound) shall be used to simulate the weight of the equipment to be installed in the case. Use of the case shall not be impaired after this test.

4.5.9 Inspection of packaging. The sampling and inspection of the preservation, packaging, and container marking shall be in accordance with the requirements of section 5.

5. PACKAGING

5.1 Preservation. Preservation shall be level A, C, or Commercial as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning. The tester shall be cleaned in accordance with MIL-P-116, process C-I.

5.1.1.2 Drying. The tester shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative applications. Preservatives shall not be used.

5.1.1.4 Unit packs. Unless otherwise specified (see 6.2), each tester shall be individually unit packed in accordance with method IIB of MIL-P-116 designated herein insuring compliance with the applicable requirements of that specification.

5.1.1.5 Intermediate packs. No intermediate packs are required.

5.1.2 Level C. The level C preservation for the tester shall conform to the MIL-STD-794 requirements for this level.

5.1.3 Commercial. The commercial preservation of tester shall be in accordance with the requirements of ASTM D-3951.

5.2 Packing. Packing shall be level A, B, C or Commercial, as specified (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

5.2.1 Level A. The packaged testers shall be packed in containers conforming to PPP-B-601, overseas type; PPP-B-621, class 2 style 4. Closure and strapping shall be in accordance with applicable container specifications except the strapping shall conform to QQ-S-781, type I, or IV, finish A. When the gross weight exceeds 200 pounds or the container length and width is 48" X 24" or more and the weight exceeds 100 pounds, 3 X 4 inch skids (laid flat) shall be applied in accordance with the requirements of the container specification.

5.2.2 Level B. The packaged testers shall be packed in fiberboard containers conforming to PPP-B-636, class weather resistant, style optional, special requirements. In lieu of the closure and waterproofing requirement in the appendix of PPP-B-636, closure waterproofing shall be accomplished by sealing all seams, corners and manufacturer's joints with waterproof packaging tape or box closure and sealing tape, two inches minimum width.

5.2.3 Level C. The level C packing for tester shall conform to the MIL-STD-794 requirements for this level.

5.2.4 Commercial. The preserved tester shall be packed in accordance with the requirements of ASTM D-3951.

5.2.5 Palletized loads. When specified, (see6.2) palletized loads, commensurate with the level of packing specified in the contract or order, shall be palletized in accordance with MIL-STD-147. Palletized loads shall be uniform in size and quantities to the greatest extent possible. If the container is of a size which does not conform to any of the pallet patterns specified in MIL-STD-147, the pallet pattern used shall first be approved by the contracting officer.

5.3 Marking. In addition to any special or other identification marking required by the contract (see 6.2), each unit pack, intermediate and exterior container and unitized load shall be marked in accordance with MIL-STD-129 or ASTM D-3951 as applicable.

5.3.1 Commercial. Commercial markings shall be in accordance with the requirements of ASTM D-3951.

5.4 General.

5.4.1 Exterior containers. Exterior containers (see 5.2.1, 5.2.2, 5.2.3 and 5.2.4) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.5.9.

6. NOTES

6.1 Intended use. The tester covered by this specification is intended for use in determining the proper operation of the diluter demand, pressure breathing oxygen masks, communication systems, and EEU-2P goggles.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

6.2 Ordering data.

6.2.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number, and date of this specification.

b. First article requirements.

c. Unit quantities.

d. Selection of applicable levels of preservation, packaging, packing, marking and commercial/industrial (see 5.1, 5.2 and 5.3).

e. Where palletized loads are required (see 5.4).

6.2.2 Data requirement. When this specification is used in an acquisition and data are required to be delivered, the data requirements identified below shall be developed as specified by an approved Data Item Description (DD Form 1664) and delivered in accordance with the approved Contract Data Requirements List (CDRL), incorporated into the contract. When the provisions of DOD FAR Supplement, Part 27, Sub-Part 27.410-6 (DD Form 1423) are invoked and the DD Form 1423 is not used, the data specified below shall be delivered by the contractor in accordance with the contract or purchase order requirements. Deliverable data required by this specification are cited in the following paragraphs.

Paragraph no.	Data requirement title	Applicable DID no.
4.4.2	First Article Inspection Report	DI-T-4902

(Data item descriptions related to this specification, and identified in section 6 will be approved and listed as such in DOD 5010.12-L. AMSDL. Copies of data item descriptions required by the contractors in connection with specific acquisition functions should be obtained from the Naval Publications and Forms Center or as directed by the contracting officer.)

6.4 First article. When a first article inspection is required, the item should be a first article sample. The contracting officer should include specific instructions in acquisition documents regarding arrangements for examinations, approval of first article test results and disposition of first articles. Invitations for bids should provide that the Government reserves the right to waive the requirement for samples for first article inspection to those bidders offering a product which has been previously acquired or tested by the Government, and that bidders offering such products, who wish to rely on such production or test, must furnish evidence with the bid that prior Government approval is presently appropriate for the pending contract.

6.5 Government-loaned property. The contracting officer should arrange to loan the property listed in 3.10.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

6.6 Subject term (key word) listing.

Oxygen mask tester

Portable oxygen mask tester

Pre-flight tester, oxygen mask

Tester, oxygen, mask

Tester, oxygen mask, headset and microphone, type MQ-1A

Tester, portable, oxygen mask

Tester, pressure demand, oxygen mask

6.7 Changes from previous issue. Asterisks (or vertical lines) are not used in this revision to identify changes with respect to the previous issue due to the extensiveness of the changes.

Custodian:
Air Force - 99

Reviewer:
DLA -GS

Preparing activity:
Air Force - 82

(Project 6695-F072)

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T06:49Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEPARTMENT OF THE AIR FORCE

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 73236 WASHINGTON D. C.

POSTAGE WILL BE PAID BY THE DEPARTMENT OF THE AIR FORCE

[redacted]

Source: https://assist.dla.mil -- Downloaded: 202610-20T06:49Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR ☐ USER ☐ MANUFACTURER ☐ OTHER *(Specify)*: _____
b. ADDRESS *(Street, City, State, ZIP Code)*	

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 202610-20T06:49Z
Check the source to verify that this is the current version before use.