INCH-POUND

A-A-54089A
30 June 1992
SUPERSEDING
A-A-54089
9 February 1990

COMMERCIAL ITEM DESCRIPTION

BLOOD RECIPIENT SET, INDIRECT TRANSFUSION (Disposable)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a sterile, non-toxic, disposable "Y" blood recipient (transfusion) set suitable for use by all standard blood collecting and dispensing bags, and all standard glass or flexible parenteral solution containers. The blood recipient set shall be provided in Type I or Type II as specified herein.

Salient characteristics:

General. The set shall be sterile, non-toxic, disposable "Y" blood transfusion set having two piercing devices, an air vent with a check valve covered by a removable bacterial filter, two shut-off control clamps, a drip chamber containing a filter, a male needle adapter, a roll-flow control device, easily removed end protectors and a distal injection bulb. The blood recipient set shall be capable of being used with all standard blood collecting and dispensing bags, and all standard glass or flexible parenteral solution containers.

Material. Plastic tubing shall be colorless, transparent polyvinyl chloride, the filter element shall be nylon or polyester mesh, the end protectors shall be polyethylene and the distal injection bulb shall be natural rubber. Other plastic components shall be fabricated of material suitable for the intended purpose.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Construction. The blood recipient set shall be constructed as shown in Figure 1 and shall have an overall length of 80 ± 2 inches for Type I set. The dimension from the spikes to the drip chamber shall be approximately 11-1/2 inches for the Type I set. The drip chamber shall be a single unit consisting of drip device containing a filter element. As an alternate, the drip and filter chambers for Type I may be separate. The fluid passages into the drip chamber shall blend into a single drip orifice which shall be calibrated to deliver 12 ± 3 drops per ml.

For Type II set the tubing dimension from the solution and blood bag connectors to the drip chamber/filter, shall be a minimum length of 9 inches (22.86 cm) and each tube shall have an on/off clamp, drip chamber/filter chamber (pressure pump). For Type II set the tubing from needle adapter end to drip/filter chamber shall be a minimum of 60 inches (152.40 cm) long with an on/off clamp and needle adapter with protector.

The filter element shall be fabricated of nylon or polyester mesh and shall have a minimum filtering area of 4.33 square inches and shall conform to the requirements of Standard Sieve Numbers 70 to 100 of the current United States Pharmacopeia (USP).

The solution container piercing device shall consist of an integrally molded unit including a piercing spike. The piercing spike tip shall be 7/8 to 1 inch long with a diameter of 0.258 to 0.267 inch at the base. The piercing tip shall be suitable for puncture and insertion into a stopper of a standard solution container without coring or leakage. The unit shall contain an air vent with a check valve covered by a removable bacterial filter.

The blood bag piercing device shall consist of an integrally molded unit including a piercing spike. The piercing spike tip shall be 1-1/4 ± 1/8 inches long with a tapered shaft having a base diameter of 0.258 to 0.267 inch. The piercing spike shall be formed or molded in such a way as to function as an automatic stop. The tip shall be designed with either a side opening, a distal opening or three ribbed openings, and shall be of sufficient length to rupture the inlet seal on existing blood bags; however, not of such length to reach far enough into the bag as to perforate the side walls during insertion.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

The plastic tubing shall be firmly interconnected and permanently secured as shown in Figure 1. The outside diameter of the tubing shall be 0.189 ± 0.003 inch with a 0.032 ± -.002 wall thickness, or as an alternate, shall have an outside diameter of 0.183 ± 0.003 inch with a wall of 0.024 ± 0.001 inch.

The distal injection bulb shall be ball-shaped and located adjacent to the needle adapter, molded from natural rubber with targeted resealable needle puncture sites.

The control clamp shall be a screw-type or roller clamp used for solution or blood flow regulation. The roller shall be permanently secured in the clamp. The roller in the fully open position shall be able to withstand a 3.65 kg load directed toward the open end of the clamp without the roller being removed from the clamp body. The roller clamp shall be easily operated with one hand.

The male needle adapter shall be fabricated of suitable translucent plastic and shall be tapered to fit a needle having standard Luer hub in accordance with ANSI/HIMA Standard MD70.1.

Shut-off control clamps shall be provided, one on each tubing leg connected to the drip chamber. Clamps shall allow complete shut-off or complete open flow of fluids in the legs. End protectors shall be attached to each end of the blood recipient set to maintain sterility of the fluid path.

Sterility, pyrogenicity, toxicity. The blood recipient set shall have a sterile, non-toxic and pyrogen-free fluid path completely sealed to maintain sterility. The fluid path shall be non-toxic, and pyrogen-free in accordance with United States Pharmacopeia (USP). The blood recipient st shall meet the requirements for transfusion and infusion assembles and the added requirements for Class II plastics as stated in the current USP. The sterility assurance level shall be 1 X 10-6 in accordance with the Association for the Advancement of Medical Instrumentation (AAMI) guidelines.

All surfaces coming in contact with administered blood or fluid shall contain no more than 5 parts per million (PPM) of lead when tested in accordance with USP.

Leakage. The set shall have a priming volume of 46 ml or less and shall not leak or show any damage when subjected to an internal pressure of 8 psig.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Instructions. Each individual set shall have detailed instructions for proper use and shall indicate the calibration drop size of 12 drops per ml.

Workmanship. The blood recipient shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). For Type I, one package containing forty-eight individually packaged blood recipient sets, each with instructions for use, as specified, constitutes one unit.

For Type II, packaging shall appear in the solicitation.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one blood recipient set as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one blood recipient set. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/ ontractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6515-01-128-1407	BLOOD RECIPIENT SET, Indirect Transfusion, Disposable, Y-Type, 48's	I
6515-00-071-0796	BLOOD RECIPIENT SET, Indirect Transfusion, Y-Type sterile fluid path, disposable, Two beveled spike connectors with tip protectors (one blood and one solution connector), with pressure pump.	II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5418
Location: c:\word\nish\bloodcid

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

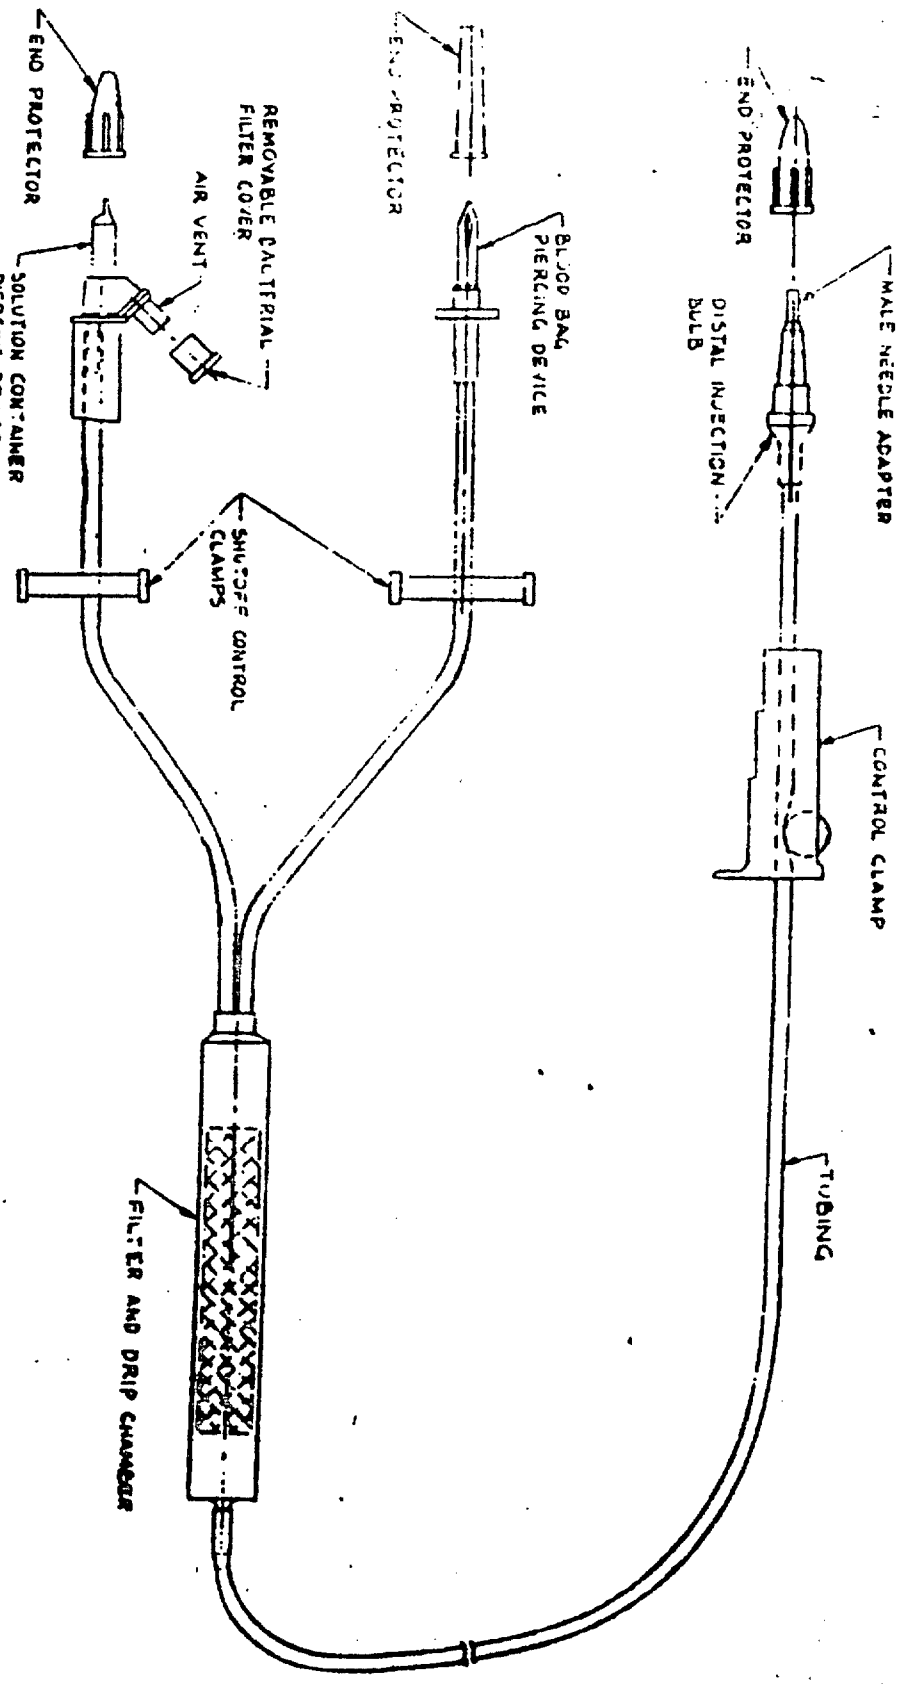


FIGURE 1 BLOOD RECIPIENT SET, INDIRECT TRANSFUSION

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54089A	30 June 1992

3. DOCUMENT TITLE
BLOOD RECIPIENT SET, INDIRECT TRANSFUSION (Disposable)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, MI) (Optional)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	c. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial 215-737-2870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.