A-A-54397
30 April 1991

COMMERCIAL ITEM DESCRIPTION

TIP, DENTAL SUCTION APPARATUS, PLASTIC

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a soft plastic disposable suction tip suitable for use with high-volume oral evacuation systems.

Salient characteristics:

Material. The tip shall be fabricated from polyethylene.

Style, design and dimensions. The tip shall be of one-piece construction. The tip shall be round in cross section and beveled at both ends such that the bevels are near parallel. The design and dimensions of the tip shall conform to Figure 1. The side-vented design shall serve to eliminate soft-tissue lock while providing maximum aspiration of fluid and debris.

Finish. The tip shall be white and have a bright, smooth finish.

Workmanship. The tip shall be clean-cut and free from defects which detract from its appearance or impair its serviceability, proper functioning and intended use.

Unit. Package (PG). One package containing one hundred tips, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Examination and testing shall be performed to determine compliance with specification requirements.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one tip. Unless otherwise specified, sampling for dimensional examination shall be conducted at inspection level S-2, AQL 2.5 and sampling for other examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

National Stock Number	Item Identification
6520-01-173-2469	TIP, DENTAL SUCTION APPARATUS, High Volume, Double-Ended, Side-Vented, 7/16 inch by 5 inch (11.11 mm by 12.7 cm), Soft Plastic, White, Disposable, 100's

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

A-A-54397

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6520-2463
Location: PL2TIP

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

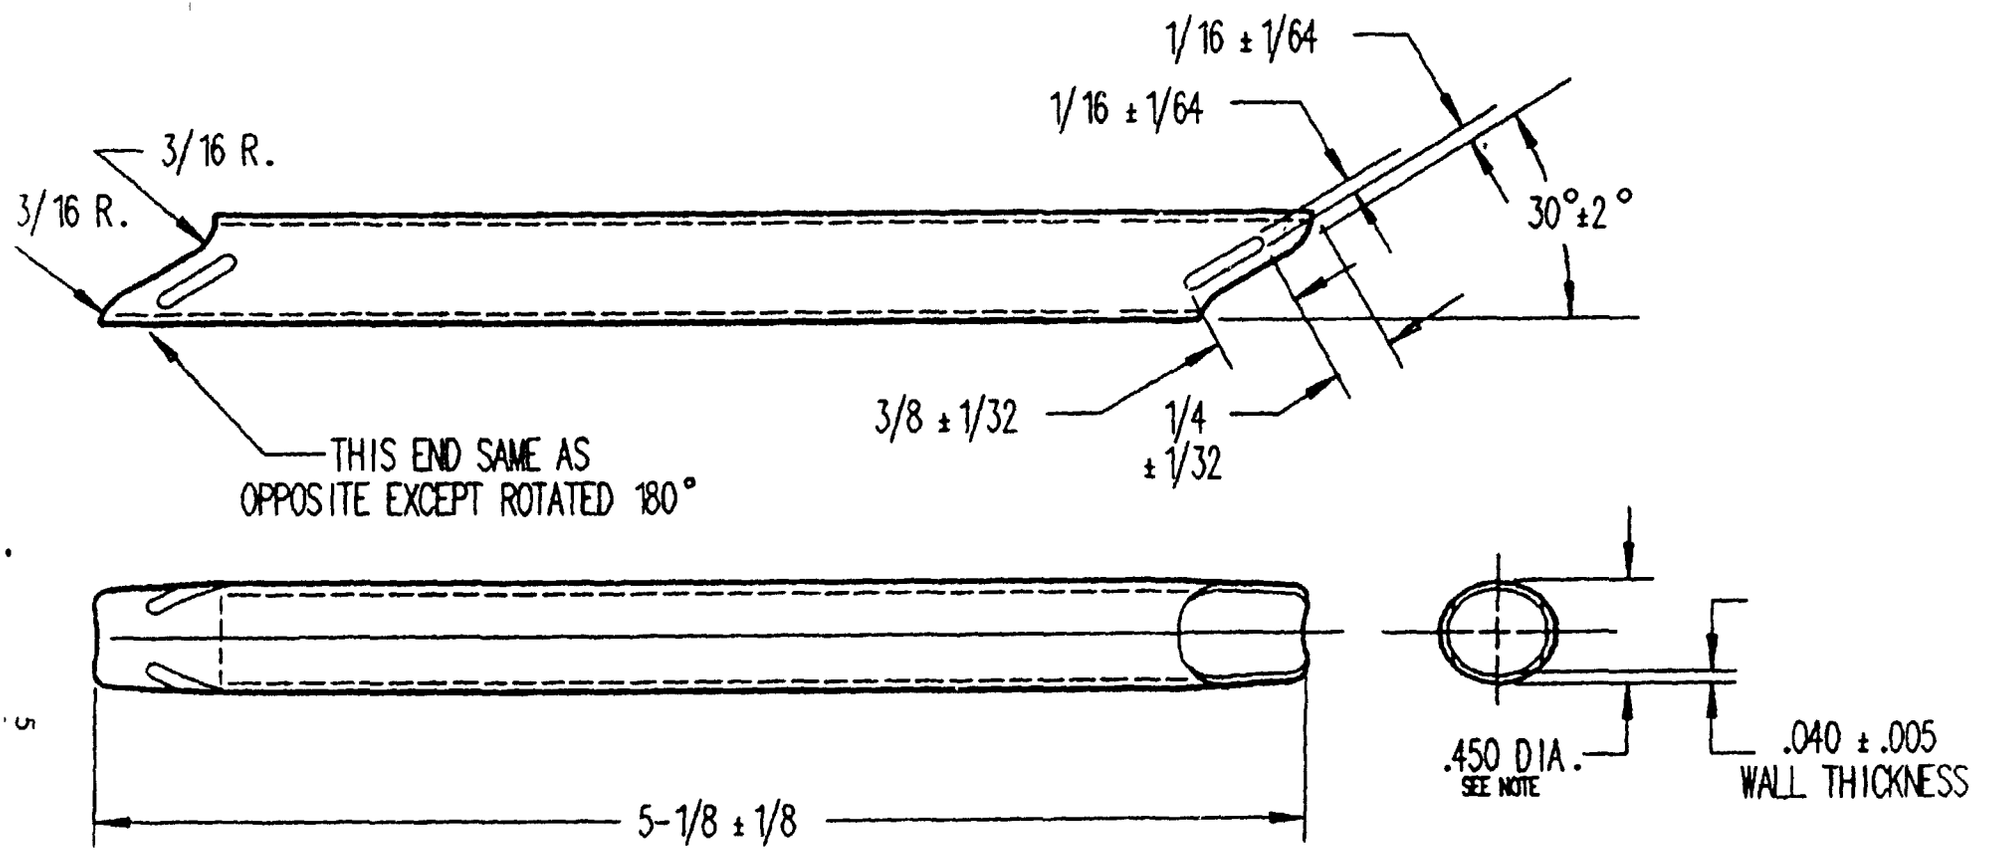

NOTE:

1. FOR TOOLING PURPOSES ONLY. PRECISE SIZES SHALL BE DETERMINED BY FABRICATOR TO FIT PROPERLY WITH STANDARD 7/16" HIGH VOLUME EVACUATION SYSTEM.

FIGURE 1 - TIP, DENTAL SUCTION APPARATUS NSN 6520-01-173-2469

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER: A-A-54397	2. DOCUMENT DATE (YYMMDD): 4-30-91

3. DOCUMENT TITLE: TIP, DENTAL SUCTION APPARATUS, PLASTIC

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable) / 7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center	(215)737-2870	444-2870
c. ADDRESS (Include Zip Code): ATTN: DPSC-MSTE, 2800 S. 20th Street, Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office, 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466, Telephone (703) 756-2340, AUTOVON 289-2340	

DD Form 1426, OCT 89 — Previous editions are obsolete — 98/298

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.