A-A-54434
25 June 1991

COMMERCIAL ITEM DESCRIPTION

DRAPE OPERATING MICROSCOPE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for MIL-D-37587 which is cancelled

This Commercial Item Description covers a sterile, disposable, plastic drape suitable for covering a surgical operating microscope

Salient Characteristics

The operating microscope drape shall be a transparent plastic sterile, disposable drape for covering a Zeiss type operating microscope its integral observer arms and supporting horizontal arm, permitting access to all controls without contamination to surgeon or staff

The drape shall be a tapered tubular type open at one end and sealed at the other See figure 1 for dimensions The open end shall have a minimum flat width The sealed end shall terminate in two eyepiece covers and shall have two observer arm covers extending from the opposite side of drape There shall be a minimum flat width of the drape at the sealed end measured at the base of the two centrally located eyepiece covers and excluding the observer arm covers All seams in the body of the drape shall be heat sealed Seams and the attachment of the lens ring, shall be continuous to maintain sterility One rubber band, suitable for attaching the drape to the eyepiece housing and conveniently located for that purpose shall be supplied for each eyepiece cover

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

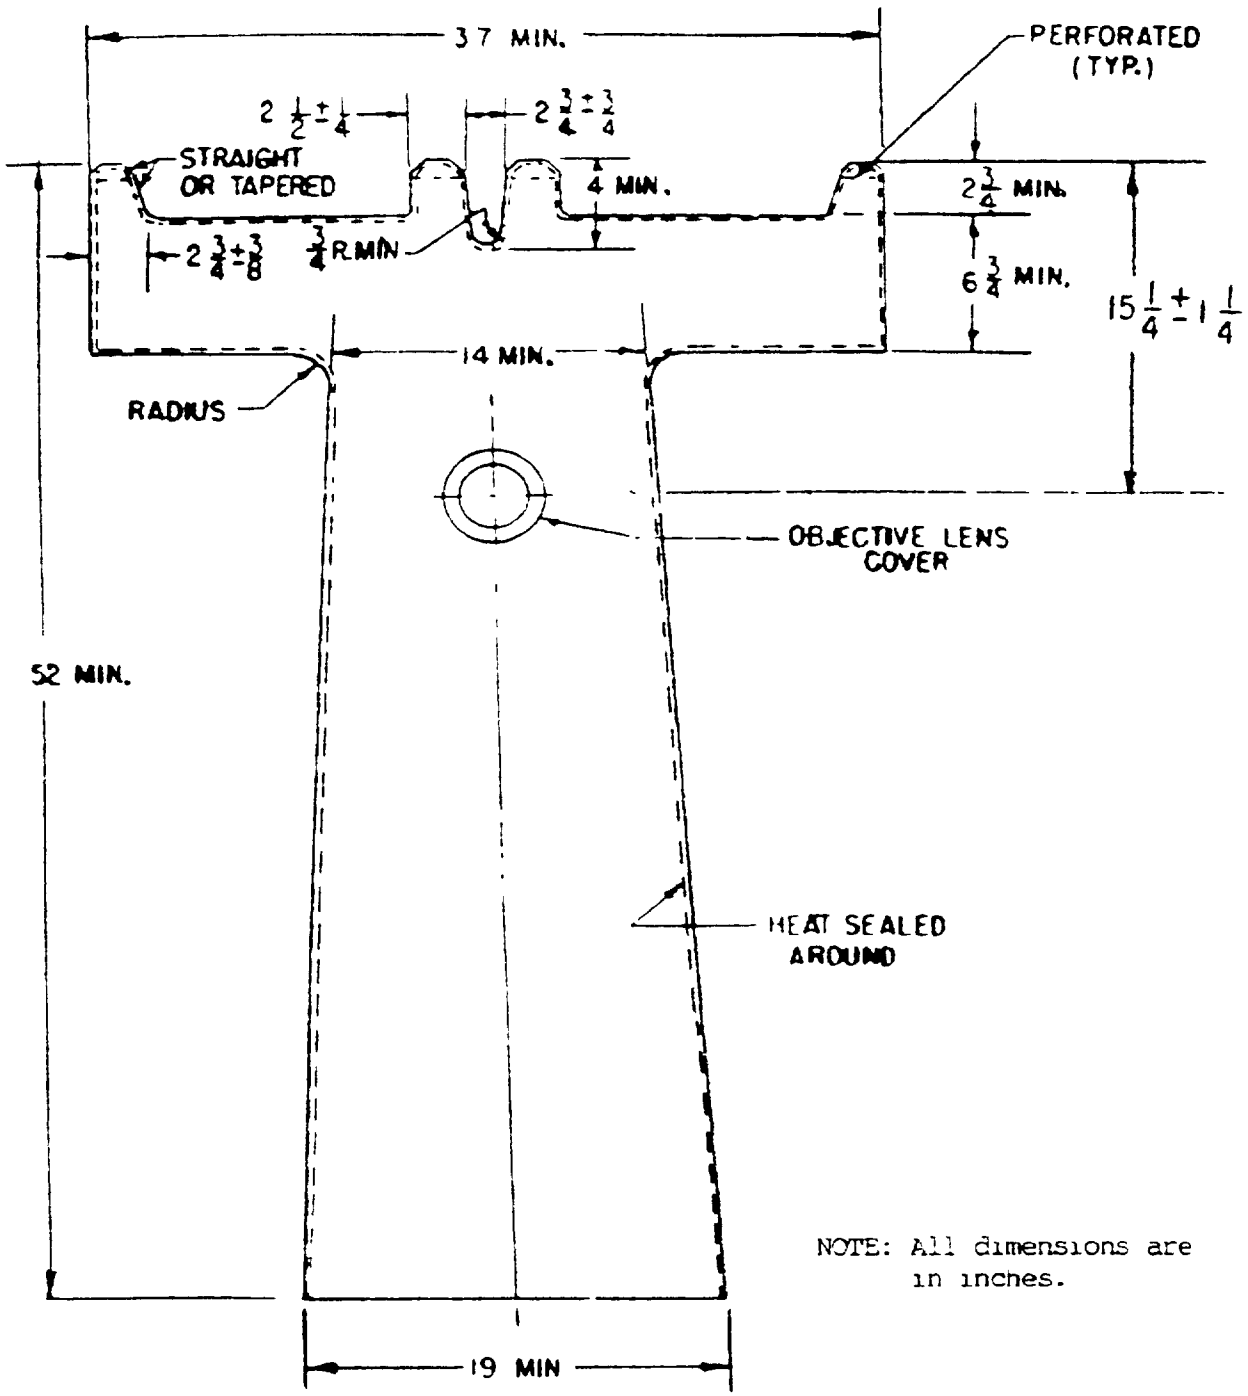


FIGURE 1. Drape, operating microscope (4 eyepieces).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

A lens ring shall be secured to the drape by means of a suitable adhesive, or by heat sealing. The lens ring shall contain a removable, optically-clear, distortion-free plastic lens cover. The lens ring shall fit snugly over an objective-lens housing having an outside diameter of 1.89 inches plus or minus 0.03 inch, and a minimum length of 0.2 inch. The lens ring shall sustain a weight of 1/2 pound without being dislodged from the lens housing.

The polypropylene film used in the body of the drape shall be approximately 0.001 inch thick and shall have the properties listed below:

Tensile strength (pounds/square inch)	
Machine direction	7,000 minimum
Transverse direction	4,000 minimum
Tear strength (grams/.001 inch)	
Machine direction	20 minimum
Cross direction	100 minimum

The polypropylene film shall be tested for tensile strength in accordance with ASTM Standard Test Method D-882, Tensile Properties of Thin Plastic Sheeting.

The film shall be tested for tear strength in accordance with ASTM Standard Test Method D-1922, Propagation Tear Resistance of Plastic Film and Thin Sheeting.

The plastic lens cover shall be free of distortion and shall have the properties listed below:

Luminous transmittance (percent)	90 minimum
Haze (percent)	1 maximum

The lens cover shall be tested for luminous transmittance and haze in accordance with ASTM Standard Test Method D-1003, Haze and Luminous Transmittance of Transparent Plastics.

The drape shall be sterile when tested for sterility in accordance with the method specified in the USP using inoculated product or paper spore strip (carrier).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

The drape body shall have no tears or holes The drape shall be free of dirt oil grease or other foreign matter The lens cover shall be free of chips cracks, or visual imperfection

Each drape shall be individually packaged in a sealed paper or plastic enclosure which will maintain sterility of the contents until opened Instructions for application shall be imprinted on each individual package

Workmanship The operating microscope drape shall be free from defects which detract from its appearance or impair its serviceability

Unit Package (PG) One package containing twelve sterile drapes as specified, constitutes one unit The individual package shall be a suitable container capable of maintaining sterility of contents unless the package is damaged or opened

Quality Assurance Provisions

Responsibility for inspection Unless otherwise specified in the contract or purchase order the contractor is responsible for the performance of all inspection requirements as specified herein Except as otherwise specified in the contract or purchase order the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein unless disapproved by the Government The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements

Records Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time or from time to time during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate

Inspection Inspection, as used herein is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

Sampling for examination Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4 0 (percent defective) and an inspection level of S-4 The unit of product for examination purposes shall be one operating microscope drape

Sampling for tests Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for test purposes shall be one operating microscope

Tests Tests shall be conducted to determine compliance with specification requirements Where feasible the same sample shall be used for the determination of two or more test characteristics

Metric products Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units a request should be made to the contracting officer to determine if the product is acceptable

The contracting officer has the option of accepting or rejecting the product

Contractor certification The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications standards, and quality assurance practices The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

Regulatory requirements

Federal Food, Drug and Cosmetic Act If the product covered by this document has been determined by the U S Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended and regulations promulgated thereunder In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances and regulations

Recovered materials The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23 4 to the maximum extent practical

Preservation, packaging, packing, labeling, and marking Unless otherwise specified preservation packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc involving shipment from the supply source to the receiving activity plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order

Ordering data Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order

NOTE The following National Stock Number is covered by this document

6530-00-420-0513

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS

Custodians

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6530-2243

Location: DRAP13A1 CID

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1 2 3 and 8 In block 1 both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4 5 6 and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I. RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54434	2 DOCUMENT DATE (YYMMDD) 25 June 1991

3 DOCUMENT TITLE
DRAPE, OPERATING MICROSCOPE

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME DEFENSE PERSONNEL SUPPORT CENTER ATTN: DPSC-MSE	b TELEPHONE (Include Area Code) (1) Commercial AC 215-737-2870	(2) AUTOVON AV 444-2870
c ADDRESS (Include Zip Code) 2800 SO. 20TH STREET PHILADELPHIA, PA 19101-8419	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041 3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete 98/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.