MIL-C-36235A
19 June 1972

SUPERSEDING
MIL-C-36235(DM)
16 July 1964

MILITARY SPECIFICATION

CHAIR, SITZ BATH, MOBILE

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of mobile, sitz bath chair, suitable for bedside treatment of patients requiring aqueous - conducted heat to perineal, genital, and rectal areas.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

QQ-A-250/8 Aluminum Alloy, 5052, Plate and Sheet.
WW-T-700/6 Tube, Aluminum Alloy, Round, Square, Rectangular, and other Shapes, Drawn, Seamless, 6061 and 6062.
PPP-B-585 Boxes, Wood, Wirebound.
PPP-B-601 Boxes, Wood, Cleated-Plywood.
PPP-B-621 Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 Box, Fiberboard.

Military

MIL-L-10547 Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-M-7298 Manual, Technical Commercial Equipment.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

Fed. Std. No. 66 Steel: Chemical Composition and Hardenability.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

UNDERWRITERS' LABORATORIES, INC. (UL)

No. 499 Standards for Safety - Electric Heating Appliances.

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., Walt Whitman Road, Melville, Long Island, New York 11749, 207 East Ohio Street, Chicago, Illinois 60611, and 1655 Scott Boulevard, Santa Clara, California 95050)

3. REQUIREMENTS

3.1 Fire and casualty hazards.

3.1.1 The contractor shall submit proof, prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of UL 499. Proof shall consist of one of the following: A UL label or UL listing of the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the UL report directly to the Contracting Officer, upon the latter's request. A laboratory report from a qualified independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with UL standards. The qualification of such laboratory shall be determined by the Government which reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified. Compliance with this paragraph does not excuse compliance with all other requirements of the contract and specifications.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

3.2 Materials.

3.2.1 Tubing. Tubing shall be 6061-T6 aluminum alloy conforming to WW-T-700/6

3.2.2 Aluminum sheet. Aluminum sheet shall be 5052-H34 alloy conforming to QQ-A-250/8

3.2.3 Corrosion-resisting steel. Corrosion-resisting steel shall be AISI 302 or 304 conforming to Fed. Std. 66.

3.3 Construction. Construction style and design shall be as shown in figure I, and as hereinafter specified. Shall be a mobile chair type sitz bath for providing aqueous conducted heat treatment to patients at bedside. Shall have a light durable frame, a backrest, four casters-two casters equipped with foot operated locking brakes, an electric heater assembly, a water pan, a seat, and a power cord. Dimensions shall be as follows:

	Inches
Overall height	34
Height of seat from floor	15-1/2
Width of frame (facing chair)	24
Depth of frame (front to back)	19

Tolerance for all dimensions shall be ± 1/2 inch. Tolerances shall not be accumulative. Commercial tolerances shall apply to all gauges specified herein.

3.3.1 Aluminum frame. The frame shall be made of round aluminum tubing. The main frame shall be 1 inch in outside diameter by 0.065 inch, No. 16 Birmingham Wire (B. W.) gage thick wall. Cross rungs shall be 3/4 inch in outside diameter by 0.049 inch No. 18 B. W. gage thick wall. Heater support rungs shall be 1/2 inch in outside diameter by 0.049 inch, No. 18 B.W. gage thick wall. The main frame may have one mechanical splice at the top center. The cross rungs shall be notched for intersection, and all notched intersections shall be aluminum brazed. The heater support rungs shall be slip jointed without brazing.

3.3.2 Backrest. The backrest shall be made of aluminum sheet, 0.064 inch thick, No. 14, Brown and Sharpe (B. and S.) gage. The ends of the backrest shall conform to the tubular frame, and shall be fastened to the frame with monel blind rivets.

3.3.3 Suspension seat. The suspension seat shall be designed to conform to the gluteal region of the patient. It shall be made with a central opening, to permit access of the solution to the affected parts and to relieve body pressure from the painful area. The seat shall be suspended from the upper front and rear cross rungs, and shall be removable for cleaning and sterilizing. The seat shall be of four-piece corrosion-

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

resisting steel construction, 0.048 inch thick, No. 18, United States Standard (U.S.S.) gage. Seat dimensions shall be 15 inches ± 1/2 inch wide by 19½ inches ± ½ inch long.

3.3.4 Water pan. The water pan, placed under the seat and suspended from the upper front and rear cross rungs, shall be removable for cleaning and sterilizing. The pan shall be of one-piece drawn construction, of stainless-steel sheet, 0.0359 inch, No. 20, U.S.S. gage in original thickness. The water pan shall be 17-1/2 inches ± 1/2 inch wide, 21 inches ± 1/2 inch long, by 7-1/4 inches, ± 1/2 inch, - 0 inch, deep. The pan shall be flanged to engage the supporting frame. A chrome-plated bronze drain cock shall be soldered to a stainless-steel nipple, which in turn is staked and soldered into the recessed hole of the pan. The pan shall have a permanent mark at the 12-quart level.

* 3.3.5 Electric heating assembly. The chair shall be provided with an electric heating assembly located under the water pan. The heating assembly shall be designed to maintain the temperature of the water, which has been preheated to 115 degrees Fahrenheit (F.) before placing in the pan, at no less than 108 ± 2°F.

The input wattage to the heater shall be 200 ± 5 percent when tested as specified in 4.4.1 Maximum temperatures of various parts of the unit shall be as follows when tested as specified in 4.4.2

Location of thermocouple	Temperature (degrees centigrade (C))
Side of heating element enclosure	96
Back of heating element enclosure	126
Outlet box	28
Entrance hole of heating element enclosure	118
Lead near heating element terminal	195
Temperature of water	45

The unit shall show no dielectric breakdown, when tested as specified in 4.4.3.

3.3.5.1 Heating element mounting plate. The heating element mounting plate shall be aluminum sheet, 0.081 inch thick, No. 12, B. and S. gage. The two long sides shall be flanged, and the two short sides shall overlap the enclosure body 1/4 to 3/8 inch to prevent entrance of water into the heating element enclosure. The mounting plate shall be fastened to the heater box with two steel, zinc-plated, sheet metal screws.

3.3.5.2 Heating element. Heating element shall be rated for 120 volts, 200 watts. The heating element shall be fastened to the mounting plate by means of two bolts.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

3.3.5.3 Heating element enclosure. The heating element enclosure shall be a long rectangular box, with the mounting plate as the top closure. Enclosure base shall be a U-shaped aluminum sheet form, 0.032 inch thick, No. 20, B. and S. gage. Enclosure dimensions shall be 15-1/2 inches ± 1/2 inch long, 5 inches ± 1/4 inch wide, and 1-3/4 inches ± 1/4 inch deep. The U-form shall be closed by two staked, lapped ends. Enclosure supports shall be two aluminum angles, 0.064 inch thick, No. 14, B. and S. gage. Fastening to the angles shall be by means of nickel-plated steel screws and self-clinching aluminum fasteners. The entire assembly shall be securely fastened to the frame with zinc-plated, steel, tube clamps.

3.3.6 Switch and timing mechanism.

3.3.6.1 Switch box. The switch box shall be drawn from a one-piece, aluminum sheet, 0.051 inch thick, No. 16, B. and S. gage. Dimensions shall be 2-1/2 by 4 by 2-1/4 inches. Tolerance shall be ± 1/4 inch for all dimensions. The box shall be secured to a chair leg by two assembly screws, threaded into a stainless-steel channel, riveted to the leg of the frame. Holes shall be provided for the flexible metallic tubing connector and supply cord strain relief. The cover shall be drawn of one-piece, aluminum sheet, 0.051 inch thick, No. 16, B. and S. gage. The cover shall be flanged to fit over the box and shall be fastened to the outlet box by two screws in the flange. Holes shall be provided in the cover for mounting the switch and switch nameplate.

3.3.6.2 Timer-Switch. A mechanical wind-up interval timer switch, having a 1-hour range, and rated at not less than 2 amperes at 125 volts, shall be provided. The timer shall have an accuracy of ± 10 percent, when tested as specified in 4.4.2.

3.3.7 Cable assembly.

3.3.7.1 Flexible metallic tubing. A U.L. listed flexible metallic tubing shall extend from the heating enclosure to the switch box. The tubing shall be provided with antishorting bushings and connectors. The metallic tubing shall be covered with listed, extruded, 105°C., polyvinyl chloride tubing.

3.3.7.2 Heater leads. Heater leads shall be No. 18 American Wire (A.W.) gage, covered with 1/32-inch-thick asbestos, and a fiber-glass outer braid.

3.3.7.3 Supply cord. The supply cord shall have a minimum length of 10 feet. The cord shall be a labeled, No. 18 A.W. gage, type SJ, three-conductor cord. The green conductor shall be grounded. The connection to the frame made within the switch box shall be by means of a solderless connector under a screw head. A strain relief of the cord in the switch box shall be provided. The attachment plug shall be a parallel-blade grounded type, rated at 15 amperes and 125 volts, and shall be provided with strain relief.

3.3.8 Casters. The four legs shall ride on double ball-bearing swivel casters. The caster stems shall be provided with steel sockets. Caster wheels shall be 3-inch conductive rubber wheels, with a minimum moving load capacity of 90 pounds per caster. The front casters shall be provided with foot-operated brakes. All casters shall be supplied with umbrella rubber bumper covers.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

3.4 Finish. The brazed frame shall be washed to neutralize brazing flux, and then polished to a satin finish. The aluminum backrest shall also have a satin finish. The corrosion-resisting steel seat and water pan shall be finished to a satin finish, or better.

* 3.5 Identification marking. The chairs shall be permanently and legibly marked with the manufacturer's name or registered trademark, the Federal stock number, contract or purchase order number, and the letters U.S. Name plates secured by adhesives shall not be acceptable.

3.6 Workmanship. Workmanship shall be first class throughout. Chairs shall be free from defects which detract from their appearance or may impair their serviceability.

3.7 Service Data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance, and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon requests to the Contracting Officer, Waiver of submission of drafts and submission of 15 additional copies shall be at the option of the Government.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the metals may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the Federal Stock Number, the Item Identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and Table I.

TABLE I

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	S-4	1.0
Minor defects	S-4	4.0
For dimensional examination	S-1	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

TABLE II

Component (unit of product)	Characteristic	Requirement	Test Procedure	Inspection level	AQL
Heater	Input wattage	3.3.5	4.4.1	S-2	*
Timer switch	Accuracy	3.3.6.2	4.4.2	S-2	*
Chair	Normal temperature	3.3.5	4.4.2	S-2	*
Chair	Dielectric strength	3.3.5	4.4.3	100%	*

* Not less than three samples shall be taken regardless of lot size. Acceptance number shall be zero for all sample sizes.

4.3 Examination. The chairs shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects as shown in Table III.

TABLE III CATEGORIES AND DEFECTS *

CATEGORIES	DEFECTS
MAJOR	
101	Any component missing, incomplete or damaged.
102	Exposed edges not free of burs or sharpness.
103	Any part misplaced, loose, not in proper alignment.
104	Any weld cracked, broken, or not sound.
MINOR	
201	Unit not clean, not free of dirt, oil and grease.
202	Identification marking not present, complete, legible, not permanently attached.
203	Service data not supplied.
204	Casters and caster brakes not free moving.
205	Finish not as specified, not free of scratches, blemishes.

* Examination shall not be restricted to the classified possible defects listed above.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Wattage. The heater shall be connected to a circuit with voltage adjusted to 120 volts, and the wattage shall be measured with a wattmeter.

4.4.2 Normal temperature. Thermocouples shall be attached at the various points specified, and the heater shall be connected to a circuit with

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

the voltage adjusted to give an input of 200 watts. The water pan shall be filled to the mark with tap water at 45°C. The test shall be conducted in an ambient temperature of 21° to 27° (C). The heater shall be started and set for a full hour. The time (using an accurately calibrated watch) and temperature readings shall be recorded during the 1-hour period of operation. The water temperature shall be determined by a suitable thermometer. Other temperatures shall be measured by means of thermocouples and a temperature-indicating instrument. The test shall be allowed to continue until the timer switch shuts off the mechanism.

4.4.3 Dielectric strength. A gradually rising potential, from 0 to 1000 volts plus twice the rated voltage alternating current, shall be applied across current-carrying parts and metal non-current-carrying parts. The voltage shall be maintained for a period of 1 minute.

5 PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.4).

5.1.1 Unit of issue. One chair, as specified, constitutes one unit of issue.

5.1.2 Level A

5.1.2.1 Unit preparation. Each unit shall be disassembled as far as is practicable. Exterior surfaces shall be effectively protected by wrapping and cushioning material to ensure against damage. Component shall be packaged in cartons of appropriate size and design. Closure of containers shall be adequate to prevent accidental opening.

5.1.3 Level C. Units shall be prepared for shipment which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.4).

5.2.1 Level A

5.2.1.1 Exterior container. Each unit shall be packed in a exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601 overseas type; PPP-B-621, class 2. Closure and strapping shall be as specified in the appendix of the applicable box specification. Each unit and component parts shall be blocked and braced to prevent damage to contents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.2 Level B.

5.2.2.1 Exterior container. Each unit shall be packed in a exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, type 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Each unit shall be blocked and braced to prevent damage to contents.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use: Bedside treatment of patients requiring aqueous conducted heat to perineal, genital, and rectal areas, in military medical facilities.

6.2 A suitable heating element is the "Chromalox" completely enclosed strip heater, rated at 200 watts, 115 volts, manufactured by the Edwin L. Wiegand Co., Pittsburgh, Pa., as Model No. SE1405W.

6.3 A suitable switch is manufactured by the Lux Clock Manufacturing Co., Waterbury, Conn., as Model No. 1500.

6.4 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

* 6.5 This specification covers the following item appearing in the Federal Supply Catalog

Stock Number	Item Identification
6530-896-1465	Chair, Sitz Bath, Mobile, 110 Volt, 60 Cycle, AC

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

6.6 This specification does not include all types, classes, grades, and sizes, of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, which are normally procured to meet Military requirements.

6.7 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.


Custodians:
Army.-MD
Navy.-BuMed
Air Force.-AFMSC

Review activities:
Army.-MD
Navy.-BuMed
Air Force.-AFMSG

Preparing activity:
Defense Supply Agency.-DM
Project No. 6530-1166

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation shall be based on the information in the current DODISS

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

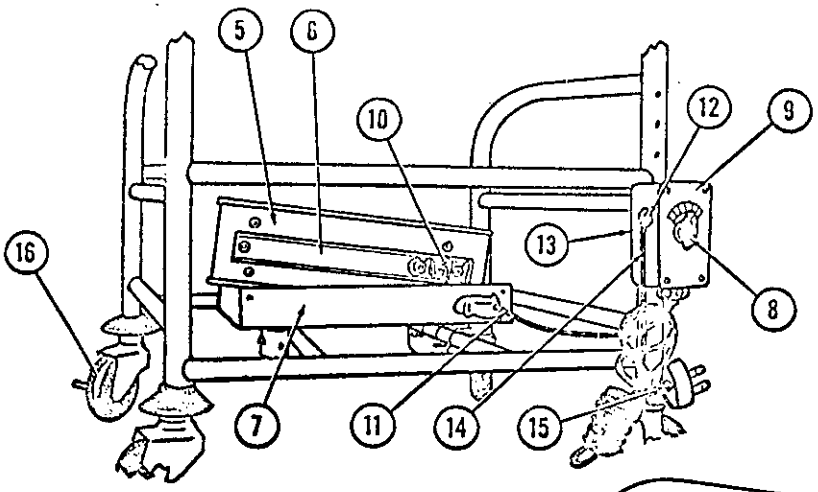

Key

1. Frame
2. Seat
3. Water Pan
4. Backrest
5. Mounting Plate Heating Element
6. Heating Element
7. Heating Element Enclosure
8. Switch
9. Switch Box Cover
10. Heater leads
11. Flexible Metallic Tubing
12. Strain Relief and Bushing
13. Switch Box
14. Supply Cord
15. Attachment Plug Cap
16. Casters

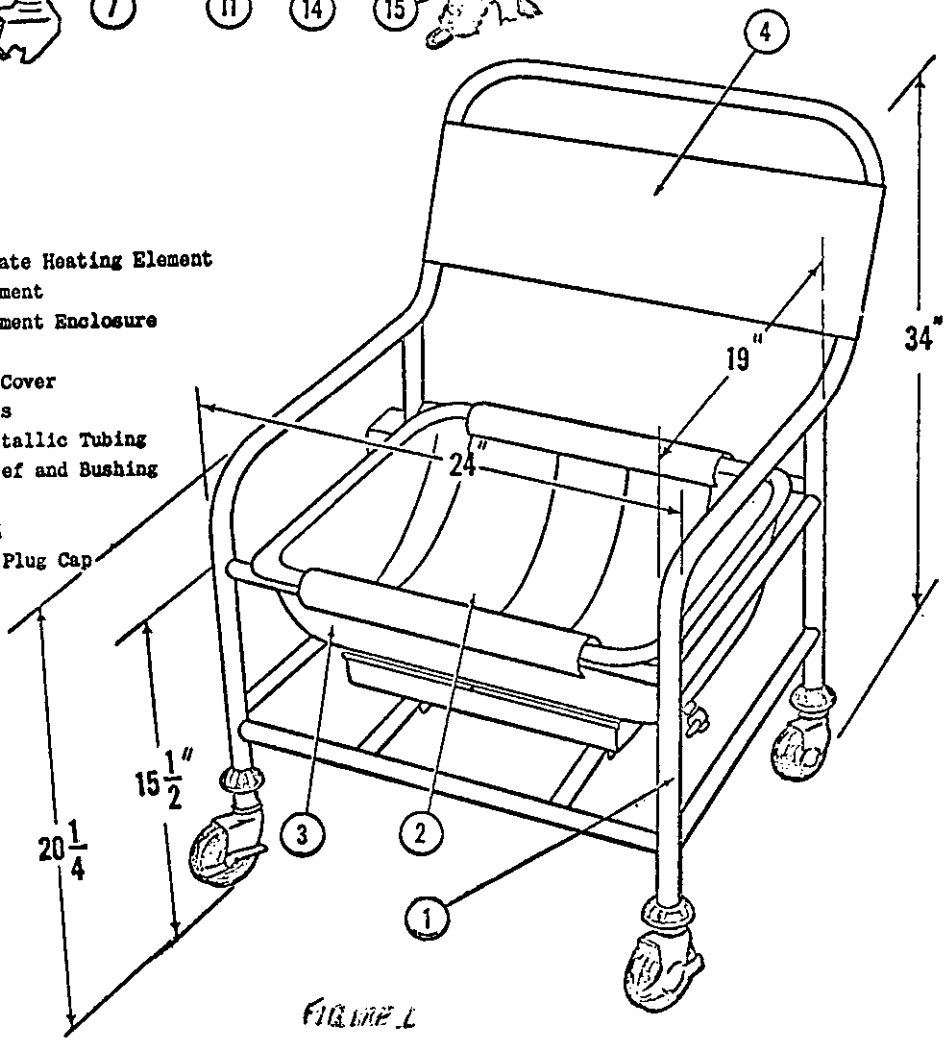


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE: MIL-C-36235A

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

Defense Supply Agency

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DOD-304



HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:15Z
Check the source to verify that this is the current version before use.