MILITARY SPECIFICATION

INDICATOR, CLINICAL CHART HOLDER, METAL, 12s

1. SCOPE

1.1 This specification covers one type of visual indicator, suitable for directing attention to individual clinical chart holders in military medical treatment facilities.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-up, Paperboard.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper, Water-Resistant (for Carton Sealing).

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material. All material used in the construction of the indicator shall be of the quality best suited for the purpose.

3.2 Construction. The indicator shall consist of a slide receiver with a length of pressure sensitive adhesive tape on the back and a slide which may be positioned manually to expose or cover a colored "flag". The indicator shall be in strict accordance with figure I.

3.2.1 Slide receiver. The slide receiver shall be a length of aluminum, "C" section channel designed to retain the slide when the unit is assembled. The back of the channel shall contain two holes located to mate with a spring loaded ball in the slide. Tabs shall be turned up at either end of the receiver to limit the travel of, and to retain the slide in the receiver when the device is assembled. The right end of the receiver shall be lined with a brilliant red paper or other suitable material, to serve as a visual indicator or "flag", when uncovered by moving the slide to its left most position.


3.2.2 Slide. The slide shall be a flat metal piece designed to fit into, and slide in, the "C" channel retainer. It shall be retained by the lip of the "C" and shall slide freely along the receiver. The slide shall cover and uncover the red "flag" on the receiver in its extreme positions. The slide shall be fitted with a knob for moving it in the receiver. The knob shall contain a spring loaded ball which shall mate with the holes in the receiver channel back to locate and hold it in its extreme position, until deliberately moved.

3.2.3 Tape. A length of double faced pressure sensitive tape shall cover the back of the slide receiver. The other side of the tape shall be protected with a removeable paper covering. The tape shall be adequate to provide mounting of the unit on a chart holder securely enough to permit normal operation and to prevent inadvertent removal.

3.3 Identification marking. The indicator shall be clearly and permanently marked with the name or registered trademark of the manufacturer.

3.4 Workmanship. Workmanship shall be first class throughout. The indicators shall be free from defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 20260-21T08:16Z
Check the source to verify that this is the current version before use.

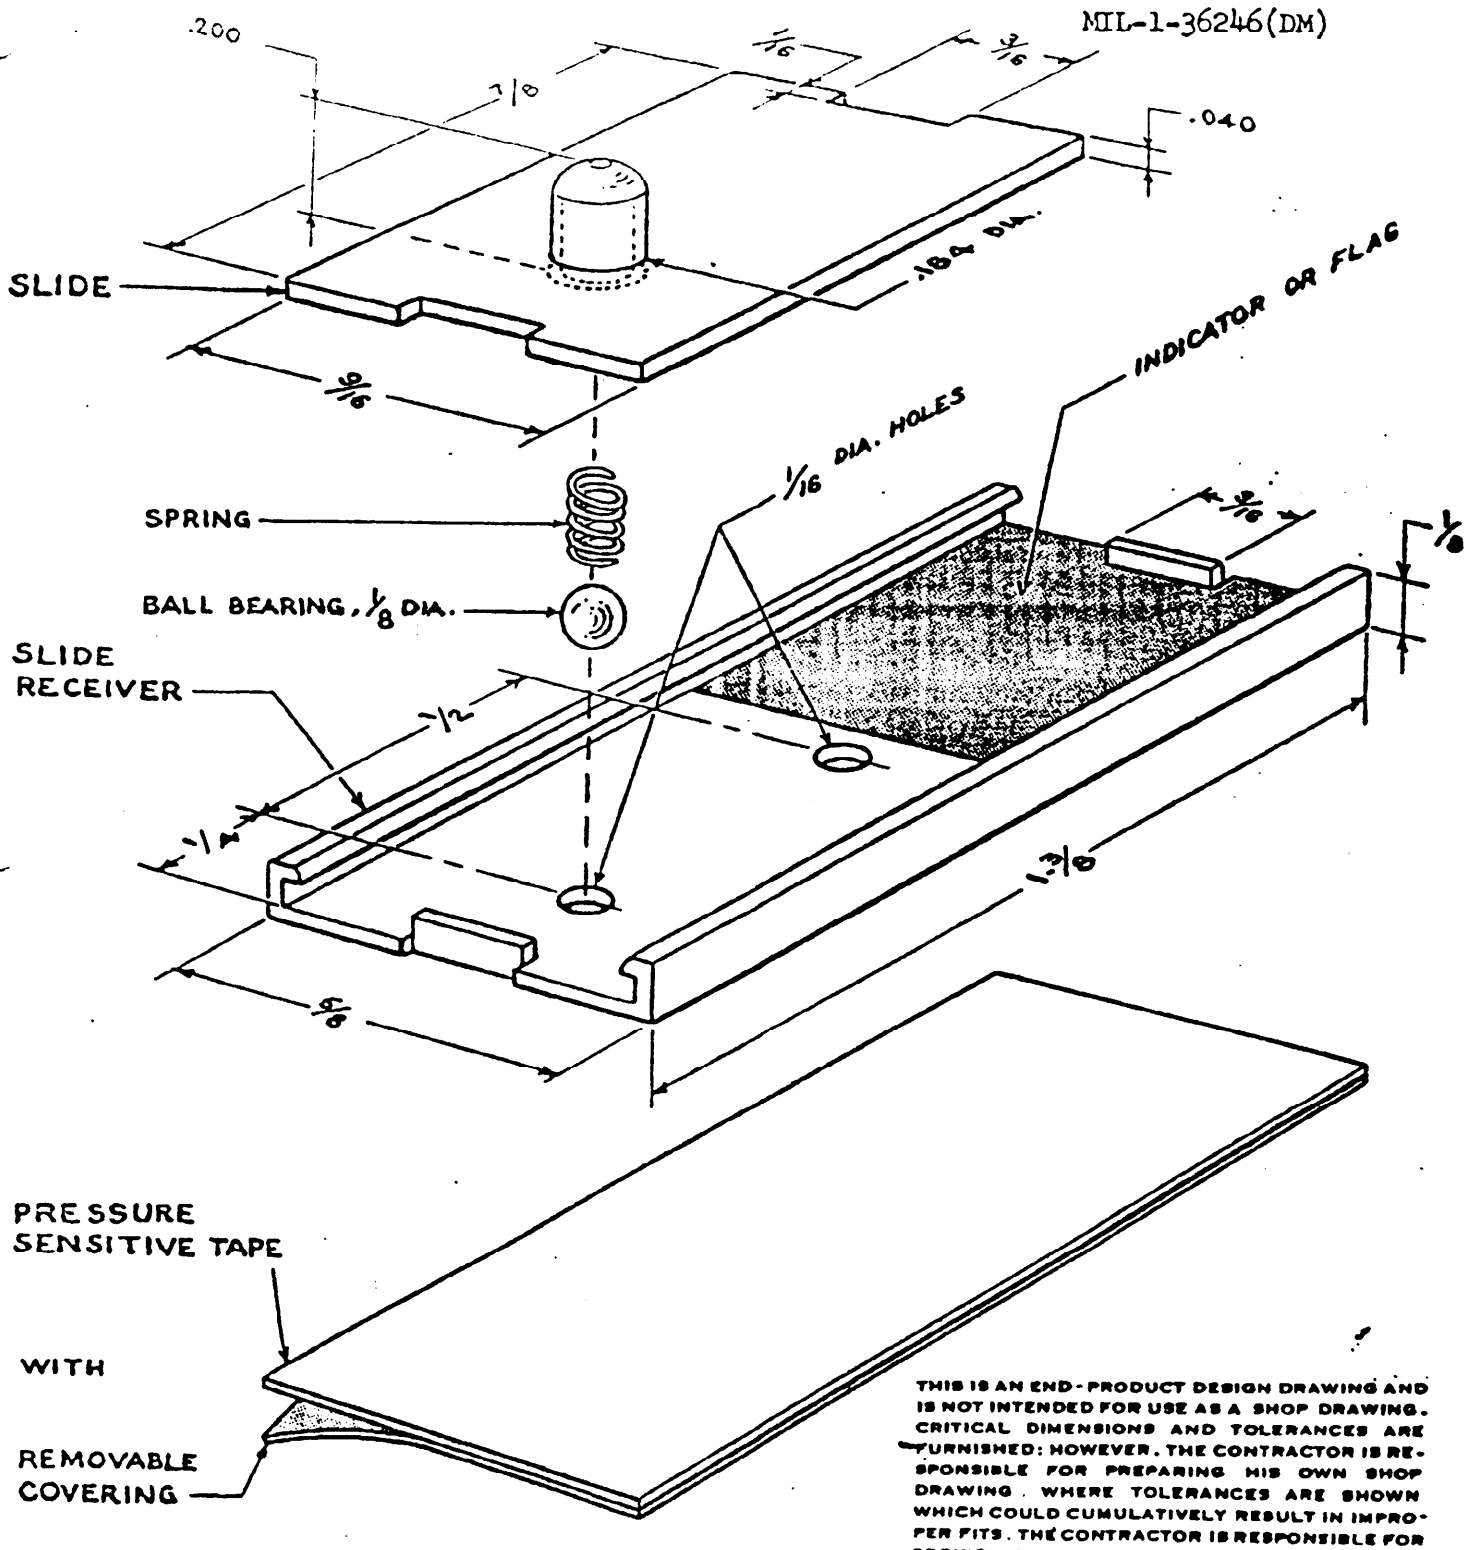

THIS IS AN END-PRODUCT DESIGN DRAWING AND IS NOT INTENDED FOR USE AS A SHOP DRAWING. CRITICAL DIMENSIONS AND TOLERANCES ARE FURNISHED: HOWEVER, THE CONTRACTOR IS RESPONSIBLE FOR PREPARING HIS OWN SHOP DRAWING. WHERE TOLERANCES ARE SHOWN WHICH COULD CUMULATIVELY RESULT IN IMPROPER FITS, THE CONTRACTOR IS RESPONSIBLE FOR PROVIDING TOLERANCES IN ACCORDANCE WITH GOOD COMMERCIAL PRACTICE WITHIN THOSE INDICATED ON THIS DRAWING TO INSURE PROPER FIT AND ASSEMBLY.

INDICATOR,
CLINICAL, CHART HOLDER, METAL, 12"
6530-890-1882

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.

FIGURE 1.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with Standard MIL-STD-105.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	2.5
Minor defects	II	4.0
For dimensional examination	S-1	2.5

4.3 Examination. The indicators shall be examined to determine compliance with all requirements contained in this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects *

Major

101	Any component missing.
102	Any component fractured, split, cracked, punctured, cut, dented, sprung, malformed, creased, or otherwise impaired, affecting serviceability.
103	Any part misplaced, loose or not in proper alignment, affecting serviceability.
104	Indicator not free of sharp edges, burs, or slivers.
105	Any operation omitted or not properly performed.
106	Any functioning component inoperative or will not operate as intended.

Minor

201	Pressure sensitive adhesive tape not properly mounted on slide receiver.
202	Protective covering for tape not properly in place.
203	Slide sticks or is not easily operable.
204	Identification marking missing, not correct, not permanent, not legible, or not complete.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The indicators shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. Twelve (12) indicators, as specified, constitutes one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.

5.1.2 Packaging quantities. The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table I. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	144 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676, except that commercial colors shall be acceptable. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.3.2 Intermediate package. Intermediate package shall be a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676, except that commercial colors shall be acceptable, or PPP-B-636. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with Federal Specification PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type I, class 2.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to Military Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:16Z
Check the source to verify that this is the current version before use.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix of Federal Specification PPP-B-636. In addition, all seams, including manufacturer's joint, shall be closed by tape conforming to the requirements of Federal Specification PPP-T-76. The tape shall be not less than 2 inches wide. Three strips shall be applied to both top and bottom so that all seams and joints shall be covered their full length. Tape applied over the lengthwise seams shall extend a minimum of 2 inches onto each of the end panels. Tape applied over the end edge seams shall extend a minimum of 2 inches along the side and top, and side and bottom panels.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to Federal Specification PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with Federal Specification PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type I, class 1.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with Military Standard MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with Military Standard MIL-STD-129. In addition, the letter "L" shall precede the Federal stock number. One space shall be allowed between the letter "L" and the first digit of the stock number. The terms "Stock number" or "FSN" shall not be indicated.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. The indicator shall be designed to operate with the following item:

Stock No.	Item Identification
6530-781-8535	HOLDER, CLINICAL CHART

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

Custodians:
Army. - MD
Navy. - BuMed
Air Force. - AFMSHB (03)

Review activities:
Army. - MD
Navy. - BuMed
Air Force. - AFMSHB (03)

Preparing activity:
Defense Supply Agency. - DH

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

FORM APPROVED BUDGET BUREAU NO. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use of the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity.

SPECIFICATION: MIL-I-36246 (DM) Indicator, Clinical Chart Holder, Metal, 12s, Dated 23 July 1964

ORGANIZATION	CITY AND STATE

CONTRACT NO.	QUANTITY OF ITEMS PROCURED	DOLLAR AMOUNT
		$

MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

   A. GIVE PARAGRAPH NUMBER AND WORDING

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

   ☐ YES ☐ NO IF "YES" IN WHAT WAY?

4. REMARKS (ATTACH ANY PERTINENT DATA WHICH MAY BE OF USE IN IMPROVING THIS SPECIFICATION. IF THERE ARE ADDITIONAL PAPERS, ATTACH TO FORM AND PLACE BOTH IN AN ENVELOPE ADDRESSED TO PREPARING ACTIVITY)

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:16Z
Check the source to verify that this is the current version before use.

SUBMITTED BY (PRINTED OR TYPED NAME AND ACTIVITY)

FOLD

DEFENSE SUPPLY AGENCY
DEFENSE MEDICAL SUPPLY CENTER
3RD AVENUE AND 29TH STREET
BROOKLYN, N.Y., 11232

OFFICIAL BUSINESS

POSTAGE FEES PAID
DEFENSE SUPPLY AGENC

Defense Supply Agency
Defense Medical Supply Center
ATTN: Directorate of Technical Operations (Code T-H5)
3rd Avenue and 29th Street
Brooklyn, N.Y., 11232

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:16Z
Check the source to verify that this is the current version before use.