MIL-T-36295A
29 September 1977
SUPERSEDING
MIL-T-36295
5 October 1964

MILITARY SPECIFICATION

TABLE, EXAMINING AND TREATMENT, CABINET TYPE, STEEL, ENAMELED

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of enameled, steel, cabinet-type, examining table with an adjustable, upholstered top.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

QQ-Z-363	- Zinc Base Alloy; Die Castings.
ZZ-C-450	- Cloth, Coated (Rubber and Plastic) and Plastic Sheeting for Hospital Use.
CCC-A-680	- Artificial Leather (Cloth Coated), Vinyl Resin, Expanded Layer, (Upholstery).
DDD-C-95	- Carpet and Rug, Wool, Nylon, Acrylic, Modacrylic.
PPP-B-640	- Box, Fiberboard, Corrugated, Triple-wall.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

MILITARY

MIL-P-116 - Preservation-packaging, Methods of.

STANDARDS

FEDERAL

FED-STD-No. 66 - Steel, Chemical Composition and Hardenability.
FED-TEST-METHOD-STD-No. 151 - Metals; Test Methods.
FED-TEST-METHOD-STD-No. 191 - Textile Test Methods.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

U. S. DEPARTMENT OF COMMERCE

Commercial Standard CS 236 Mat-Formed Wood Particleboard.

(Copies of Commercial Standard CS 236 may be obtained upon application, accompanied by money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington, DC 20406. Price may be obtained from the Superintendent of Documents.)

UNDERWRITERS' LABORATORIES, INC.

UL 65 - Wired Cabinets.
UL 498 - Attachment Plugs and Receptacles.

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., 207 East Ohio Street, Chicago, IL 60611, 333 Pfingsten Road, Northbrook, IL 60062, 1285 Walt Whitman Road, Melville, LI, NY 11746, 1655 Scott Blvd., Santa Clara, CA 95050.)

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:21Z
Check the source to verify that this is the current version before use.

AMERICAN NATIONAL STANDARDS INSTITUTE (ANSI)

ANSI C73.11 Plugs and Receptacles - General Purpose, 125 volt, 15 amperes, 2 pole, 3 wire, Grounding Type.

(Application for copies should be addressed to the American National Standards Institute, 1430 Broadway, New York, NY 10018.)

AMERICAN SOCIETY FOR TESTING & MATERIALS (ASTM)

A-591 Sheet Steel, Cold-Rolled, Electrolytic Zinc-Coated.
D-751 Coated Fabrics.
D-2406 Flexible Cellular Materials - Molded Urethane Foam.

(Application for copies should be addressed to the American Society for Testing & Materials, 1916 Race Street, Philadelphia, PA 19103.)

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Fire and casualty hazards.

3.2.1 The contractor shall submit proof, prior to delivery, that the cord, plug, and receptacle included in the table to be delivered under the contract conform to the applicable requirements of Underwriters' Laboratories, Inc. (U.L.) Standard of Safety UL 498. Proof shall consist of one of the following:

a. U.L. label affixed to the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the U.L. report directly to the Contracting Officer, or the Government Inspector, upon request.

b. Laboratory report from a nationally recognized independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with U.L. standards. The Government reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified. Compliance with this paragraph does not excuse compliance with all other requirements of the contract and specifications.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

3.3 Materials.

3.3.1 Corrosion-resisting steel. Corrosion-resisting steel shall comply with AISI 300 series of FED-STD-No. 66 when tested as specified in 4.5.1. Standard commercial tolerances shall apply to thickness.

3.3.2 Carbon steel. Carbon steel shall be cold-rolled, electrolytic zinc-coated in accordance with ASTM A591. Standard commercial tolerances shall apply to thickness.

3.3.3 Zinc alloy. Zinc-base alloy shall conform to QQ-Z-363.

3.3.4 Particleboard. Particleboard shall conform to Type 1, Density B, class 2 of CS-236.

3.3.5 Upholstery. Upholstery material shall consist of a polyvinyl chloride resin or copolymer thereof, suitably compounded to form an expanded material with an unexpanded surface skin. The resulting material shall be supported with a synthetic material, and shall form satisfactorily in a vacuum forming operation. The color shall be black, dark brown, or dark green. The material shall meet the following requirements when tested as specified in 4.5.2.

TABLE I. Upholstery material, requirements.

Characteristics	Units	Value
Weight		
Solid vinyl skin	ounces/square yard	22.5 min.
Expanded layer	ounces/square yard	13.5 min.
Supporting fabric	ounces/square yard	2.0 min.
Total	ounces/square yard	39.0 min.
Thickness	inches	.058 min.
Tensile strength		
Warp	pounds	100 min.
Filler	pounds	100 min.
Tear strength		
Warp	pounds	20 min.
Filler	pounds	20 min.
Cold crack resistance	degrees	-20°F (-29°C) Max.
Wear resistance (surface skin)	cycles at 1000 grams load	4,000 min.
Burn time	seconds	2 max.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

3.3.6 Foam padding. Foam padding shall be polyurethane which meets the following requirements when tested as specified in 4.5.3.

TABLE II. Foam padding, requirements.

Characteristic	Units	Value
Density	pounds/cubic foot	2.5 ± 0.2
Indentation load deflection (25% for 4-inch thickness)	pounds	35 ± 7
Steam autoclave, load loss	percent	20 max.
Flame retardance, burn diameter	inches	2 max.

3.4 Design and construction. The table shall consist of an adjustable, upholstered top mounted on a welded steel cabinet-type body. The body shall be bolted to a welded steel base. Figure 1 illustrates a typical configuration.

3.4.1 Upholstered top. The upholstered top shall consist of a head-end and foot-end section. Each section shall be covered with a contoured, thermo-formed vinyl-over-fabric upholstered over a molded cushion of polyurethane foam. The top and side edges shall be raised for patient security. The upper portion of the head section shall be raised for a length of 13 ± 1 inch, to serve as a pillow. The foot-end section shall have a perineal cutout and a separate filler, upholstered in the same manner, for the cutout section. The entire top shall be upholstered over particleboard at least 5/8 inch thick. The upholstery shall have a minimum thickness of 1-1/2 inches. The head-end and foot-end shall be joined by a combination of angle iron with 5 hinges or with a piano hinge. If 5 hinges are used, each hinge shall be at least 2 inches wide and 1/16 inch thick.

3.4.1.1 Head end elevating and locking mechanism. The head end of the upholstered top shall be adjustable to any desired angle, up to and including 85 degrees, and shall lock in place by a 9/16 inch diameter round elevating rod and eccentric plate friction-type lock, controlled by a handle. The lock shall be positive in action throughout the adjustable range of the top. The elevating rod shall be securely hinged to the top section. The friction plate locking device shall be spring loaded to hold the elevating rod in the locked position. Where the rod enters the body section, there shall be a length of 1-1/2 x 1-1/2 inch square tubing not less than .065 inch thick (No. 16 Birmingham wire gage (BWG)) with 6 x 3 x 1/8 inch plates welded to each end of the square tubing; the square plates shall be spot welded to the body side panel, to serve as the rod bearing. The head end of the top shall show no distortion or failure to operate smoothly when tested as specified in 4.5.4.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

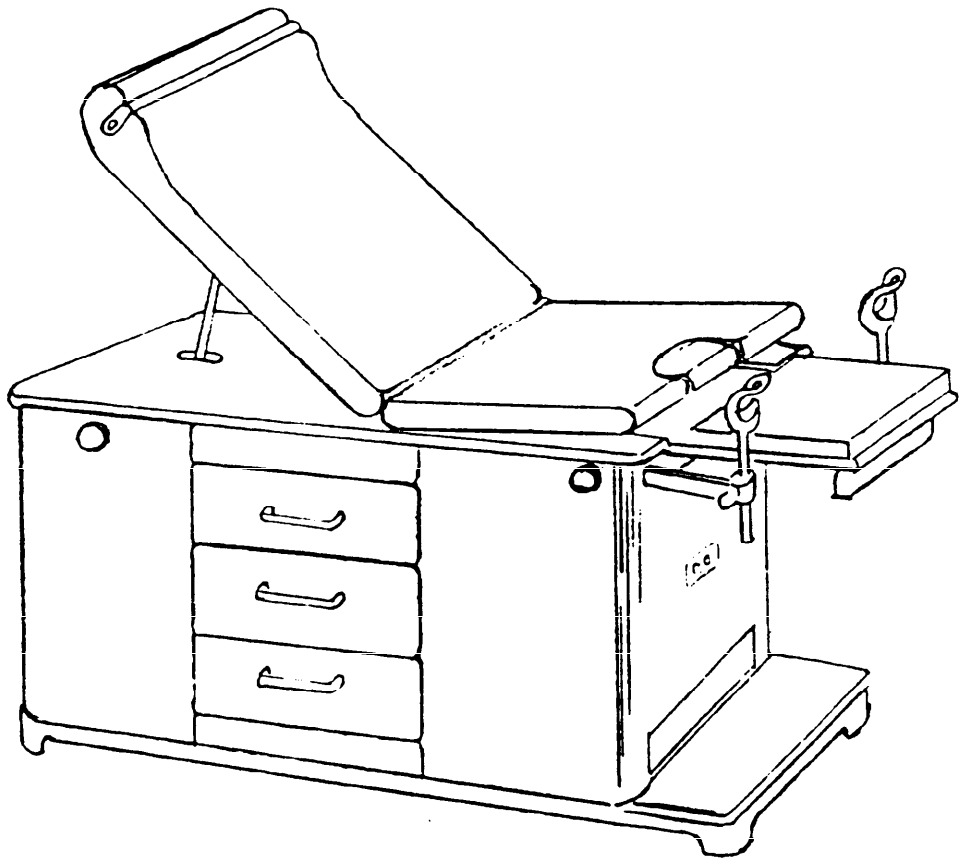


FIGURE 1. Table (Typical Configuration).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

3.4.1.2 Foot end raising device. The foot end of the top shall be provided with a raising device which shall raise the foot section not less than 3-1/2 inches.

3.4.1.3 Foot end protector bib. The foot end of the top shall have a protector bib made of type I, color 3, white-coated cloth in accordance with ZZ-C-450. The bib shall cover the entire foot section and shall have a matching perineal cutout. The bib shall be held in place by four snap fasteners. Each button on the bib shall have a vinyl tab to prevent the rubber from tearing when pulling the bib fron the snap fasteners.

3.4.1.4 Concealed paper roll attachment. The head end of the table shall be equipped with a concealed paper roll attachment for holding rolls of paper 18 inches wide x 3-1/2 inches in diameter. A steel spring shall be provided under the head to hold the paper tight on the roll. The top shall be equipped with two paper clamps at the foot end, and one plastic combination retaining-strap and paper-cutter at the head end. The paper attachment shall be equipped with a 3/8 inch diameter steel rod to accommodate the paper roll.

3.4.2 Body of table. The body of the table shall be formed of carbon steel, not less than .0359 inch thick (No. 20 Manufacturers' Standard gage). The body shall be 44-1/2 to 45-1/2 inches long, 18-1/2 to 22-3/4 inches wide, and 20 to 23 inches high. The long sides shall each consist of two panels, spotwelded together. The corners of the body shall have not less than a 1 inch radius. A subtop of carbon steel, not less than 0.060 inch thick (No. 16, Manufacturers' Standard gage), having an overhang of 3/4 ± 1/4 inch and corners of not less than 1 inch radius, shall be securely spotwelded to the body. The left side of the body (when viewed from the foot end) shall be equipped with a drawer and a storage compartment or, as an alternate, three drawers. The foot end of the body shall contain two stirrups, a sliding leg rest, and a duplex electrical outlet. A kick plate, at least 14-3/4 inches by 2-3/4 inches, made of corrosion-resistant steel not less than .037 inch thick (No. 20, United States Standard (USS) gage), shall be centered on the foot end directly above the mounting step. The kick plate shall be secured by six aluminum pop rivets. The body shall be bolted securely to the base. Spaces around door and drawer openings shall be uniform and shall not exceed 1/16 inch.

3.4.2.1 Storage compartment. The storage compartment, when supplied, shall be located directly underneath the drawer. Inside dimensions shall be 45 ± 1 inch long by 19 ± 1 inch deep by 15 ± 1/2 inch high. Storage compartment door shall be of double-wall construction with a suitable sound-deadening material between the walls. Walls shall be carbon steel; the outer wall shall be not less than .0359 inch thick (No. 20, Manufacturers' Standard gage) and the inner wall not less than .0239 inch thick (No. 24 Manufacturers' Standard gage). The door shall have concealed hinges and shall close flush with the outside of the body, against rubber bumpers. The door shall have a knob and a spring-catch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

3.4.2.2 Alternate Storage. As an alternate to the storage compartment, the table shall have a total of three drawers, identical to the drawer specified in 3.4.2.3, aligned vertically, as illustrated in figure 1.

3.4.2.3 Drawer. The drawer shall be formed of carbon steel. The inside of the drawer shall measure 15-1/2 ± 1 inches wide, 15 ± 1-1/4 inches from front to back, and 3-3/4 ± 1/4 inches high. The front shall be of double-wall construction with a suitable sound-deadening material between the walls. The outer wall shall be not less than .0359 inch thick (No. 20, Manufacturers' Standard gage) and the inner wall not less than .0239 inch thick (No. 24, Manufacturers' Standard gage). Total thickness of the flush-fitting drawer front shall be 3/4 ± 1/6 inch. The drawer shall close against rubber bumpers and shall be fitted with safety stops, which will prevent inadvertent removal of the drawer, but permit it to be removed for cleaning. The drawer shall open and close smoothly on drawer guides made of carbon steel at least .0598 inch thick (No. 16, Manufacturers' Standard gage). A suitable drawer pull shall be provided.

3.4.2.4 Stirrups. There shall be two carbon steel, or zinc alloy stirrups at the foot end of the table. The stirrups shall extend to at least 18 inches from the foot end of the table on adjustable extension rods, each extending out from the table at an angle of 14 ± 3 degrees with respect to the long axis of the table. Each stirrup shall be attached to a supporting rod at least 10 inches long. Suitable locks shall permit the stirrups to swivel, to be adjustable in height and extension length, and to lock in any position. Stirrups, supporting rods, extension rods, and hardware shall be chromium-plated. Stirrups and supporting system shall exhibit no permanent distortion when tested as specified in 4.5.5.

3.4.2.5 Sliding leg rest. At the foot end of the table there shall be a sliding leg rest. The leg rest shall be provided with an upholstered cushion. When fully extended, the top of the leg rest shall be level, within plus 1/2 inch, minus 1-1/2 inches, with the top of the upholstered top section. The leg rest shall extend 18-1/2 ± 1/2 inches beyond the end of the upholstered top when fully opened, and not more than 1-1/2 inches beyond the upholstered top in the closed position. The support shall be constructed of 5/8 inch particle-board and upholstered in the same manner as the top (3.4.1). The cushion shall be removable to permit access to a removable, corrosion-resisting steel treatment basin 9-1/8 ± 1/4 inches long by 11-1/2 ± 1/4 inches wide, by 3-1/4 ± 1 inches deep with a 5/8 ± 1/16 inch flange around the top.

3.4.2.6 Electrical outlet. At the foot end of the table there shall be mounted an enclosed duplex electrical receptacle. The receptacle shall be connected to 10 feet of No. 14, 3-conductor, rubber covered cord, complete with a male, 125 volts, 15 amperes, 2-pole grounding-type plug conforming to ANSI C73.11. Both the plug and the receptacle shall be Hospital Grade, as specified in UL 498. The cord shall come out of the table bottom through a hole fitted with a rubber grommet. The wiring shall be attached to the walls of the cabinet in such a manner that opening and closing the drawer shall not damage the wires. Wiring shall conform to UL Standard 65.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

3.4.3 Base. The base shall be formed of carbon steel, not less than .0478 inch thick (No. 18, Manufacturers' Standard gage). The base shall be flush with the body, within + 1/8 inch on all sides, and shall have a clearance of not less than 3-1/2 inches above the floor, except in the vicinity of the legs. The lower edge shall be folded under at a right angle or hemmed for at least 1/4 inch. The four corners of the base shall be reinforced by legs, 6 + 1/4 inches long, constructed of carbon steel tubing at least .065 inch thick (No. 16, B.W.G.). Each leg shall terminate in a metal or plastic glide. The foot end of the base shall extend the entire width of the table and 8 + 1/4 inches beyond the body to accommodate the mounting step. The mounting step shall be made of 5/8 inch particleboard 8 + 1/4 inches wide and extending to within 1/4 inch of the width of the table, securely fastened to the base. The step shall be covered with rubber matting, not less than 1/8 inch thick and shall have a binding strip of corrosion-resisting steel, .078 inch thick (No. 14, USS gage), around the edge of the plywood and flush with the rubber matting, attached by corrosion-resisting steel screws. The step shall exhibit no distortion when tested as specified in 4.5.6.

3.4.4 Dimensions. The examining table shall have the following overall dimensions, + 1 inch:

	Inches
Height to top of table at foot end	31
Height overall at head end	33-1/2
Width of top	23-1/2
Length of top	50-1/4
Length of top with sliding leg rest extended	67-1/2
Length of head end section	31-1/2
Length of foot end section	17 to 20

3.5 Finish.

3.5.1 Cleaning and surface preparation. All metal surfaces shall be thoroughly and completely washed. All welds on exposed surfaces shall show no objectionable pits or extrusions. When surface of metal is defaced, it shall be ground smooth and, when necessary, filled to prevent unsightly blemishes on the finish surface.

3.5.2 Primer. After cleaning, all metal surfaces to be enameled shall be given one coat of metal primer. The primer shall be baked in accordance with the primer manufacturer's directions. Primer shall then be completely sanded before applying baking-type enamel.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

3.5.3 Enamel. All exposed metal surfaces, except corrosion-resisting steel and chrome-plated metal, shall be covered with two coats of modified gloss alkyd baking-type enamel, having 60 ± 1.0% of solids weight, 40 ± 1.0% of volume solids. The finish surface shall be smooth, uniform, without runs, wrinkles, orangepeel, or grit. The total dry film thickness shall be not less than 1.1 ± 0.1 mil.

3.5.4 Color. Color shall be light green with black base.

3.5.5 Corrosion-resisting steel. Corrosion-resisting steel shall have a standard commercial No. 4 finish.

3.6 Dielectric withstand. The unit shall be capable of withstanding without breakdown, for one minute, a potential of 1240 volts, 60 Hz applied between live and dead metal parts.

3.7 Identification marking. Each unit shall be marked permanently and legibly with the following:

Contract or purchase order number or traceable serial number.
Name or registered trademark of the manufacturer.
Manufacturer's model number.

3.8 Service data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, maintenance, cleaning and lists of component parts.

3.9 Workmanship. Workmanship shall be first class throughout. The table shall be free from defects which detract from its appearance or impair its serviceability. All burrs and sharp edges shall be removed from the table.

3.9.1 Welding. Welding shall be durable, sound in every detail and in accordance with the latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive splatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:21Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the table when a first article sample is required (see 3.1 and 6.2). This inspection shall include examination of 4.4 and tests of 4.5.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.4 and tests of 4.5.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

4.2 Inspection lot.

4.2.1 Raw materials. An inspection lot for raw material inspection shall be all material produced under the same conditions and controlled to the degree that uniformity of product within the designated lot can be assured. Lot identification of the raw material by the manufacturer is one method of control, as cited above, which is considered acceptable.

4.2.2 End product. An inspection lot for inspection of end product shall consist of all tables of the same type produced under essentially the same conditions and offered for inspection at one time.

4.3 Sampling.

4.3.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table III. The unit of product for sampling purposes shall be one table.

TABLE III. Sampling for examination.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	1.0
Total defects (Major and Minor combined)	II	4.0
For dimensional examination	S-1	2.5

4.3.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table IV, for an acceptance level of zero.

TABLE IV. Sampling for tests.

Component (unit of product)	Characteristic	Requirement	Test procedure	Inspection level
Corrosion-resisting steel	Chemical composition	3.3.1	4.5.1	1/
Upholstery	Physical properties	3.3.5	4.5.2	2/
Foam padding	Physical properties	3.3.6	4.5.3	2/
Head end of upholstered top	Load strength	3.4.1.1	4.5.4	S-2
Stirrups	Load strength	3.4.2.4	4.5.5	S-2
Mounting step	Load strength	3.4.3	4.5.6	S-2
Table	Dielectric withstand	3.6	4.5.7	100%

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

1/ A sufficient quantity of each lot of corrosion-resisting steel used in the manufacture of the table shall be selected for chemical analysis as specified in 4.5.1.
2/ A sufficient quantity of each lot of upholstery and foam padding shall be tested as specified in 4.5.2 and 4.5.3 respectively.

4.4 Examination. The table shall be examined to determine compliance with all requirements contained in this specification.

4.4.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table V. Examination shall not be restricted to the classified possible defects listed below.

TABLE V. Classification of defects.

Categories	Defects
Major	
101	Any component missing or not as specified.
102	Table and components not properly aligned.
103	Any weld incomplete, broken, or cracked.
104	Burr or sharpness on exposed surface.
105	Upholstery cut, torn, or improperly fastened.
106	Any surface not enameled as specified - paint cracked, peeled, or blistered.
107	Any adjustment does not function smoothly within specified limits.
108	Head end section does not lock securely at any point in specified range of adjustment.
109	Table does not rest evenly on a level floor surface.
110	Spaces around door and drawer openings not uniform.
111	Space around door or drawer openings exceeds specified requirement.
Minor	
201	Unit not clean; shows dirt, oil, or grease.
202	Identification marking not present, permanent, complete, and legible.
203	Weld has pitting or spatter.
204	Exposed weld not ground smooth to blend with adjacent surfaces.
205	Upholstery uneven or discolored.

4.4.2 Dimensional examination. The table shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4.3 Packaging inspection. The inspection of the interim wrapping and cushioning shall be in accordance with the group A quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the container specification and the marking requirements of MIL-STD-129.

4.5 Tests. Tests shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:21Z
Check the source to verify that this is the current version before use.

4.5.1 Chemical composition. Four ounces from each lot of material shall be tested in accordance with Fed. Test Method Std. 151.

4.5.2 Upholstery. Testing of upholstery shall be in accordance with the ASTM Standard Methods of Test and the Federal Specifications listed in table VI.

TABLE VI. Testing of upholstery.

Characteristic	Test Method
Weight	ASTM D-751
Thickness	ASTM D-751
Tensile strength	ASTM D-751
Tear strength	ASTM D-751
Cold crack	FED-TEST-METHOD-STD-191, Method 5874
Wear	FED-TEST-METHOD-STD-191, Method 5306
Burn time	CCC-A-680

4.5.3 Foam padding. Testing of foam padding shall be in accordance with the ASTM Standard Methods of Test and the Federal Specifications listed in table VII.

TABLE VII. Testing of foam padding.

Characteristic	Test method
Density	ASTM D-2406
Indentation load deflection	ASTM D-2406
Steam autoclave	ASTM D-2406
Flame retardance	DDD-C-95

4.5.4 Load test (headrest section). A 50 pound weight shall be placed on the headrest section of the head-end and secured in position. The loaded head-end section shall be raised to the full 85 degree position and locked in place. The section shall then be lowered, allowing the locking mechanism to engage at 45 degrees and at 15 degrees. This operation shall be repeated 15 times. At the end of this procedure, the table shall be examined for distortion.

4.5.5 Load test (stirrup). Each stirrup shall be extended to its full length and full height and locked in position. A 50 pound weight shall be placed on each stirrup for 30 minutes. The stirrups and supporting system shall then be examined for distortion.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

4.5.6 Load test (mounting step). A 250 pound load shall be applied to the mounting step, distributed over an area of 1 square foot or less, for 30 minutes. The step shall then be examined for distortion.

4.5.7 Dielectric withstand. A slowly rising potential, from 0 to 1240 volts, 60 Hz, shall be applied between live and dead metal parts. This potential shall be maintained at maximum for one minute.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit preparation. Each table shall be disassembled as far as is practicable. Disassembled parts shall be properly protected and packed within the unit in such a manner as to prevent movement. Doors and drawers shall be closed and secured in position. All exterior surfaces shall be protected by wrapping with kraft paper and cushioning with flexible corrugated fiberboard or similar material. Wrapping and cushioning material shall be secured by tying with tape. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit.

5.1.2 Level C. Each table shall be prepared for shipment in a manner which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A or C as specified (see 6.2).

5.2.1 Level A. Each table shall be overpacked in an exterior container constructed in accordance with PPP-B-640, class 2, style E. The table shall be secured to the base of the container in such a manner that the weight of the table shall not be carried directly by its legs. In addition, the table shall be further secured within the container by means of interior fittings and fillers made from corrugated fiberboard to insure against shifting of or damage to the contents. The exterior container shall be designed with three skids of not less than 1-1/2 inches in thickness applied crosswise of base, so positioned as to facilitate handling with a forklift truck and to maintain the table in an upright position. Closure and sealing against entry of water shall be in accordance with the appendix of box specification.

5.2.2 Level C. Tables shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking.

5.3.1 Interior packages. Interior packages shall be marked to identify their contents.

5.3.2 Exterior container. Each exterior container shall be marked as specified in MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:21Z
Check the source to verify that this is the currenversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS: This form is provided to solicit beneficial comments which may improve this document and enhance its use. DoD contractors, government activities, manufacturers, vendors, or other prospective users of the document are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity. A response will be provided to the submitter, when name and address is provided, within 30 days indicating that the 1426 was received and when any appropriate action on it will be completed.

NOTE: This form shall not be used to submit requests for waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

DOCUMENT IDENTIFIER (Number) AND TITLE

MIL-T-36295A TABLE, EXAMINING AND TREATMENT, CABINET TYPE, STEEL, ENAMELED

NAME OF ORGANIZATION AND ADDRESS OF SUBMITTER

☐ VENDOR ☐ USER ☐ MANUFACTURER

1. ☐ HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE? ☐ IS ANY PART OF IT TOO RIGID, RESTRICTIVE, LOOSE OR AMBIGUOUS? PLEASE EXPLAIN BELOW.

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDED WORDING CHANGE

C. REASON FOR RECOMMENDED CHANGE(S)

2. REMARKS

SUBMITTED BY *(Printed or typed name and address — Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 OCT 76 1426 EDITION OF 1 JAN 72 WILL BE USED UNTIL EXHAUSTED.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:21Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:21Z
Check the source to verify that this is the current version before use.