FED. SUP CLASS
6640

REVIEW ACTIVITIES: ARMY - CE
NAVY - AS
AIR FORCE - 82

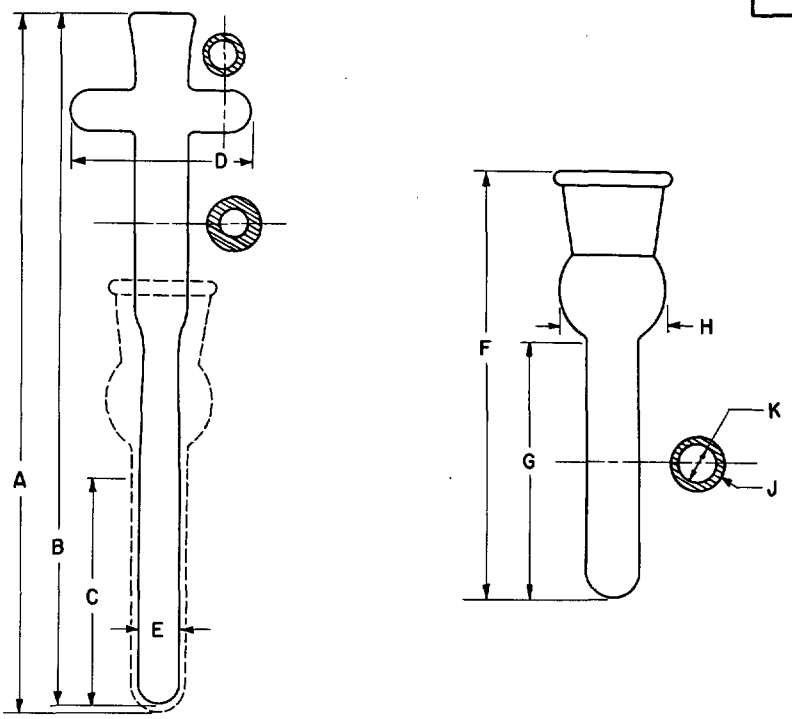

NOMINAL DIMENSIONAL DATA millimeters										
PART NUMBER	A OVER-ALL LG OF PESTLE AND TUBE	B LG OF PESTLE	C & G LG OF SECTION OF PESTLE AND TUBE TO BE GROUND	D WIDTH OF HANDLE	E DIA OF GROUND PORTION OF PESTLE (GROUND TO FIT WITH TUBE)	F OVER-ALL LG OF TUBE	H OD OF CATCH BASIN	J OD OF GROUND SECTION OF TUBE	K ID OF GROUND SECTION OF TUBE	SIZE
(A) MS36109-1	200	196	80	51	11	120	30	16	11	Small
MS36109-2	340	335	130	90	20	210	55	25	20	Large

MATERIAL: Pestle and tube shall be of borosilicate glass in accordance with Federal Specification DD-G-541, Type I, Class A.

DESIGN: The pestle and the inside surface of the tube shall be coarse ground. The difference between the inside diameter of the tube and the outside diameter of the pestle shall be 0.12 to 0.17 mm to insure proper maceration of tissues.

NOTES:
1. For design feature purposes, this standard takes precedence over procurement documents referenced herein.
2. Referenced documents shall be of the issue in effect on date of invitations for bid.

APPROVED 22 SEPT 1960 REVISED (A) 31 MAY 1967

This military standard is approved by the Department of Defense and is mandatory on all activities. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A. MU	TITLE	MILITARY STANDARD
Other Cust MS 82	TISSUE GRINDER, TEN BROECK glass	MS36109
PROCUREMENT SPECIFICATION DD-T-363	SUPERSEDES:	SHEET 1 OF 1

DD FORM 1 SEP 67 672-1 (Coordinated)

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:34Z
Check the source to verify that this is the current version before use.