MILITARY SPECIFICATION

HOLDER, SUTURE NEEDLE, HEGAR-MAYO

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers two sizes of Hegar-Mayo suture needle holders.

1.2 Classification.

1.2.1 Sizes. Holders shall be of the following sizes, as specified:

Size	Length (in inches)
1	6
2	7

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

GG-I-526	- Instruments, Dental and Surgical; General specifications.
PPP-B-585	- Boxes, Wood, Wirebound.
PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	- Boxes, Shipping, Fiberboard.

MILITARY

MIL-P-116	- Preservation, Methods of
MIL-L-10547	- Liners, Case and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The holders shall be in accordance with the applicable requirements of GG-I-526 and as specified herein.

3.2 Material.

3.2.1 Holder proper. The holder proper shall be fabricated from Class 4, type 410 or Class 4, type 420.

3.2.2 Jaw inserts (or material plated on inside of jaws). The jaw inserts, or plating on inside of jaws, shall be tungsten carbide (Class 9).

3.3 Hardness. After proper stress relieving, Rockwell hardness shall be C40 to C45 for holder proper. Tungsten carbide on jaws (insert or plating) shall have a Rockwell hardness of A80, minimum.

3.4 Style, design and dimensions. Shall be a suture needle holder of the Hegar-Mayo design. Serrated inserts shall be brazed to jaws with a uniform flow of silver solder and be free of crevices at all interfaces. As an alternate, the serrated inside surfaces of the jaw shall be flame plated (reference thickness: .003 inch to .005 inch). Size 1 shall be in accordance with Figure 1. Size 2 shall be in accordance with Figure 2.

3.5 Locks. Shall be box lock type. Shanks shall be tested for stiffness in accordance with GG-I-526.

3.6 Finish. Holders, except jaw inserts, or jaw plating, shall have a mirror finish.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

3.7 Identification marking. In addition to GG-I-526 requirements, forceps of foreign manufacture shall also be marked "stainless".

3.8 Workmanship. Workmanship shall be first class throughout. Holders shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Shall be in accordance with GG-I-526.

4.1.2 Records. Records of examination and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the corrosion resisting steel and tungsten carbide may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the government. The certificates shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock No., the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, the individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in table I. The unit of product for examination purposes shall be one holder.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

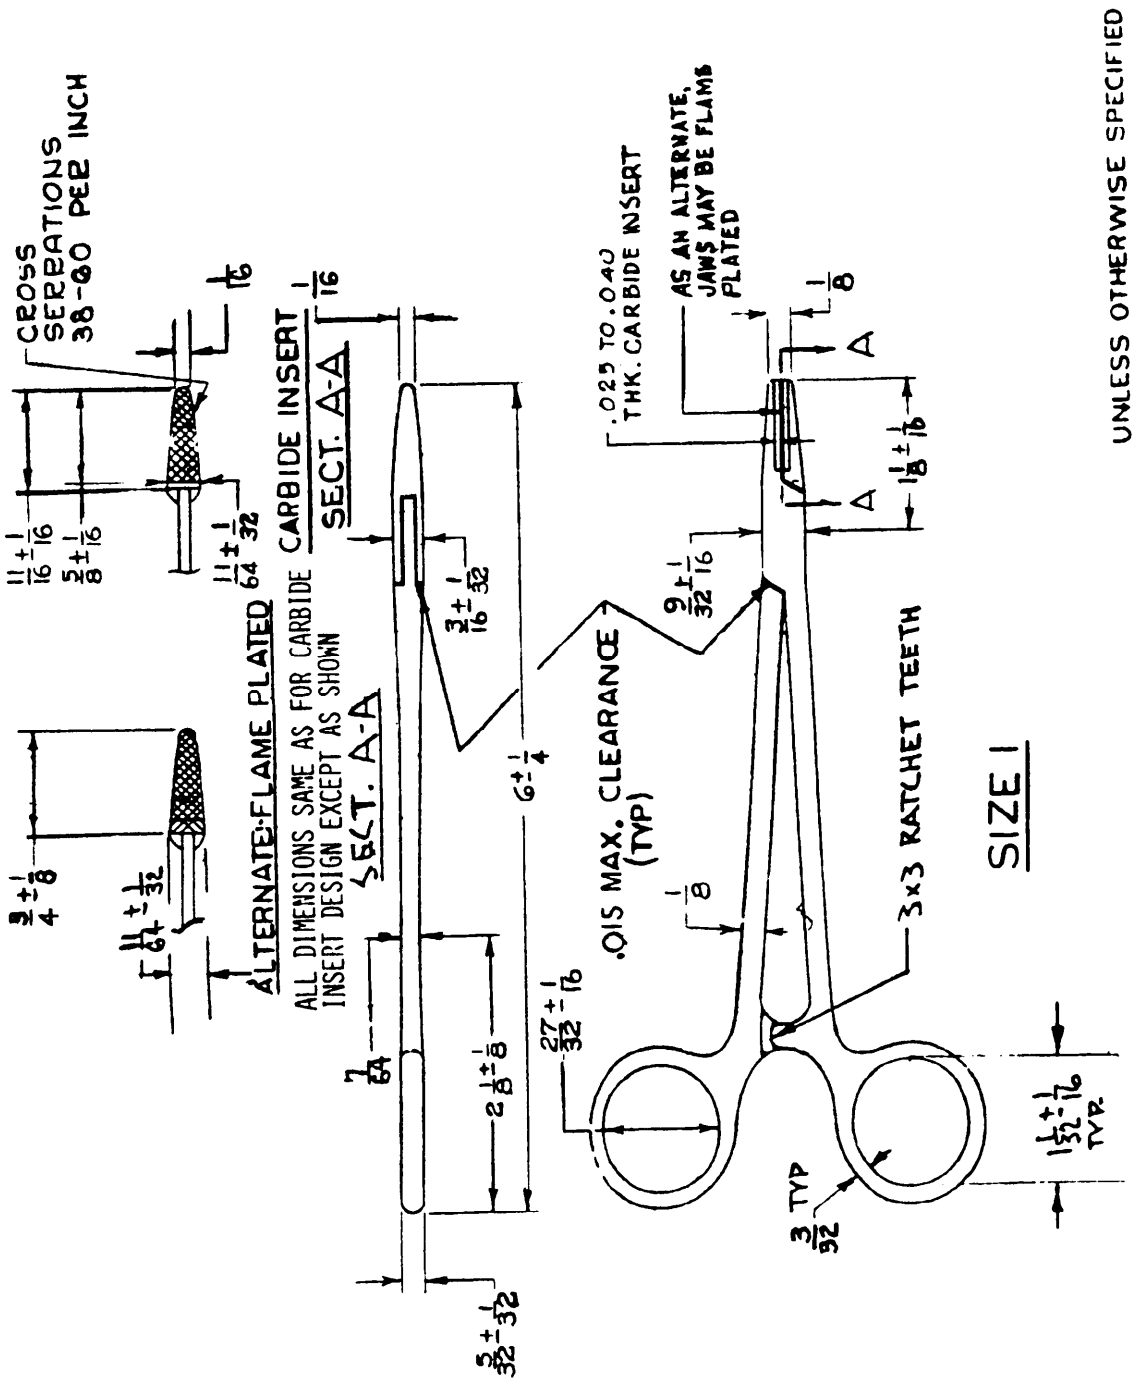


FIGURE 1. Holder, suture needle, Hegar-Mayo, 6 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

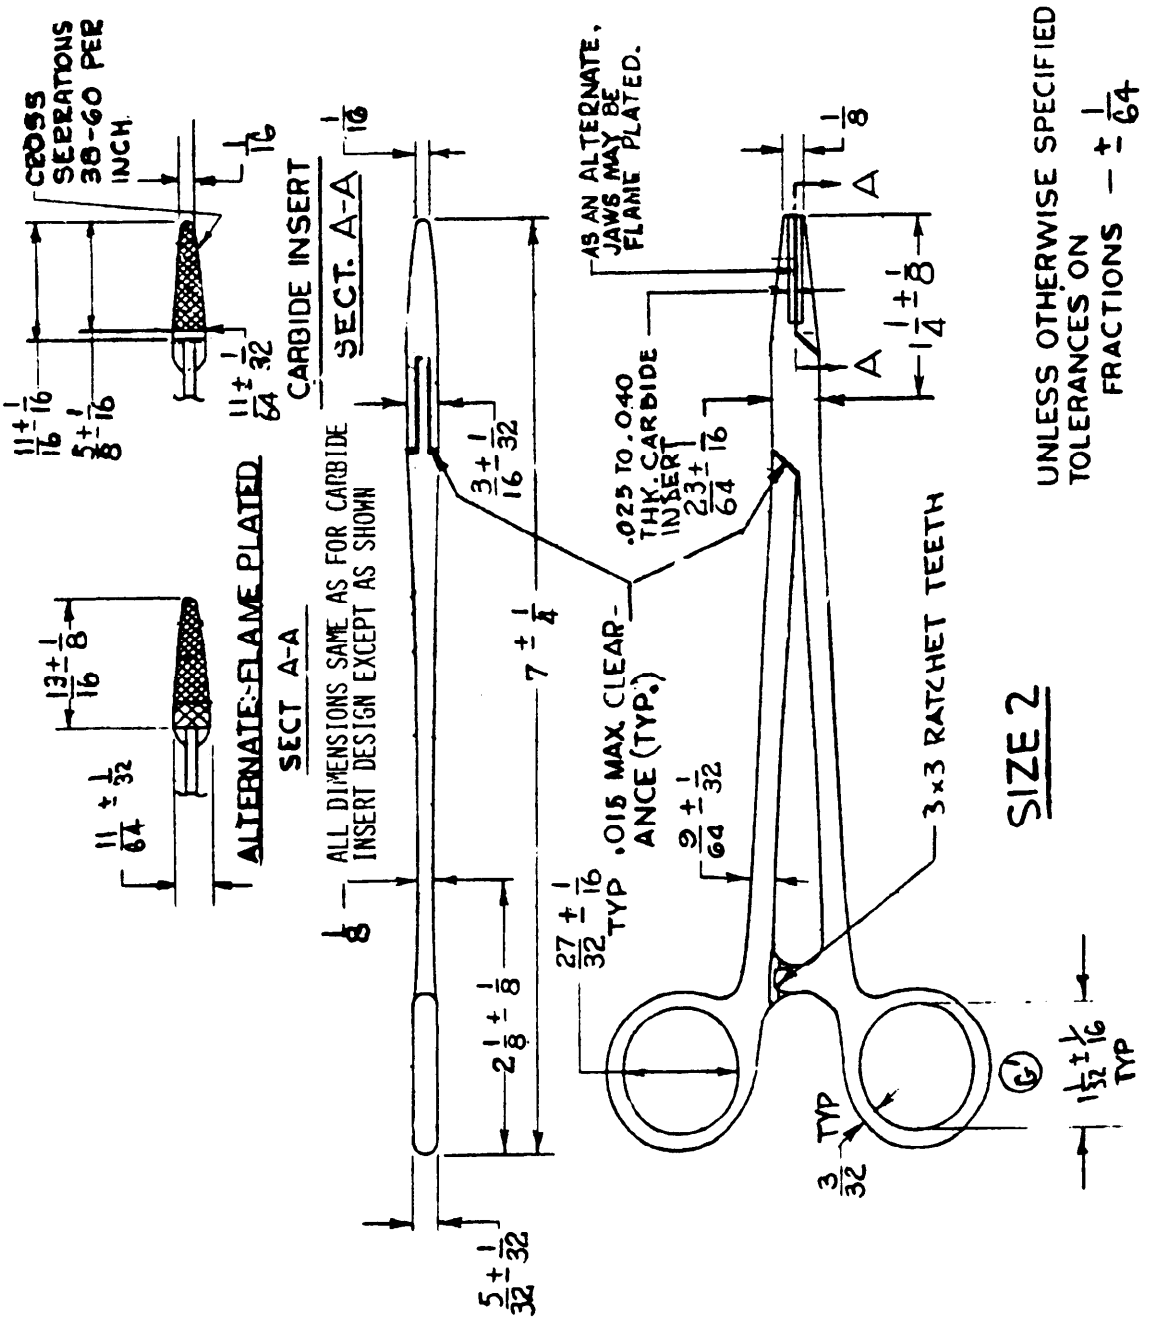


FIGURE 2. Holder, suture needle, Hegar-Mayo, 7 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

TABLE I. Sampling criteria for examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II. Unit of product for test purposes shall be one holder.

TABLE II. Sampling criteria for tests

Component	Characteristic	Requirement	Test procedure	Insp. level	AQL
Holder	Hardness	3.3 and GG-I-526	GG-I-526	S-2	1.5
	Dimensions	3.4	--------	S-2	4.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0
	Copper sulfate	GG-I-526	GG-I-526 and 4.4.1	S-2	1.0
	Box-lock test	3.5	GG-I-526	S-2	2.5

4.2.3 Raw materials. Four ounces of each lot of each metal used in the manufacture of the holders shall be selected for chemical analysis.

4.3 Examination.

4.3.1 Examination of holder. The holders shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in tables I and III. Examination, however,

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

shall not be restricted to defects listed in table III. Any holder in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

TABLE III. Classification of defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Holders not free from cracks, pits, dents, nicks, sharp edges and burrs.
103	Serrations not as specified.
104	Ratchet teeth not uniform.
105	Ratchet teeth do not function properly.
106	Holders not free from excessive play in box-lock area.
Minor	
201	Finish (except jaw insert or jaw plating) not mirror and not uniform.
202	Identification marking not present, correct, complete or legible.

4.3.2 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0.

TABLE IV. Examination for preparation for delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and Packing Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Copper sulfate test. In lieu of total immersion of instrument, as specified in GG-I-526, the holder shall be immersed in copper sulfate only from the proximal end to beginning of box lock. The jaws (stainless steel portions only) shall have drops of copper sulfate placed on four different spots.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning, drying and preservative. Each holder shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116. Preservative shall not be applied.

5.1.1.2 Unit package. Each holder shall be wrapped in neutral tissue or other suitable anticorrosive material. Each holder shall be further packaged in accordance with MIL-P-116, method 1C-1.

5.1.1.3 Intermediate package. Twelve (12) holders shall be packaged in a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening.

5.1.2 Level C. Holders shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Two hundred and eighty eight (288) holders shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2 or PPP-B-636, class water resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard boxes shall be waterproof as specified in the appendix of PPP-B-636.

5.2.2 Level B. Two hundred and eighty-eight (288) holders shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, type CF class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. Holders shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior and exterior containers. Interior and exterior containers shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. These suture needle holders of Hegar-Mayo design are to be used for grasping suture needles during surgery.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Applicable National Stock Number (NSN)
(c) Selection of applicable levels of packaging and packing required (see 5.1 and 5.2).

6.3 National Stock Number (NSN) coverage. This specification covers the following items listed in the Federal Supply Catalog:

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

National Stock Number	Item Identification
6515-00-299-8736	HOLDER, SUTURE NEEDLE, Hegar-Mayo 6 inch
6515-00-299-8737	HOLDER, SUTURE NEEDLE, Hegar-Mayo, 7 inch

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1950

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-H-37236 HOLDER, SUTURE NEEDLE, HEGAR-MAYO

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:15Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:15Z
Check the source to verify that this is the current version before use.