MILITARY SPECIFICATION

TAG, MEDICAL WARNING

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type and size of medical warning tag used by the Army, capable of being readily embossed with medical warning information identifying the wearer's sensitivites, allergic reactions, or selected health problems in the absence of medical records.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

QQ-A-250/8	Aluminum Alloy, 5052, Plate and Sheet
PPP-B-566	Boxes, Folding, Paperboard
PPP-B-585	Boxes, Wood, Wirebound
PPP-B-601	Boxes, Wood, Cleated-Plywood
PPP-B-621	Boxes, Wood, Nailed and Lock Corner
PPP-B-636	Boxes, Shipping, Fiberboard
PPP-B-676	Boxes, Setup

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap Water-Vaporproof or Waterproof, Flexible

STANDARDS

Federal

Fed. Test Method Std. 151	Metals, Test Methods

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Materials. Material shall conform to the requirements specified herein.

3.1.1 Aluminum. The aluminum for the tag shall be alloy 5052-H34 as specified in QQ-A-250/8, having a mill finish.

3.2 Finish. The aluminum shall be anodized on both sides to match the red of a standard sample that will be furnished by the Government. The anodic coating shall be a minimum of 0.0004 inch thick and shall be sealed with a nickel acetate sealer. The dye used shall be an aluminum fast red organic dye with a light fast and weather fast rating of excellent to perfect.


3.3 Construction. The medical warning tags shall be fabricated from pre-anodized aluminum specified in 3.1.1 and shall conform to the details and dimensions of Figure 1. The edges of the finished tag shall be clean, smooth and free from burs and rough or sharp edges. Slight streaking caused by manufacturing mill marks shall not be cause for rejection. Figure 1 is dimensioned in inches.

3.4 Workmanship. Workmanship shall be first class throughout. The tags shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

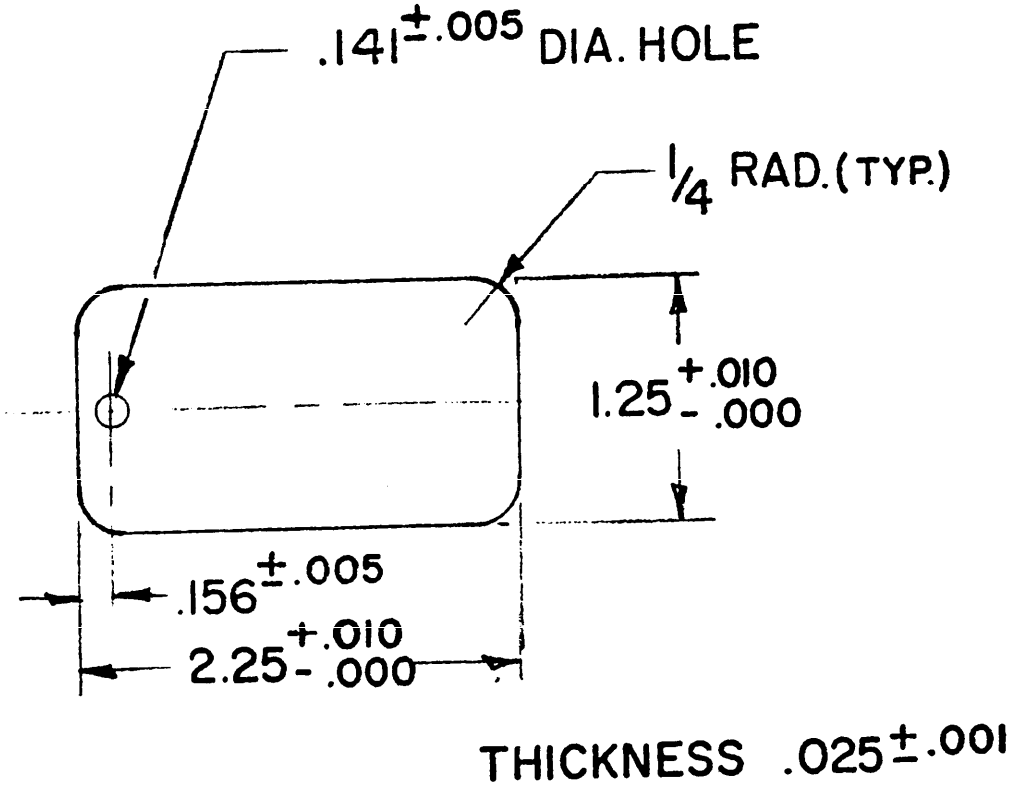

TAG, MEDICAL WARNING

FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the aluminum may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the supplier, lot number, and chemical analysis of the lots of aluminum supplied.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and Table I. The unit of product for inspection purposes shall be the individual tag (except where otherwise specified). Sample tags shall be selected at random in such a manner that not more than two individual tags shall be selected from one package.

Table I. Sampling for Examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defect	I	1.0
Total (major and minor combined)	I	4.0
For dimensional examination	S-2	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with Inspection level S-1 of MIL-STD-105. The acceptance level shall be zero.

4.3 Examination. The tags shall be examined to determine compliance with all the requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in Table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

Table II. Classification of Defects

Categories and defects*	
Major	
101	Finish not anodized mill finish on both sides or not correct color.
102	Exposed edges not free of burs or sharpness.
103	Finish not free of oil, grease, dirt or other foreign matter.
104	Tag not free of cracks, dents or excessive distortion.
Minor	
201	Finish not free of chipped areas, scratches, or roughness.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The tags shall be examined for compliance with dimensional requirements. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of FED-STD-151.

4.5 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

Table III Examination for Preparation for Delivery

Examination	Defect
Containers Quantity	Not as specified. Quantity in interior packages and shipping containers not as specified.
Packaging and Packing Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY.

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One package containing one hundred (100) tags as specified, constitutes one unit of issue.

5.1.1.1 Level A.

5.1.1.1.1 Unit package. Each unit of issue shall be packaged in a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676. Closure shall be adequate to prevent accidental opening.

5.1.1.1.2 Intermediate package. Twelve (12) units of issue shall be packaged in a box of appropriate size constructed in accordance with PPP-B-676 or PPP-B-636, class domestic. Closure shall be adequate to prevent accidental opening.

5.1.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Seventy-two (72) units of issue shall be packed in a box designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with PPP-B-636.

5.2.2 Level B. Seventy-two (72) units of issue shall be packed in a box designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

5.3 Markings.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Intended for use as a Medical Alert Tag.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-142-8775	TAG, MEDICAL WARNING, Red, Aluminum, 100s

6.4 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6530-1336
cs

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-T-37202 TAG, MEDICAL WARNING

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:11Z
Check the source to verify that this is the current version before use.