A-A-51239
17 December 1985

COMMERCIAL ITEM DESCRIPTION

HOOK, SKIN,
Kleinert-Kutz, Sharp Point, Medium

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a skin hook for use in general and plastic surgical procedures.

Salient characteristics

Shall be a sharp skin hook, Kleinert-Kutz style, 7 inch (18 cm) overall length, with medium 3/4 circle tip for use in general and plastic surgical procedures.

The skin hook shall be in accordance with Federal Specification GG-I-526 and as specified herein.

Material. Shall be fabricated from a corrosion-resistant austenitic stainless steel, class 3, in accordance with ASTM F 899.

Hardness. After proper annealing the Rockwell hardness shall be B75 to B100.

Passivation. The instrument shall be properly passivated.

When tested as specified in the boil test, the surface of the skin hook shall show no signs of corrosion (without magnification).

Style and design. The skin hook shall have a knurled handle to prevent slippage during use. The tip of the skin hook shall be 4 cm in diameter. The style and dimensions of the skin hook shall be in accordance with figure 1.

Finish. The finish of the instrument shall be mirror or satin.

Workmanship. The skin hook shall be free from defects which detract from its appearance or impair its serviceability.

PRODUCT QUALITY LEVEL

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One skin hook, as specified, constitutes one unit.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release, distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one skin hook.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6515-01-164-3144

Hook, Skin, Single Sharp Point, Medium #2, 7 inch, Kleinert-Kutz.

MILITARY INTERESTS:

Custodians.

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA - DM

CIVIL AGENCY COORDINATING ACTIVITY:
VA-OSS

52043

Project No. 6515-3331

Location S1-9-19

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

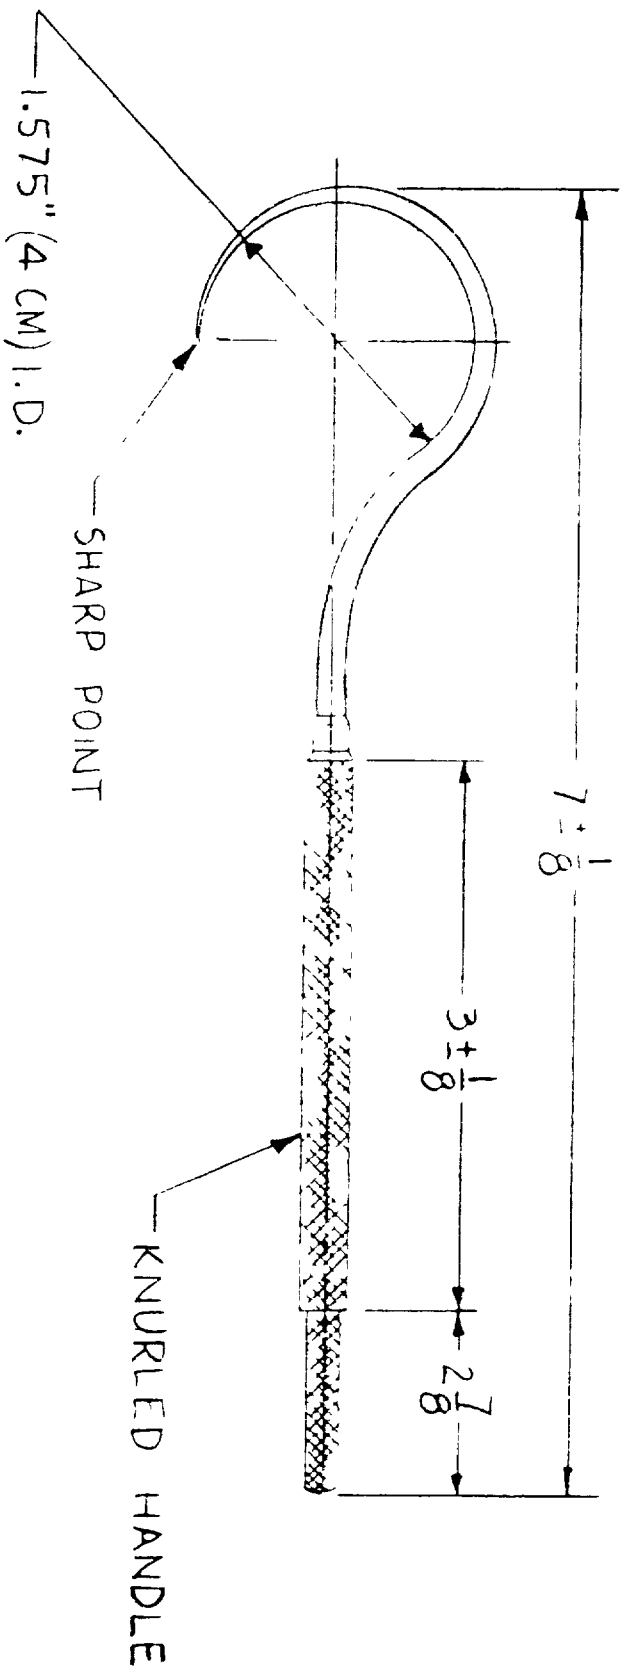


FIGURE 1 HOOK, SKIN, MEDIUM NO. 2, KLEINERT-KUTZ DESIGN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.