MILITARY SPECIFICATION

# DILATOR SET, COMMON BILE DUCT, BAKES, SET OF 9

This specification is approved for use by Defense Personnel Support Center, Defense Supply Agency, and is available for use by all Departments and Agencies of the Department of Defense.

## 1. SCOPE

1.1 Scope. This specification covers a set of nine common bile duct dilators of the Bakes design suitable for use in exploring the common duct and gall bladder.

## 2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

| | |
|---|---|
| PPP-B-636 | - Boxes, Shipping, Fiberboard. |

MILITARY

| | |
|---|---|
| MIL-P-116 | - Preservation, Methods of. |

STANDARDS

MILITARY

| | |
|---|---|
| MIL-STD-105 | - Sampling Procedures and Tables for Inspection by Attributes. |
| MIL-STD-129 | - Marking for Shipment and Storage. |

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

## 3. REQUIREMENTS

3.1 General requirements. The metal dilators shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The dilators shall be fabricated from Class 3, Type 302, 303, or 304 material.

3.3 Hardness. Shaft portion of instrument shall have a Rockwell hardness of B25 minumum.

3.4 Style, design and dimensions. The dilator set shall consist of nine common bile duct dilators suitable for medical procedures in exploring the common duct and gall bladder. The dimensions of the dilators shall be in accordance with Figure 1. The dilators shall be contained in a suitable folding canvas case with a tie string.

3.5 Finish. Eliptical tip of dilators shall have mirror finish. Remainder of instrument shall be mirror or satin.


3.6 Identification marking. In addition to GG-I-526 requirements, dilators of foreign manufacture shall also be marked "stainless". The handle of each dilator shall be permanently and conspiciously marked, as by embossing, with the applicable size (ie. 3mm) in millimeters.

## 4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.



Source: https://assist.dla.mil -- Downloaded: 20260-21T10:33Z
Check the source to verify that this is the current version before use.

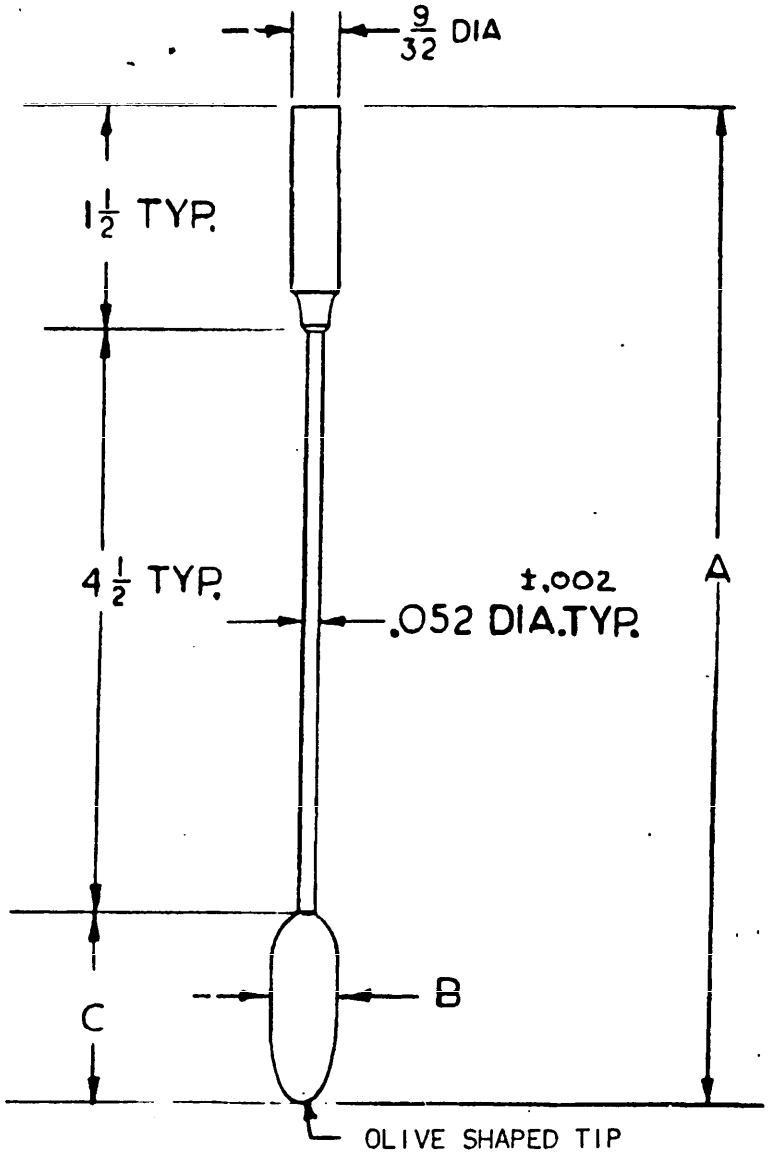


| SIZE | "A" | "B" DIA | "C" |
|---|---|---|---|
| 3 MM | 6-11/16 | 1/8 | 11/16 |
| 4 MM | 6-13/16 | 5/32 | 11/16 |
| 5 MM | 6-7/8 | 3/16 | 13/16 |
| 6 MM | 7 | 1/4 | 15/16 |
| 7 MM | 7 | 9/32 | 31/32 |
| 8 MM | 7-1/8 | 5/16 | 31/32 |
| 9 MM | 7-5/16 | 3/8 | 1-1/4 |
| 10 MM | 7/3 8 | 13/32 | 1-3/8 |
| 11 MM | 7-7/16 | 7/16 | 1-7/16 |
| TOLERANCE | ± 1/32 | ± 1/64 | ± 1/16 |

DIMENSIONS IN INCHES

**FIGURE 1. Dilator set, common bile duct, Bakes, set of 9**



Source: https://assist.dla.mil -- Downloaded: 202610-21T10:33Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in table I. The unit of product for examination purposes shall be one dilator set.

TABLE I. Sampling for examination

| Type of defect | Inspection level | AQL (percent defective) |
|---|---|---|
| Major | II | 1.0 |
| Minor | II | 2.5 |

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in table II. Where feasible, the sample shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one dilator set.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

TABLE II. Sampling for tests

| Component | Characteristic | Requirement | Test procedure | Insp. level | AQL |
|---|---|---|---|---|---|
| 1-Dilator | Composition analysis | 3.2 and GG-I-526 | GG-I-526 | 1/ | 2/ |
| 1-Dilator | Hardness | 3.3 and GG-I-526 | GG-I-526 | S-2 | 2/ |
| 1-Dilator set | Dimensions | 3.4 | -------- | S-2 | 2/ |
| 1-Dilator | Boil test | GG-I-526 | GG-I-526 | S-2 | 2/ |

1/ Sufficient amount from each lot of each metal used in the construction of the forceps shall be selected for chemical analysis.

2/ Acceptance number shall be zero for all sample sizes.

4.3 Examination. The dilators shall be examined to determine compliance with all the requirements contained in the specification. Examination shall be conducted as specified in tables I and III. Examination, however shall not be restricted to defects listed in table III. Any dilators in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

TABLE III. Classification of defects

| Categories | Defect |
|---|---|
| Critical | None defined. |
| Major | |
| 101 | Style and design not as specified. |
| 102 | Dilators not free from cracks, sharp edges, rough areas, burrs, grind marks, or overlaps. |
| 103 | Dilator tips not smoothly rounded. |
| Minor | |
| 201 | Finish not as specified. |
| 202 | Identification marking not present, correct, complete or legible. |
| 203 | Canvas case does not properly contain dilators. |



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

4.3.1 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One dilator set along with a canvas case, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Cleaning. Dilators shall be cleaned in accordance with MIL-P-116, method C-1.

5.1.2.2 Drying. Dilators shall be dried in accordance with MIL-P-116.

5.1.2.3 Preservative application. Preservatives shall not be used.

5.1.2.4 Unit packaging. Each set of dilators shall be positioned within the canvas case and the case secured with the string ties. The set shall be further packaged in accordance with MIL-P-116, method IC-2.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Forty-eight unit packages shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class weather-resistant. Closure, strapping and waterproofing shall be as specified in the appendix of the box specification.



Source: https://assist.dla.mil --Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. Forty-eight unit packages shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.3.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.4 Marking.

5.4.1 Unit packages. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.4.2 Exterior container. Exterior containers shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The dilators are used for exploring the common duct and gall bladder.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) National Stock Number.

6.3 This specification is intended to cover the following item appearing the in the Federal Supply Catalog.

| National Stock No. | Item Identification |
|---|---|
| 6515-00-325-2800 | DILATOR SET, COMMON BILE DUCT, BAKES, Set of 9 |

It does not include all types or sizes as indicated by the title which are commercially available.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1987



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-D-37371(DSA-DM) DILATOR SET, COMMON BILE DUCT, BAKES,

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER SET OF 9

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

**DD FORM 1 JAN 72 1426**

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

GPO 1974 - 603 680 6126 2-1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:33Z
Check the source to verify that this is the current version before use.