COMMERCIAL ITEM DESCRIPTION

CUFF, BLOOD WARMER

The General Services Administration has authorized the use of this commerical item description.

This commerical item description covers a sterile, disposable, dry heat blood warmer cuff for use in heating blood or intravenous fluids by a cylindrical blood warmer.

Salient characteristics:

General. The cuff shall be a blood warming cuff used in enclosing blood or parenteral fluids for heating during intravenous transfusion procedures. The blood warming cuff shall be capable of withstanding multiple single-patient transfusions.

Material. The convoluted cuff shall be fabricated of 4 ml polyurethane. The shut-off clamp shall be polypropylene, the injection site natural rubber, the tubing polyvinyl chloride and other fittings of suitable plastic.

Construction. The blood warmer cuff shall consist of a female Luer fitting, a "Y" fitting, a blood warming convoluted bag, a drip chamber, a "Y" injection site, a roller shut-off clamp, a male Luer fitting and Luer end protectors interconnected by plastic tubing.

The blood warming cuff system shall be fabricated as shown in Figure 1 and shall be compatible with Blood Warming Set (See Note 2). The Luer fittings shall be in accordance with ANSI/HIMA Standard MD70.1.

The blood warming convoluted bag shall have dimensions of 10 inches by 6 inches and contain a convoluted passage running the entire length of the cuff as shown on Figure 1.

The drip chamber shall be fabricated of rigid plastic and shall be 3 inches long.

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

The roller clamp shall provide unobstructed flow when open and complete shut-off of blood or fluid when closed. Clamp shall be adjustable to provide drip flow rates up to 20 ml per minute. After use, no more than 35 ml of blood or fluid shall remain in the convoluted bag and bubble trap.

The rubber injection site diaphragm shall reseal without a falling drop within 10 seconds after puncture with a non-lubricated 18 gage needle, and when subjected to an internal pressure (hydrostatic pressure) of 5.8 psig for 30 seconds.

The blood warming cuff when enclosed in the blood warmer (see notes) shall not leak or parts separate when subjected to an internal (hydrostatic pressure) of 5.8 psig for 30 seconds.

The roller shall not part from its housing when subjected to a 3.48 Kg load in the shut-off direction.

Sterility, pyrogenicity, toxicity and biological tests. The internal surfaces of the system shall be non-pyrogenic, non-toxic and meet Class IV plastic requirements when tested in accordance with the USP. The sterility assurance level shall be 1×10^{-6} in accordance with AAMI guidelines.

The system shall comply with all applicable requirements of the Bureau of Medical Devices and Diagnostics.

All surfaces coming in contact with administered blood or intravenous fluids shall contain no more than 5 parts per million (ppm) of lead when tested in accordance with the USP.

Compatability. The materials of construction of each cuff shall not react with, or be acted upon by the liquids with which they will be in contact during normal use and operation. There shall be no materials incorporated in the set which will cause any deleterious effect when the cuff is used for the purpose intended.

Instructions. Instructions shall be provided for the installation of the cuff in the blood warmer and use of the cuff in the intravenous procedures.

Workmanship. The blood warmer cuff shall be free from defects which detract from its appearance or impair its serviceability. System shall be free from crimps, loose parts, weak sections and foreign material.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Unit. Package (PG). One package containing ten individually packaged sterile blood warming cuffs, as specified, constitutes one unit. The individual package shall be a sealed, peel open type container capable of maintaining sterility of contents unless package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Inspection level shall be S-3 with an AQL of zero. The unit of product for test purposes shall be one blood warmer cuff.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM DESCRIPTION
6515-01-153-5413	CUFF, BLOOD WARMER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

NOTE 2: Blood Warming cuff shall mount in and be compatible with Warmer, Blood and Fluid (NSN 6515-01-120-2636).

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4225

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

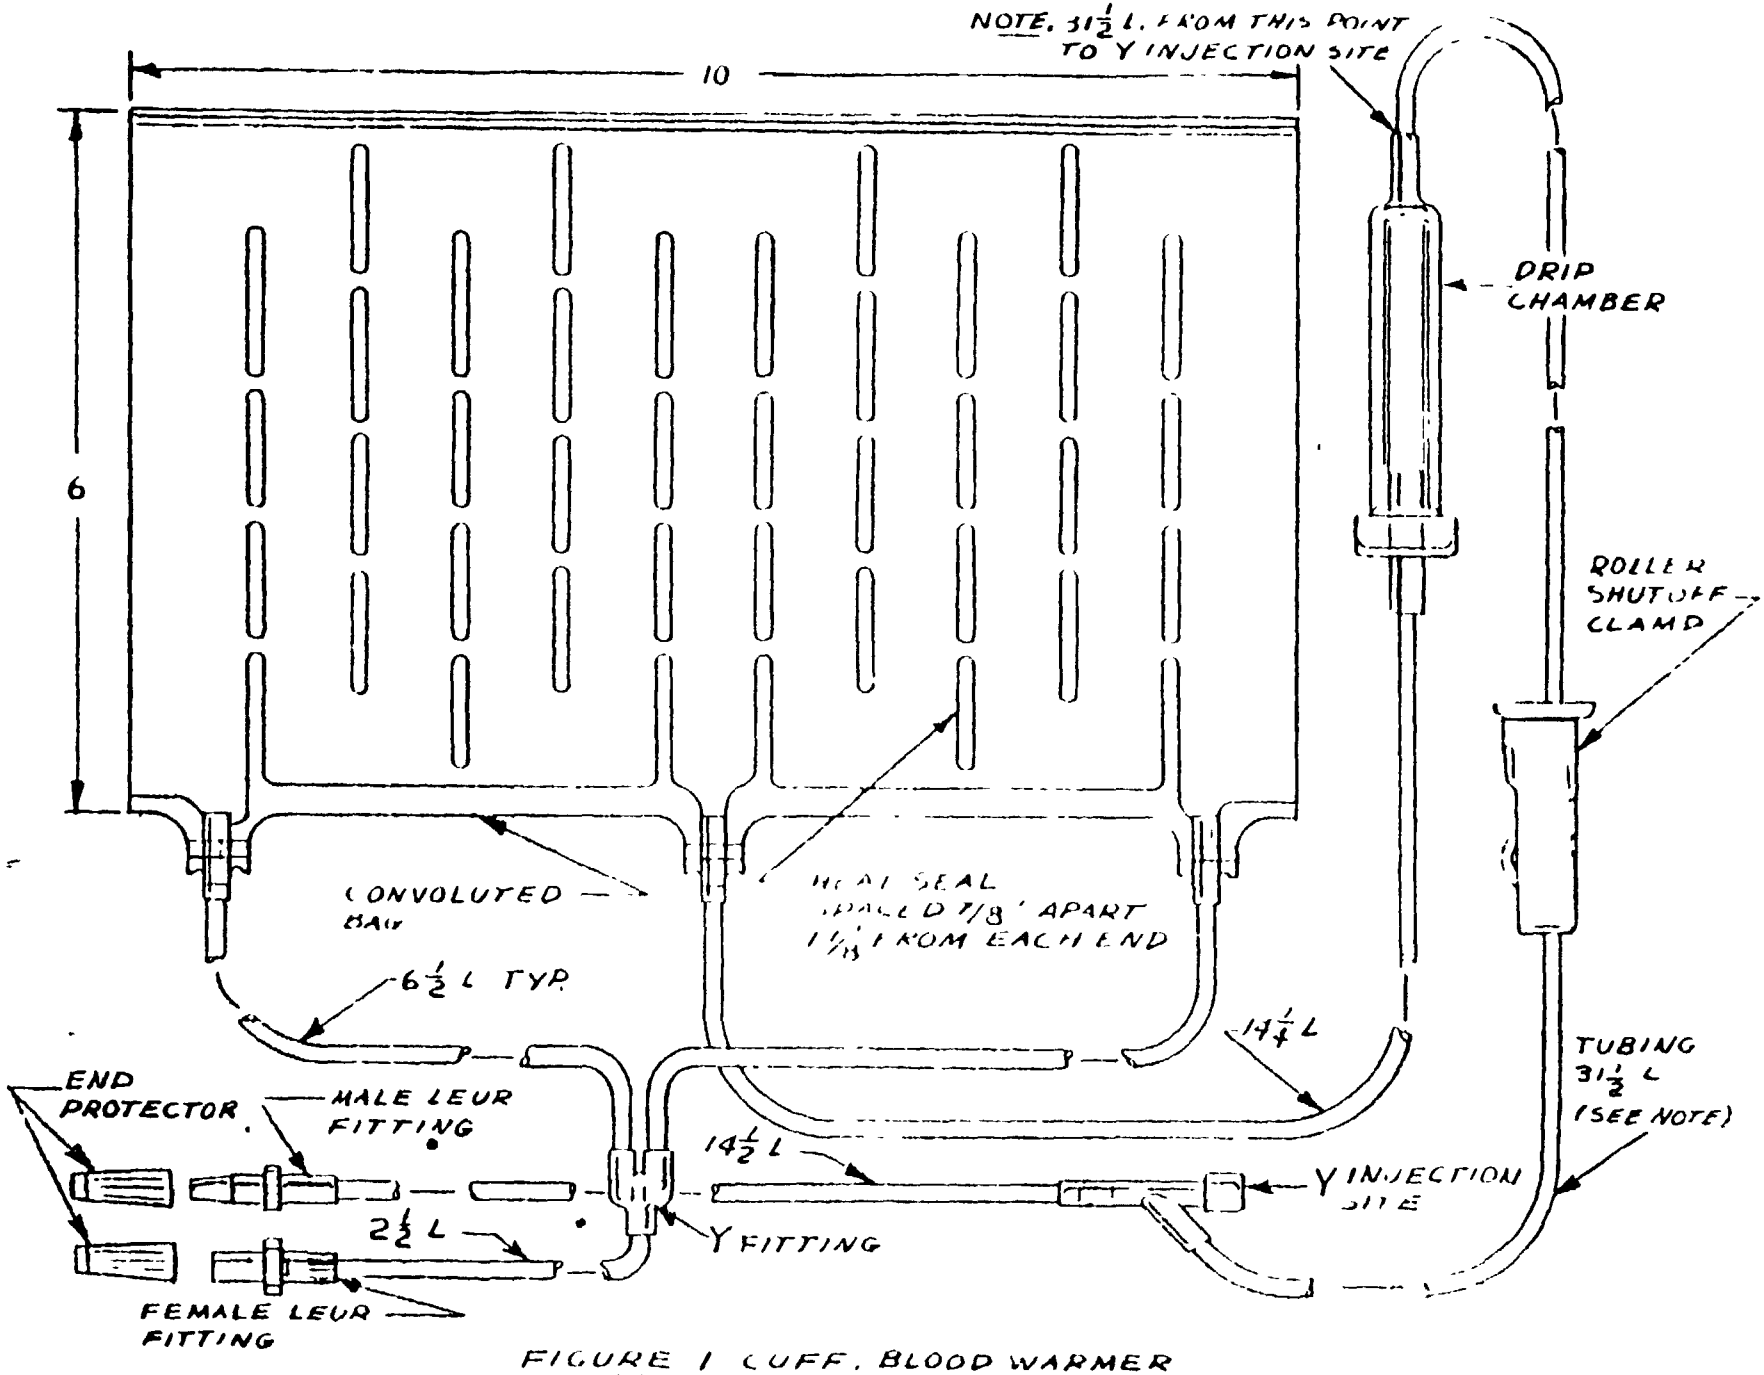

A-A-55971

FIGURE 1 CUFF, BLOOD WARMER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.