GG-B-00686D(DSA-DM)
June 7, 1973
SUPERSEDING
Int. Fed. Spec. GG-B-00686c(DSA-DM)
September 28, 1967 and
Interim Revision of
Fed. Spec. GG-B-686b
August 13, 1957

INTERIM FEDERAL SPECIFICATION

BROACHES, PULP CANAL, BARBED, DENTAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-B-686b.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers barbed pulp canal broaches suitable for use in endodontic procedures.

1.2 Classification. The barbed pulp canal broaches shall be furnished in the following sizes, as specified (see 6.1):

Size 1. Extra fine
Size 2. Medium
Size 3. Coarse

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

QQ-A-225/5	Aluminum Alloy Bar, Rod, and Wire, Rolled, Drawn, Or Cold Finished 2017
QQ-W-423	Wire, Steel, Corrosion-resisting.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

STANDARDS

Federal

FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.)

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

SPECIFICATION

Military

MIL-L-10547	Liners, Case and Sheet, Overwrap; Water-Vaporproof Or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other Publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

E8-69	Tension Testing of Metallic Materials

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa. 19103).

3. REQUIREMENTS

3.1 Material.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.

3.1.1 Operative end. Operative end shall be fabricated of AISI 301 or 302 austenitic stainless steel having a minimum tensile strength value of 262,000 pounds per square inch (p.s.i.) when tested as specified in 4.4.1.


3.1.2 Handle. Handle shall be fabricated of either aluminum or plastic as specified in 3.1.2.1 and 3.1.2.2. Handles shall be capable of being autoclaved or dry heat sterilized without losing the shape of the handles or bleaching out the color when tested as specified in 4.4.2.


3.1.2.1 Aluminum. Aluminum rod for handles shall conform to alloy 2017-T4 of QQ-A-225/5 for chemical composition and tensile strength. Material shall be anodized to the applicable color to conform to the color coding system specified in 3.3.

3.1.2.2 Plastic. Handles shall be fabricated of plastic material which shall be impregnated with the applicable color to conform to the color coding system specified in 3.3.

3.2 Style, design, and dimensions. Barbed broaches shall be of two-piece construction, consisting of an operative end (working end, neck, and shank) and a handle. Operative end shall be securely and permanently affixed into the handle with no movement of the operative end permitted. The barbed broaches shall be suitable for use in extirpating pulpal tissue and debridement of pulp canals during endodontic procedures. The broaches shall be straight. The full diameter of the wire shall be present over the entire length of the shank portion of the broach. The working end and neck of the broaches shall be tapered along their entire length, from the full wire diameter at the base of the shank to a bullet-shaped point at the extreme tip. The working end shall include a barbed section containing a minimum of 40 barbs. The barbs shall be properly cut to a depth of 10 to 15 percent (%) of the diameter of the working end. The cross section of each barb shall increase parabolically from the tip to the base of the barb. Broaches shall be tapered for their full working length, with barbs arranged in uniformly spaced helical rows, projecting from the working end. Broaches shall be furnished in three sizes (see 6.1). Size 1 shall be extra-fine; size 2 shall be medium; and size 3 shall be coarse. Style, design, and dimensions of the broaches shall be as shown in Figure 1 and Table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

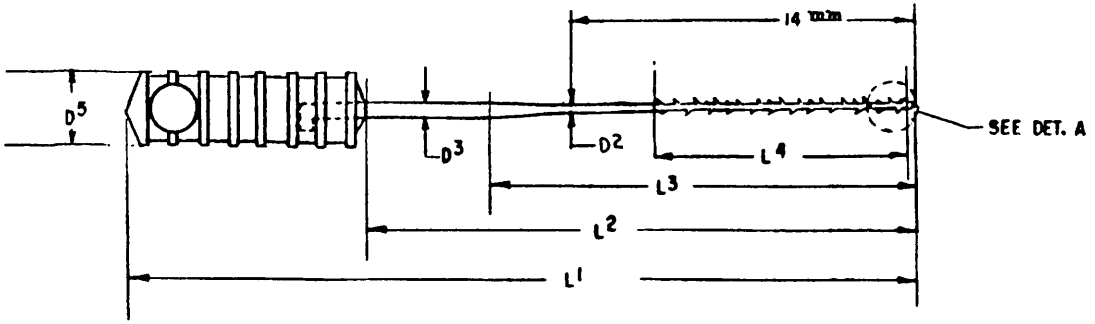

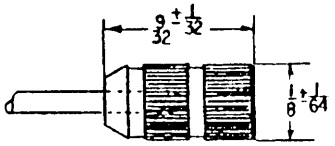


ALTERNATE HANDLE
(ALUMINUM)


NOTE: HANDLE (PLASTIC OR ALUMINUM) SHALL HAVE EITHER A HOLE OR A GROOVE FOR ATTACHMENT OF LIGATURE

GENERAL NOTES

1. DIAMETER D' SHALL BE MEASURED OVER BARBS.
2. LENGTH L4 SHALL BE THE TOTAL LENGTH OF THE BARBED SECTION.
3. LENGTH L5 SHALL BE LENGTH FROM TIP OF BROACH TO ROOT OF FIRST BARB.

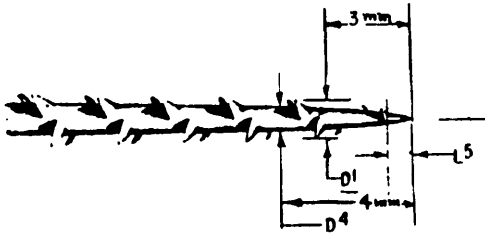

DETAIL A
(ENLARGED)

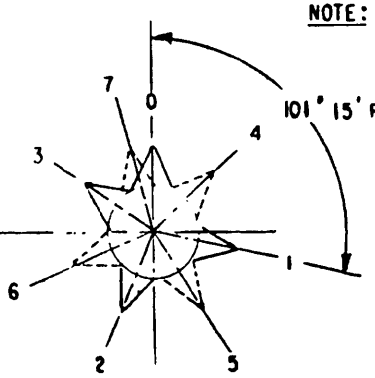

NOTE:

BARB DISTANCE IS 101° 15' WITH A STEADY SPIRAL INCLINATION OF 0.9 MM REF. BY 360° IN SEQUENCE 1 THRU 7 AS SHOWN.

NOTE: THE HANDLES SHOWN ABOVE ARE TYPICAL FOR STYLE AND DESIGN AND ARE NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF BROACHES WHICH ARE OTHERWISE IN ACCORDANCE WITH THE REQUIREMENTS OF THE APPLICABLE SPECIFICATION.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Table I. Dimensions*

Size	D_1 ±0.03	D_2 ±0.02	D_3 ±0.2	D_4 ±0.02	D_5 ±0.10	L_1 ±1.0	L_2 ±0.5	L_3 ± 0.5	L_4 ±0.5	L_5 ±0.2
Extra fine	0.49	0.32	0.60	0.25	3.0	32	23	19	10.5	1.0
Medium	0.69	0.42	0.60	0.35	3.0	32	23	19	10.5	1.0
Coarse	0.79	0.47	0.60	0.40	3.0	32	23	19	10.5	1.0

* All dimensions are in millimeters

D_1 refers to the diameter over barbs at 3 mm. from tip.
D_2 refers to the diameter at 14 mm. from tip.
D_3 refers to the shank diameter.
D_4 refers to the diameter (without barbs) at 4 mm. from tip.
D_5 refers to the handle diameter.
L_1 refers to the total length of broach.
L_2 refers to the length of the operative end.
L_3 refers to the length of the working end and neck.
L_4 refers to the length of the barbed section.
L_5 refers to the length from the tip of the broach to the base of the first barb.

Note: Barb height is based on formula $\frac{D^4}{2}$ for each size broach.

3.2.1 Figures. The figures forming a part of this specification are specification control figures. The supplier shall be responsible for preparing his own shop drawings. Where tolerances prescribed could cumulatively result in improper design, the supplier shall provide a product with dimensions within the tolerances prescribed on the drawing to insure proper design, function, fit, assembly and operation of the item. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.

3.3 Identification marking. Handles shall be color coded according to the applicable size as follows:

Color	Size
Black	Coarse
Green	Medium
Red	Extra fine

For plastic handles, the color shall be impregnated into the plastic formulation. For aluminum handles, the aluminum handle shall be anodized to produce the applicable color. The presence of a letter or word on the handle corresponding to the size of the instrument shall be optional.

3.4 Finish. Barbed section of operative end of broaches shall have a bright and smoothly cut finish. Aluminum handles shall be longitudinally serrated or shall have diamond crosscut serrations. The entire handle may be serrated or only the hand-gripping portion need be serrated. Plastic handles shall be grooved to provide a positive gripping surface.

3.5 Corrosion resistance. Broaches shall not show any evidence of corrosion when tested as specified in 4.4.3.

3.6 Barb breakage. No barbs shall break off, and not more than 10% of the barbs shall bend out of position, when tested as specified in 4.4.4 or 4.4.4.1.

3.7 Cold bends. The shank (uncut portion) of the broaches shall withstand a minimum of 8 bends, when tested as specified in 4.4.5.

3.8 Recoil. The shank (uncut portion) of the broaches shall have a recoil of no less than 22-1/2°, when tested as specified in 4.4.6.

3.9 Workmanship. Workmanship shall be first class throughout. The broaches shall be free from all defects, such as cracks, grind marks, seams, pits, or laminations, which affect their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the raw materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in Tables II and IV (see 4.2.1 and 4.3) and Table III (see 4.2.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in Table II. Unit of product for examination purposes shall be one individual broach.

Table II. Inspection and Acceptable Quality Levels

Type defect	Inspection level	AQL (Percent defective)
Major A	II	1.0
Major B	S-2	1.5
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table III, except that the acceptance number shall be zero for all sample sizes. Unit of product for test purposes shall be as specified in Table III.

Table III. Tests

Component	Characteristic	Requirement	Test procedure	Unit of product	Inspection level
Operative end	Tensile strength	3.1.1	4.4.1	Lot of steel stock	1/
Entire Instrument	Sterilization	3.1.2	4.4.2	Individual broach	S-2
	Corrosion resistance	3.5	4.4.3	Individual broach	S-2
	Barb breakage	3.6	4.4.4	Individual broach	S-2
	Cold bends	3.7	4.4.5	Lot of steel stock	1/
	Recoil	3.8	4.4.6	Lot of steel stock	1/

1/ A minimum of three specimens from each lot of steel stock.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.

4.2.3 Raw materials. A sufficient quantity of each lot of each raw material used in the construction of the broaches shall be selected for chemical analysis.

4.3 Examination. Broaches shall be examined for defects, including, but not limited to, those listed in table IV.

Table IV. Classification of defects

Category	Defect
Major A:	
101	Working end and neck of broach not tapered from base of shank to extreme tip.
102	Broach not free from cracks, grind marks, seams, pits, laminations or other defects which may impair serviceability.
103	Broach not barbed.
104	Style and design not as specified.
105	Barbs not arranged in uniformly spaced helical rows.
106	Finish of operative end not as specified.
107	Operative end bent, deformed, or otherwise damaged.
108	Operative end not firmly affixed in handle.
109	Handle not properly color coded for applicable size.
Major B:	
151	Operative end dimensions not as specified in Figure 1 and Table I.
152	Number of barbs not as specified

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the current version before use.

Table IV. (Cont'd.)

Minor A:	
201	Tip of broach not bullet-shaped.
202	Rust or other corrosion present.
203	Packaging and packing not as specified.
204	Marking illegible, incorrect or incomplete.
205	Finish of handles not as specified.
Minor B:	
251	Dimensions of handles not as specified in Figure 1 and Table I.

4.3.1 Dimensions. Examination of the dimensions, as listed in 3.2, shall be made with a toolmaker's microscope, comparator, or other instrument of equal accuracy. Manufacturer's gages may be used if properly calibrated checking standards are used in conjunction with them.

4.3.2 Microscopic examination. Examination of broach defects not readily perceptible to the naked eye shall be made using a microscope at 4 power (4X) magnification.

4.4 Tests.

4.4.1 Tensile strength. Tensile strength test shall be performed in accordance with the American Society for Testing and Materials (ASTM) Designation E8-69.

4.4.2 Sterilization test. The finished broaches shall be autoclaved under 27 pounds of pressure at 132 degrees Centigrade (°C.) (270 degrees Fahrenheit, °F.) for 20 minutes and dry heat sterilized at 160° C. (320° F.) for 120 minutes. The handles shall then be examined for compliance with specification requirements.

4.4.3 Corrosion resistance. Before testing, broaches shall be scrubbed with soap and water, rinsed thoroughly in distilled water, and dried. After cleaning, the broaches shall be boiled in distilled water in a glass beaker for 30 minutes and allowed to remain submerged for 24 hours.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4.4.4 Barb breakage. The shank portion of the barbed broach shall be held by means of hemostatic forceps or other suitable holders. The barbed section shall then be placed between two sheets of smoothly polished acrylic resin, and the required load, as shown in table V for the applicable size, applied to the top surface of the upper sheet. The applied load includes the weight of the upper sheet of acrylic resin. The broach shall then be pulled forward through the two sheets of resin. Only one forward movement shall be considered in this test.

Table V. Barb Breakage Test Loads

Broach size	Applied load
1	12 ounces
2	2 pounds
3	4 pounds

After completion of the test, the barbs shall be examined under a microscope for evidence of breaking and bending out of position.

4.4.4.1 Alternate test for barb breakage. As an alternate test, the shank of the barbed broach shall be held between the thumb and index finger. The barbed section shall be rubbed across a sheet of smoothly polished acrylic resin with ten back and forth movements (similar to a sawing motion) for a distance three times the length of the barbed section. After completion of the test, the barbs shall be examined under a microscope for evidence of breaking or bending out of position.

4.4.5 Cold bends. Test for cold bends shall be conducted as specified in QQ-W-423, except that the wire shall withstand a minimum of 8 bends.

4.4.6 Recoil. One 90-degree bend on the wire used for the shank, around a pin 1/4 inch in diameter, shall be made using a suitable recoil gage at the rate of 90 degrees per second, and the tension released. The pointer on the gage shall be brought up to the bent portion of the shank and the number of degrees of recoil recorded.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.1).

5.1.1 Unit of issue. One package, containing 12 broaches, as specified constitutes one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table VI. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	720 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A

5.1.3.1 Unit package. Each unit (12 broaches) shall be packaged in a plastic box with a slipover cover. Plastic box shall be designed with twelve cavities to hold broaches in place and prevent movement without cushioning. Closure shall be adequate to prevent accidental opening.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable; or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.1).

5.2.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with paragraph 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Size required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 National Stock Number (NSN) Coverage. This specification covers the following items appearing in the Federal Supply Catalog:

Stock No.	Item Identification
6520-00-117-7641	BROACH, PULP CANAL, Barbed, Medium, with Handle, 12s
6520-00-117-7658	BROACH, PULP CANAL, Barbed, Coarse, with Handle, 12s
6520-00-117-7692	BROACH, PULP CANAL, Barbed, Extra Fine, with Handle, 12s

6.3 Broach sizes: The broaches covered by this specification differ in one respect from those covered by GG-B-00686c(DSA-DM) in that they are dimensioned differently from those in the superseded specification. Therefore, since the broach sizes included in this specification do not correspond exactly to those in the previous specification, no attempt should be made to equate sizes from the superseded and current specification. Decision as to size of broach desired should be based on current specification requirements.

6.4 Specification changes. Because of the extensiveness of changes to this document, the margins have not been marked with an asterisk to indicate where changes from the previous issue have been made.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

6.5 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:

Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1359

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

GG-B-00686D(DSA-DM)

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.