GG-C-00921a(GSA-FSS)
June 11, 1957
Interim Revision of
Federal Spec. GG-C-921
September 28, 1948

INTERIM FEDERAL SPECIFICATION

CYSTOSCOPE

This Interim Federal Specification was developed by General Services Administration, Federal Supply Service, 7th and D Streets, S.W., Washington 25, D. C., based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized Federal agencies to use this Interim Federal Specification as a valid exception to Federal Specification GG-C-921.

1. SCOPE AND CLASSIFICATION

1.1 Scope. - This specification covers an instrument used in diagnosis and treatment of lesions of the bladder, ureter and kidney.

1.2 Classification.

1.2.1 Type, Grade and Classes. - Cystoscopes covered by this specification, shall be of but one type, grade and the following classes, as specified in the invitation for bids, (see figures 1 and 2):

Class A. - Convertible, 21 French scale.
Class B. - Convertible, 24 French scale.
Class C. - Double catheterization, 16 French scale.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following standard of the issue in effect on date of invitation for bids, forms a part of this specification:

Federal Standard:
Fed. Std. No. 102 - Preservation, Packaging and Packing Levels.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D.C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material.

3.1.1 Metal parts. -The sheaths and telescopes of the cystoscope shall be of monel tubing, nickel-plated over copper. The stopcock lock assemblies and cone fittings of the sheaths and similar parts of the telescopes shall be of brass, nickel-plated over copper.

3.1.2 Rubber parts. - The rubber parts shall be made of a good quality natural or synthetic rubber compound suitable for the purpose intended.

3.2 General description. - Cystoscopes shall be of the Borwn-Buerger design.

3.2.1 Sheaths. - The sheaths shall be of ovate shape to permit easy passage, to permit proper seating of the telescope, and to provide maximum catheter capacity.

3.2.2 Examining telescope. - The examining telescope shall have right-angle vision and shall be of maximum size proportionate to the size of the sheaths for which it is intended.

3.2.3 Convertible telescope. - The convertible telescope shall have right-angle vision with a field sufficiently large to permit easy catheterization of ureters, and operative procedures.

3.2.3.1 At the proximal end, the telescope shall have three channels terminating in a common outlet in the cone fitting. The two smaller side channels shall be used for simultaneous catheterization when the fin is in place. For operative procedures with fin removed, the center larger channel shall be employed.

3.2.3.2 The telescope shall have a suitable deflector mechanism mounted proximal of the objective lens and actuated by the knurled knobs at the proximal end of the telescope.

3.2.4 Double catheterizing telescope. - The double catheterizing telescope shall be similar in appearance to the convertible telescope, except that two catheterizing channels only shall be incorporated. No fin shall be required with the double catherterizing telescope.

3.2.5 Obturator. - An obturator of appropriate size shall be a component of each cystoscope. The one obturator shall fit both sheaths (concave and convex) supplied with each cystoscope.

3.3 Case. - Each cystoscope unit shall be packed in a case of selected walnut, which shall be well seasoned and polished to a durable finish. It shall have a hinged cover and adequate locking device. Cases shall be individually designed for each unit and shall be constructed to afford adequate protection

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the currenversion before use.

for the instruments. Felt pads shall be used where necessary, and all parts shall be fitted to the case.

3.4 Accessories. - With each cystoscope unit there shall be included two extra lamps for each lamp used in the unit, six non-perforated, and six perforated small rubber tips, two nonperferated and two perforated large rubbe tips, one 6-foot sterilizable conducting cord with suitable connections, stop-cock for the water supply, catheter clip, cleaning rod, and a small container of compound for waterproofing lamp threads, cone, or other parts of the instrument.

3.5 Name plate. - A metal or plastic plate shall be attached to the inside of the case cover. The plate shall show the name of the manufacturer name of the instrument designer, and such directions for assembling or maintenance of the instrument as the manufacturer deems necessary.

3.6 Class A cystoscopes, convertible, 21 French scale. - Class A cystoscopes shall consist of the following:

(a) One convertible telescope with double catheterizing fin
(b) One concave sheath
(c) One convex sheath
(d) One right-angle examining telescope
(e) One obturator

3.7 Class B cystoscopes, convertible, 24 French scale. - Class B cystoscopes shall consist of the following:

(a) One convertible telescope with double catheterizing fin.
(b) One concave sheath.
(c) One convex sheath.
(d) One examining telescope.
(e) One obturator

3.8 Class C cystoscopes, double catheterization, 16 French scale. - Class C cystoscopes shall consist of the following:

(a) Double catheterizing telescope.
(b) One concave sheath.
(c) One convex sheath.
(d) One right-angle examining telescope.
(e) One obturator.

3.9 Workmanship. - The workmanship shall be first class throughout The cystoscopes shall be symmetrically made, smoothly and properly finished, highly polished, and free from defects of material or plating which detract from their appearance or which may impair their serviceability. All parts shall fit easily and accurately.

4. SAMPLING, INSPECTION AND TEST PROCEDURES

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the current version before use.

4.1 Sampling and inspection. - Each cystoscope shall be inspected for material, workmanship, accessories, marking, presence of parts, size, construction, and packing.

5. PREPARATION FOR DELIVERY

5.1 Packaging. - Unless otherwise specified, commercial packages are acceptable under this specification.

5.2 Packing. - Unless otherwise specified, the subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to the point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Packages. -Unless otherwise specified, each unit shall be marked with the name of the item, class, stock number, and the name of the manufacturer or contractor.

5.3.2 Shipping containers. - Unless otherwise specified, each shipping container shall be marked with the name of the item, class, quantity contained therein, as defined by the contract or order under which shipment is made, the name of the manufacturer or contractor, the number of the contract or purchase order, and the gross weight.

6. NOTES

6.1 Federal Standard 102 should be referred to for definitions and applications of the various levels of packaging protection for supplies and equipment.

6.2 Purchasers should exercise any desired options offered herein (See 1.2.1, 5.1, 5.2, and 5.3).

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:53Z
Check the source to verify that this is the current version before use.

6.4 Federal specifications do not include all types, classes, grades, sizes, etc., of the commodities indicated by the title of the specifications, or which are commercially available, but are intended to cover the types, etc., which are suitable for Federal Government requirements.

6.5 Transportation description.

(To be furnished).

6.6 French scale. - One unit on the French scale is equivalent to 0.33 millimeter.

Notice. - When Government drawings, specifications or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility, nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is nct to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

GSA-WASH DC 57-14041

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the current version before use.

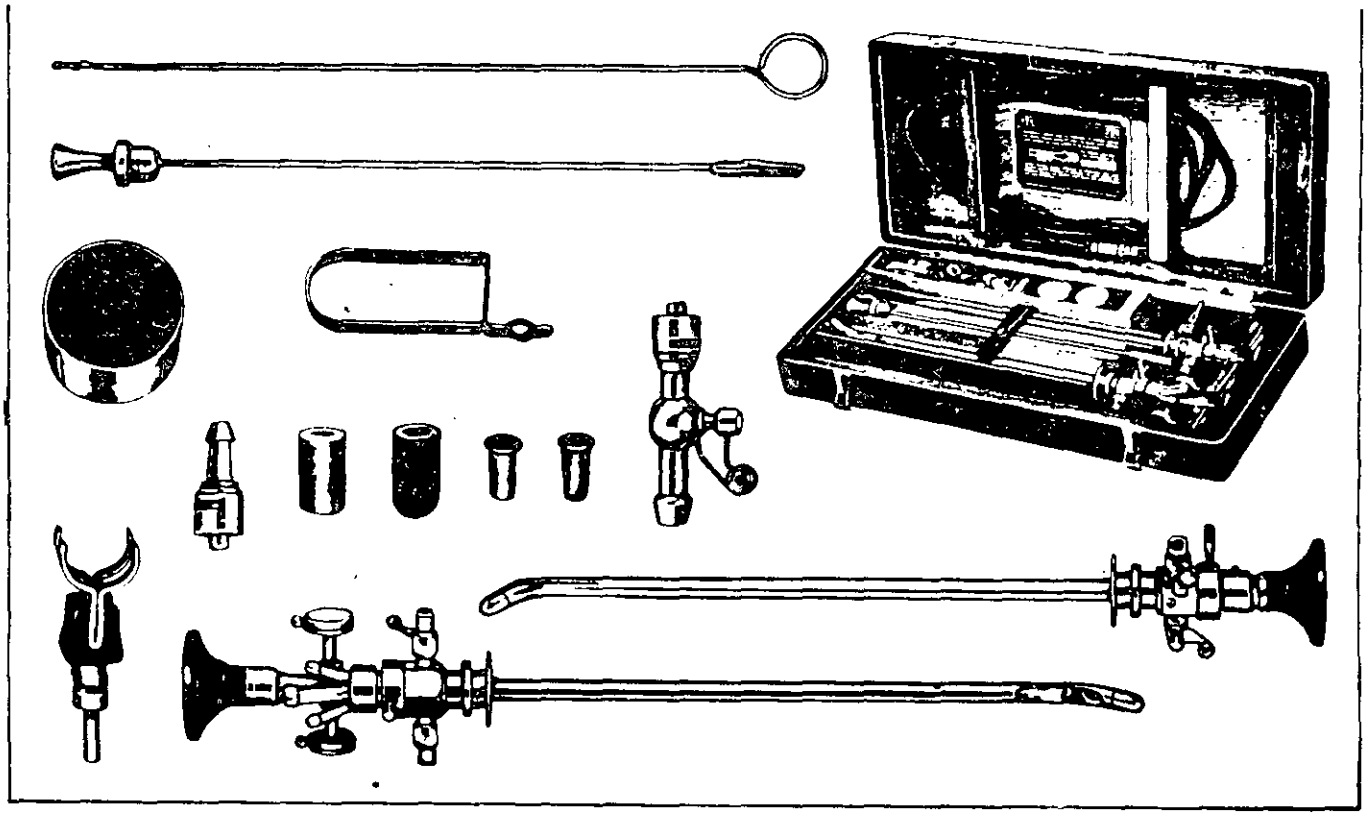


Figure 1.- Class A and class B cystoscope, convertible.

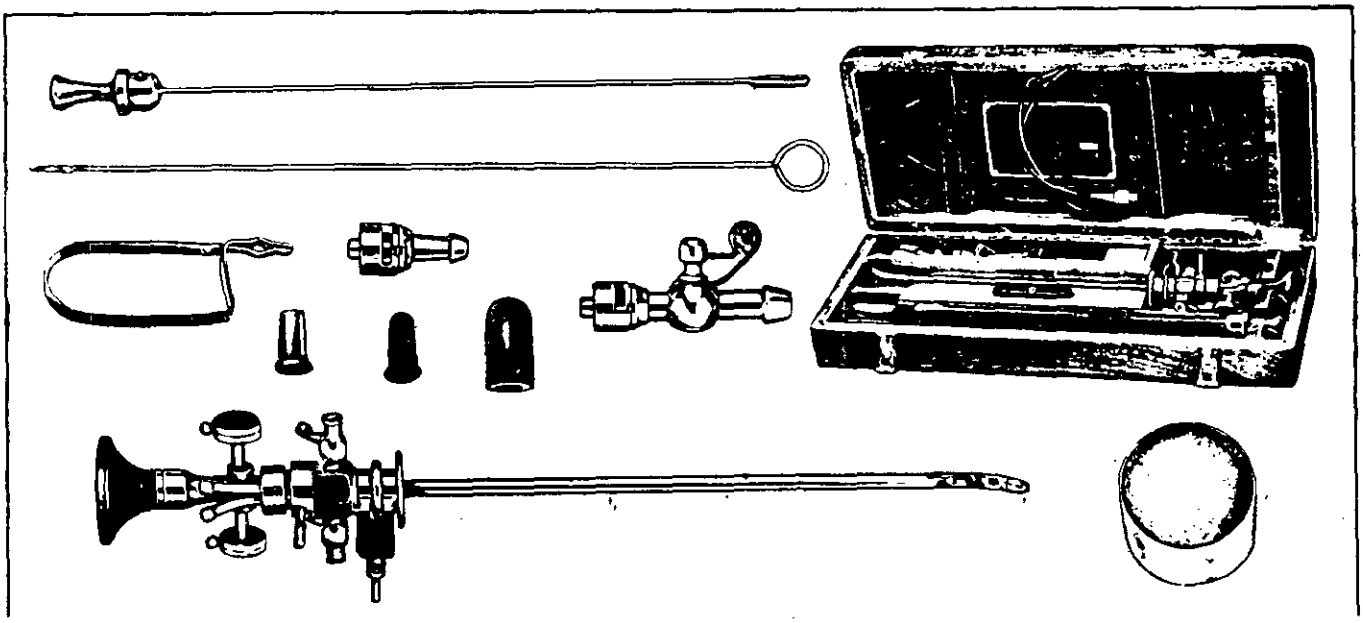


Figure 2.- Class C cystoscope, double catheterization.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.