GG-I-488C/GEN
September 8, 1976
SUPERSEDING
Fed. Spec. GG-I-488B
March 20, 1957

# FEDERAL SPECIFICATION

# INCUBATOR, BACTERIOLOGICAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

## 1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers the general requirements for bacteriological incubators suitable for use in laboratories and hospitals for incubation and development of microorganisms.

1.2 Classification. Types and classes shall be as designated in the detail specification for each incubator.

## 2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on the date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

| | | |
|---|---|---|
| PPP-B-601 | - | Boxes, Wood, Cleated-Plywood. |
| PPP-B-621 | - | Boxes, Wood, Nailed and Lock-Corner. |
| PPP-B-636 | - | Boxes, Shipping Fiberboard. |
| PPP-B-1055 | - | Barrier Material, Waterproofed, Flexible. |

Federal Standards:

Fed. Std. No. 66 - Steel: Chemical Composition and Hardenability.

FSC 6640

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL-M-7298 - Manual, Technical: Commercial Equipment.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless a specific issue is identified, the issue in effect on date of invitation for bids or request for proposal shall apply:

National Fire Protection Association:

No. 70 - National Electrical Code.

(Application for copies should be addressed to the National Fire Protection Association, 85 John Street, New York, NY 10038; 222 West Adams Street, Chicago, IL 60606; or 465 California Street, San Francisco, CA 94104.)



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

Underwriters' Laboratories (UL), Inc.

No. 499 - Standard for Electric Heating Appliances.

(Applications for copies should be addressed to the Underwriters' Laboratories, Inc., 207 East Ohio Street, Chicago, IL 60611; 1285 Walt Whitman Road, Melville, L.I., NY 11746; or 1655 Scott Boulevard, Santa Clara, CA 95050.)

American National Standards Institute (ANSI).

C73.11 - Dimensions of Plugs and Receptacles - General Purpose, 125 Volts, 15 Amperes, 2 - Pole, 3 - Wire, Grounding Type.

(Application for copies should be addressed to the American National Standards Institute, 1430 Broadway, New York, NY 10018.)

3. REQUIREMENTS

3.1 Material. The material used in the manufacture and assembly of the incubators shall be as specified in the detail specification. All metals shall be suitably protected against corrosion. Commercial tolerances shall apply to all thicknesses of material.

3.2 Fire and casualty hazards.

3.2.1 The contractor shall submit proof, prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of UL Standard No. 499. Proof shall consist of one of the following:

a. The UL label or the UL listing of the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the UL report directly to the Contracting Officer, upon the latter's request.

b. Laboratory report from a qualified independent laboratory. If an independent laboratory is used, it shall be adequately equipped and competent to determine compliance with UL standards. The qualifications of such laboratory shall be determined by the Government, which reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacing between electrical components, types of bushings, photographs, wiring diagrams, sketches and parts list, all appropriately identified.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3.3 Design. The design for the various incubator types, styles, and models shall be as specified in the detail specification. (see 6.4)

3.3.1 Dimensions. Dimensions of incubators shall be as specified in detail specification.

3.3.2 Thermometer. A thermometer shall be located on the top of the incubator, so that it may be easily read without removal. The thermometer shall be an engraved-on stem type having a temperature range from 0°C to 70°C, in 1/2°C subdivisions. The stem immersion shall be approximately 170 mm with scale starting approximately one inch above immersion line. The outside diameter shall be approximately 6 to 7 mm, and the overall length shall be approximately 335 mm. The 37°C and 56°C graduation lines shall be marked with a red color. Accuracy shall be ± 0.5°C from 0°C to 70°C. The thermometer shall be constructed with an integral bead to facilitate insertion into retainer or as an alternate the thermometer shall be supplied with a suitable compression type holder. Suitable means shall be provided to prevent air from entering the incubator around the thermometer. (see 6.3)

3.3.3 Doors. Doors shall have a minimum of two hinges and a latch fabricated of iron, steel or chromium plated brass. Iron and steel hardware shall be suitably finished to resist corrosion. Hinges for doors shall be sturdy and free from binding. Latches shall be rugged and of a suitable positive closure type. As an alternate a stainless steel continuous hinge, of sufficient thickness to support the doors shall be used. The continuous hinge shall be the full height of the doors.

3.3.4 Insulation. The incubators shall be adequately insulated with a minimum of 3 inch thick blanket of asbestos air cell or glass wool insulation to maintain the required internal temperatures within the tolerances stated in the detail specification. Insulating material shall be installed between all inner and outer surfaces including the door assembly. The insulating material shall be so installed and of sufficient density to prevent settling. The insulation shall be nonhygroscopic, noncombustible and nonpowdering. The seams of the inside walls shall be flow soldered or continuously welded to prevent the infiltration of moisture from the inner chamber to the insulation, the infiltration of insulation into the inner chamber or the collection of grime.

3.3.5 Ventilation. The incubator shall be constructed so that air shall enter at the bottom of the cabinet and be evenly diffused before entrance into the working chamber. Air flow patterns shall be such as to insure even distribution and accurate temperature control. Complete loading of lower shelf shall permit passage of rising air currents. The exhaust shall be through an adjustable ventilating shutter provided in the top of the cabinet.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3.3.6 Identification marking. In addition to commercial markings, the National Stock Number and contract or purchase order number shall be legibly and permanently shown on the outside of the cabinet. The additional markings may be secured by adhesives.

3.4 Electrical system.

3.4.1 Heating unit. The heating unit shall consist of a heater bank with nickel chromium wire or ribbon wound on porcelain or other suitable insulating material and supported by corrosion-resisting steel frames. The power requirements shall be as specified in the detail specification. The incubator shall be equipped with a terminal block to which the heater banks shall be connected. The terminal block shall be located within a control compartment that is accessible to the user. The heating units shall be sufficiently covered, top and bottom, with perforated covers to provide protection from damage, without restricting uniform air circulation throughout the incubator. The heating units shall be designed for operation at black heat. The heating units shall be located at the bottom of the cabinet and positioned to supply optimum heat distribution throughout the incubator without causing hot-spots. The entire heating units shall be easily replaced. The heating units shall have a life expectancy of five years. The heating units shall be designed to operate on the voltages specified in 3.4.2. Two suitable bus bars shall be provided for converting from one voltage requirement to the other without the use of special tools. One of the bus bars shall be clearly marked "115 VOLTS AC" and the other "230 VOLTS AC". A permanent plate shall be attached to the exterior of the access panel clearly showing the various wiring connections.

3.4.2 Operating voltage. - The incubator shall be suitable for use on 115-230 volts, 50/60 Hertz, single phase, alternating current. The incubator shall be operable with a $\pm$ 10 percent variation in the 115 volt and 230 volt supply lines.

3.4.3 Indicator lights. Indicator lights shall be provided as specified in the detail specification.

3.4.4 Power cord and plug. The incubator shall be supplied with a 3 wire, 12 AWG heavy duty heater type cord fitted with a plug. The power cord shall have a minimum length of 6 feet from the outside of the incubator to the plug. The plug shall be a 2 pole, 3 wire, grounding type with an ampacity of 25 amperes at 125 volts as specified in ANSI C73.11. The plug shall be marked with the following or similar warning: "For use with 115 VAC only. If incubator is to be used in 230 VAC supply, obtain appropriate plug for receptacle available."



Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the current version before use.

3.4.5 Temperature control. The temperature control shall be a linear expansion, bi-metallic-type suitably enclosed for protection from damage, or shall be an enclosed thermo-regulator of the expanding capsule type. Contact points shall be silver or silver cadmium, and access shall be provided for renewing or polishing their surfaces. The control shall be capable of maintaining constant temperature over the entire temperature range specified in the detail specification with not more than ± 1/2°C variation after chamber temperature has been stabilized. A suitable suppressing device shall be provided for maintaining the temperature control knob in position to prevent accidental movement or creeping due to vibration.

3.5 Tests.

3.5.1 Dielectric test. There shall be no electrical breakdown when tested as specified in 4.4.1.

3.5.2 Incubator temperature. When tested as specified in 4.4.2.1, the maximum allowable variation between the incubator temperature and the following: the thermometer readings, individual measuring points or shelf temperatures, shall be in accordance with table I. In addition, the amplitude of the individual measuring points (maximum to minimum) shall not exceed the value indicated in table I:

TABLE I. Maximum variation from incubator temperature

| Incubator temp. (°C) | Thermometer reading. (± °C) | Individual measuring point. (± °C) | Shelf temp. (± °C) | Maximum amplitude (°C) |
|---|---|---|---|---|
| 37 | 1.5 | 1.5 | 1.5 | 2.0 |
| 56 | 1.5 | 1.5 | 1.5 | 2.0 |

3.5.3 Sustained incubator temperature test. When tested as specified in 4.4.2.2, the incubator temperature shall be maintained within 1°C over the test period.

3.6 Service data (Military requirements). The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual, for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract or purchase order. In addition, the contractor



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request to the Contracting Officer. Waiver of submission of 15 additional copies shall be at the option of the Government.

3.7 Spare parts. Each incubator shall be furnished with the following spare parts:

(a) One complete set of replacement heater elements.
(b) One spare thermometer.
(c) Two indicator lamps.

3.8 Floor stand. When specified in the invitation for bids a floor stand shall be furnished. The stand shall consist of four steel legs, approximately 32 inches high with a steel shelf located approximately 12 inches above the floor. Unless otherwise specified in the invitation for bids, the stand shall be finished in a color to match the incubator.

3.9 Workmanship. Workmanship shall be first class throughout. The incubator shall be free from defects which detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificate of quality. Certificate of quality, supplied by the manufacturer of the sheet steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in table II. Unit of product for examination purposes shall be one incubator.

TABLE II. Sampling for examination

| | Inspection level | AQL (percent defective) |
|---|---|---|
| For visual examination | | |
| Major defects | II | 1.0 |
| Minor defects | II | 2.5 |
| For dimensional examination | S-1 | 2.5 |

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table III. Unit of product for tests shall be one incubator.

TABLE III. Sampling for tests

| Characteristic | Requirement | Test procedure | Inspection level | AQL |
|---|---|---|---|---|
| Dielectric strength | 3.5.1 | 4.4.1 | 100% | 1/ |
| Incubator temperature | 3.5.2 | 4.4.2.1 | S-2 | 1/ |
| Sustained temperature | 3.5.3 | 4.4.2.2 | S-2 | 1/ |

1/ Acceptance number shall be zero.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

4.3 Examination.

4.3.1 Incubator. The incubators shall be examined for defects including, but not limited to, those listed in table IV.

TABLE IV. Classification of defects

| Category | Defect |
|---|---|
| Major: | |
| 101 | Component part missing. |
| 102 | Incubator not free of sharp edges. |
| 103 | Welds not free of cracks and porosity. |
| 104 | Screws and bolts not secured. |
| 105 | Doors cannot be closed securely. |
| 106 | Thermometer graduations not present, complete, correct, or legible. |
| 107 | Shelves not sliding smoothly and easily while being inserted, withdrawn or positioned within chamber. |
| Minor: | |
| 201 | Metal surfaces of incubator not free of pits and burrs. |
| 202 | Metal surfaces not free of dents, cracks and scratches. |
| 203 | Welds not smoothly polished. |
| 204 | Plating does not adhere. |
| 205 | Identification marking not present, complete, correct, legible, or permanent. |

4.3.2 Dimensions. The incubators shall be examined for defects in dimensions. Any dimension not within the tolerance specified in the detail specification shall be classified as a defect.

4.3.3 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing and marking comply with the requirements of Section 5. Defects shall be scored as specified in table V. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 (expressed in terms of percent defective).



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

TABLE V. Examination of preparaion for delivery

| Examination | Defect |
|---|---|
| Containers | Not as specified. |
| Quantity | Quantity in interior packages and shipping containers not as specified. |
| Packaging and packing material | Any component missing or damaged. |
| Workmanship | Inadequate application of components or containers distorted. |
| Markings | Omitted, incorrect, illegible, improper size, location, sequence, or method of application. |

4.3.3.1 Examination of closure of shipping containers. When shipping containers are required to comply with PPP-B-601 or PPP-B-621, examination for defects in closure shall be in accordance with the appendix of the appropriate box specification.

4.4 Tests. Tests shall be conducted to determine compliance with requirements specified herein.

4.4.1 Dielectric test. The incubator shall be raised to maximum operating temperature, by normal means, prior to performance of the dielectric test. Each incubator shall be tested by applying a 60 Hertz potential of 1000 volts, plus double the line voltage, for a period of 1 minute, between the current carrying parts and the metal non-current carrying parts. All current carrying parts shall be in the circuit.

4.4.2 Temperature tests.

4.4.2.1 Incubator temperature test.

4.4.2.1.1 Preparation. The incubator shall be set up in a room free from excessive air currents and changing ambient temperatures. The positioning of the incubator thermometer, the setting of the exhaust ventilation and the control setting shall be as specified in the manufacturer's instruction manual. Two shelves shall be placed into operating positions with the upper shelf located approximately 4 inches from the top of the incubator chamber, and the lower shelf located approximately 4 inches from the bottom of the incubator chamber. Five thermocouples, prepared or stated below, shall be bolted to each of the two shelves as shown in figure 1. The thermocouples shall be Instrument Society of America (ISA) Type "T" fabricated of 30 B & S gage wire. The thermocouples shall be crimped in a Thomas & Betts (T & B) No. A-2 terminal, or equivalent, with the junctions making mechanical contact with the bottom of the terminal cavity.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

4.4.2.1.2 Incubator temperature test. The incubator shall be tested at temperatures of approximately 37°C. and 56°C., as indicated by the incubator thermometer. After the incubator has stabilized for 72 hours at each test temperature, a continuous and simultaneous chart recording shall be made of the thermocouple temperatures for a test period of sixty minutes, using a Honeywell Electronik Multipoint Recorder, or equivalent. The average of each individual thermocouple measuring point, over the test period, shall be considered the temperature for that thermocouple point. The incubator temperature shall be defined as the average of the temperatures of the ten measuring points. The shelf temperature shall be defined as the average of the temperatures of the five measuring points of each shelf. The amplitude of the individual thermocouple measuring point shall be defined as the difference between the maximum and minimum recorded temperatures during the test period.

4.4.2.2 Sustained temperature test. Following the test of 4.4.2.1, the incubator shall be stabilized at each test temperature and shall be continuously operated for a minimum period of 24 hours. For the final 8-hour period, the thermocouple temperatures shall be recorded in accordance with 4.4.2.1.2. The incubator temperature shall be determined from the recordings for the last 30-minute period of each hour.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.3).

5.1.1 Level A. Each unit shall be disassembled as far as is practicable. Disassembled parts shall be packaged as specified in 5.1.1.1 through 5.1.1.3.


5.1.1.1 Accessories. Accessories and spare parts (see 3.7) shall be wrapped in kraft paper and packaged in a box of appropriate size constructed in accordance with PPP-B-636, class domestic. Box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to the contents. Closure shall be adequate to prevent accidental opening.

5.1.1.2 Shelves. Shelves shall be adequately secured within the oven in a manner to prevent shifting and damage.

5.1.1.3 Cabinet. Cabinet shall be protected by wrapping with kraft paper and cushioning with flexible corrugated fiberboard or other suitable materials. Wrapping and cushioning materials shall be secured by tying or taping. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit. Doors shall be adequately secured to prevent accidental opening.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

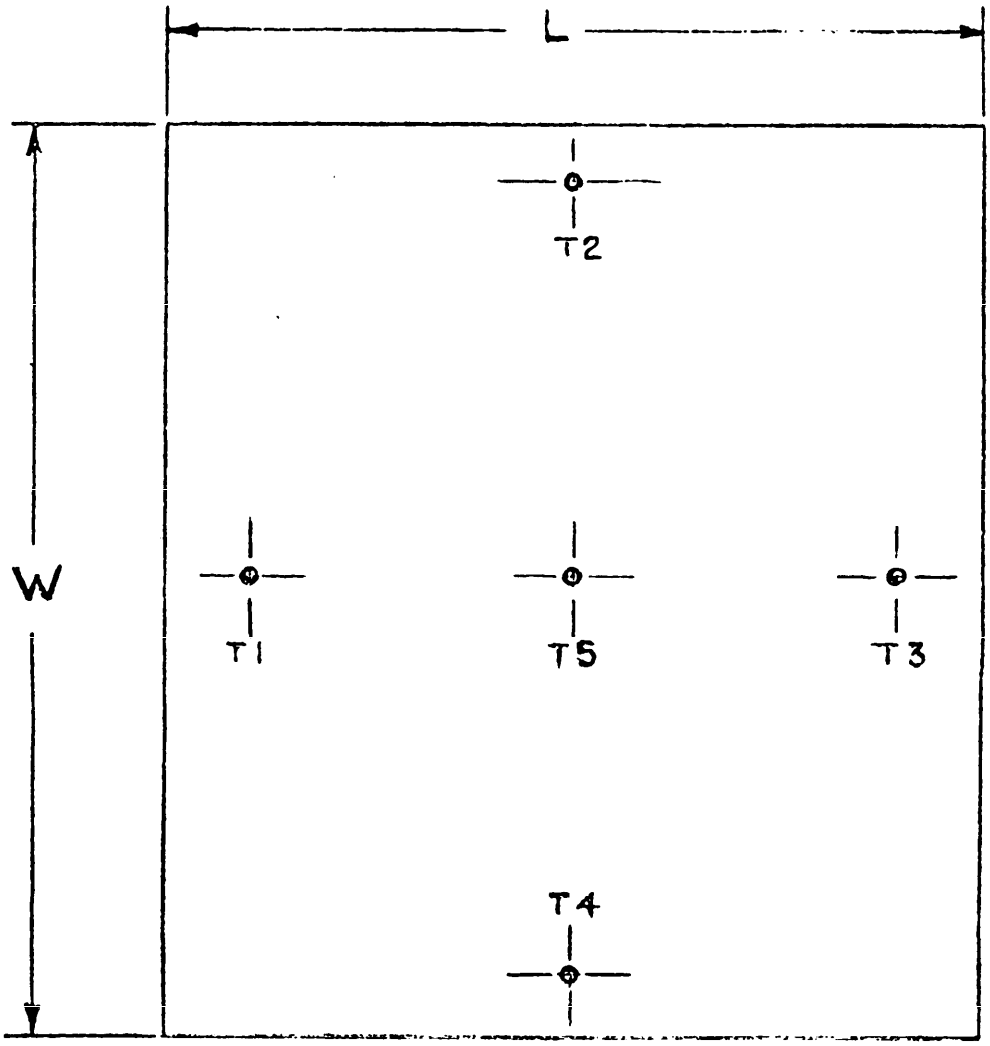


L = WIDTH OF SHELF
W = DEPTH OF SHELF

| THERMOCOUPLE LOCATION | DISTANCE FROM EDGE OF WAL |
|---|---|
| T 1 | 1/5 L (4 INCHES MIN.) |
| T 2 | 1/5 W (4 INCHES MIN.) |
| T 3 | 1/5 L (4 INCHES MIN.) |
| T 4 | 1/5 W (4 INCHES MIN.) |
| T 5 | GEOMETRIC CENTER OF SHELF |

NOTE: LINES CONNECTING T2-T4 AND T1 - T3 SHALL INTERSECT AT T5

FIGURE 1. Location of thermocouples on shelves



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

5.1.2 Level C. Each unit shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be levels A, B or C as specified (see 6.3).

5.2.1 Level A. Each unit shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-601, overseas type, or PPP-B-621, class 2. The unit shall be adequately secured within the exterior container by means of bolts, wood braces, or other interior fittings, to insure against shifting, breakage, or marring or denting of surfaces. The unit shall be secured within the container in such a manner so the weight of the unit does not rest directly on its legs. Adequate cushioning material shall be used between all bracing and the unit. The exterior container design shall include three skids of not less than 1-1/2 inches in thickness applied crosswise of base, so positioned as to facilitate handling and maintain the unit in an upright position. Closure shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. All inside box panels, except the base, shall be lined with waterproof barrier material conforming to PPP-B-1055, in such a manner as to prevent direct entry of water.

5.2.2 Level B. Each unit shall be packed as specified in 5.2.1 except the boxes shall be of the domestic type and case liner shall not be required.

5.2.3 Each unit shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance, and safe delivery by common or other carriers, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Interior packages shall be marked to identify contents.

5.3.2.2 Exterior container. Each exterior container shall be marked as specified in MIL-STD-129. The legend, "OPEN THIS SIDE", shall be shown, where applicable, to facilitate locating service data, inspecting, and removing the unit.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. (see detail specification)

6.2 Ordering data. (see detail specification)

6.3 A thermometer which meets the requirements specified in 3.3.2 is NSN 6685-00-299-8496.

6.4 Detail specifications. The following detail specifications form a part of this document.

| Detail Specification | Title |
|---|---|
| GG-I-488/1 | Incubator, Bacteriological, Small |
| GG-I-488/2 | Incubator, Bacteriological, Medium |
| GG-I-488/3 | Incubator, Bacteriological, Large |

MILITARY CUSTODIANS
Army - MD
Navy - MS
Air Force - 03

Preparing Activity:
DSA-DM

Civil Agency Coordinating Activities:
GSA-FSS
HEW-NIH
VA-DMS

Project No. 6640-0982

Orders for this publication are to be placed with General Services Administration, acting as agent for the Superintendent of Documents. See section 2 of this specification to obtain copies of documents referenced herein. Price 35 cents each.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
GG-I-488C/GEN INCUBATOR, BACTERIOLOGICAL

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4 REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

**DD FORM 1 JAN 72 1426**

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

GPO 1974—603-680/6126 2-1

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.