GG-N-00195B(DSA-DM)
20 September 1972
SUPERSEDING
Int. Fed. Spec.
GG-N-00195a(DSA-DM)
12 August 1970

INTERIM FEDERAL SPECIFICATION

NEEDLES, HYPODERMIC, Blood Collecting, Double, Pointed, Disposable, 20 Gage

This interim Federal specification was developed by the Directorate of Medical Materiel, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers disposable, sterile, double-pointed, blood-collecting, hypodermic needles.

1.2 Classification.

1.2.1 Types. Needles shall be of the following types, as specified (see 6.2):

Type I - Without shut-off sleeve
Type II - Multiple sample with shut-off sleeve

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

Federal Specifications:

GG-N-196	Needles; Hypodermic, for Luer Syringes.
GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper (for Carton Sealing).
MMM-A-250	Adhesive, Water-Resistant (for Sealing Waterproofed Paper).
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up, Paperboard.

Federal Standard:

Fed. Std. No. 66	Steel: Chemical Composition and Hardenability.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-S-36586	Sterilization Test Strip Set, Bacterial Spore.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

Military Standards:

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attrubutes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of Military specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

U.S. PHARMACOPEIAL CONVENTION, INC.:

Pharmacopeia of the United States

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pa. 18042.)

3. REQUIREMENTS

3.1 Material. Material shall be of the highest quality throughout and as specified herein.

3.1.1 Corrosion-resisting steel. Corrosion-resisting steel shall conform to AISI 304 in accordance with FED-STD-66.

3.2 Construction. Needle shall be double-pointed, hypodermic type. Construction shall comply with figure 1 for type I and figure 2 for type II, and needle shall consist of a cannula, hub and sheath. Needle shall be straight, and longitudinal axes of sheath, hub and cannula shall coincide. Needle shall be so constructed that it can be used to collect blood in combination with holder and blood collecting tube (see 6.1) without the use of instruments. Pushing the sheath toward the hub and turning the sheath clockwise shall turn the hub so that it screws into the orifice of the holder.

3.2.1 Cannula. The cannula shall be fabricated of corrosion-resisting steel tubing. Tubing shall be either seamless drawn or welded and drawn. Cannula shall be 20 gage in accordance with Specification GG-N-196 and shall be a straight tube with a point at each end. One point shall be for puncture of the vein (venipuncture). One point shall be for stopper puncture (see 3.2.1.1 and 3.2.1.2). Venipuncture point shall be Style a (regular bevel point) in accordance with GG-N-196.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the currentversion before use.

3.2.1.1 Type I stopper end. Type I stopper end shall be in accordance with figure 1. Puncture point shall be a short bevel with a flat or concave grind.

3.2.1.2 Type II stopper end. Type II stopper end shall have a side opening, a closed puncture point and a latex shut-off sleeve. Puncture point shall be flattened to form a hermetic seal. Side opening shall be so positioned and shall be of such size that the side opening does not obstruct the flow of blood when needle is used in conjunction with holder and blood collecting tubes (see 6.1). Shut-off sleeve shall be so constructed and positioned that it opens automatically when the blood-collecting tube is pushed forward and closes as the tube is removed (see 6.1). Type II stopper end shall be in accordance with figure 2.

3.2.2 Hub. Hub shall be fabricated of non-toxic, non-leaching thermoplastic and shall be secured to the cannula.

3.2.3 Sheath. Sheath shall be fabricated of polyethylene and shall protect the venipuncture end of the cannula.

3.3 Adherence. The cannula shall not separate from the hub when tested as specified in 4.4.1.

3.4 Resistance to breakage. There shall be no breakage, when the needle is tested as specified in 4.4.2.

3.5 Stiffness. The maximum deflection of the cannula shall not exceed 0.021 inch, when tested as specified in 4.4.3.

3.6 Corrosion resistance. The cannula shall meet the requirements for resistance to boiling in GG-1-526, when tested as specified in 4.4.4.

3.7 Deformation. The hub shall distort and shall not be functional, when tested as specified in 4.4.5.

3.8 Sterility. Needles shall be sterile, when tested with a biological indicator as specified in 4.4.6.

3.9 Freedom from pyrogens. Needles shall comply with the freedom from pyrogens requirements of the current edition of the U.S.P., when tested as specified in 4.4.7.

3.10 Safety. There shall be no deaths, discernible symptoms of toxicity, or evidence of irritation, when the needle is tested as specified in 4.4.8.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

3.11 Certificates. When inspection is made at destination, certificates of sterility (3.11.1), freedom from pyrogens (3.11.2) and safety (3.11.3) shall be submitted by the contractor to the Directorate of Medical Materiel, ATTN: DPSC-ATQ, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pa. 19101, and a copy forwarded with each shipment to the consignee. When inspection is made at source, certificates of sterility, freedom from pyrogens and safety shall be furnished to the cognizant Government Quality Assurance Representative for submission to the procuring activity.

3.11.1 Certificate of sterility. A certificate of sterility, stating that samples from each sterilizer lot have been tested and found to be sterile, shall be submitted to the procuring activity. The certificate of sterility shall include:

a. Item identification.
b. Federal stock number.
c. Contract or purchase order number.
d. Sterility lot or control number.
e. Date of sterilization.
f. Quantity of product in sterilizer lot.
g. Type of sterilization (gas, radiation, heat, steam, etc.).
h. Form of biological indicator (i.e., inoculated paper spore strip or carrier, inoculated product, or inoculated simulated product).
i. Test organism(s) and population density used.
j. Test medium, incubation temperature, incubation time, and dates of tests.
k. Number of test units.
l. Statement that samples comply with sterility tests.
m. Signature of head of laboratory or a designated qualified alternate.

3.11.1.2 Sterility lot. A sterility lot is that single quantity of product subjected to the same manufacturing operation and simultaneously sterilized in the same sterilizer chamber. Each unit package shall be clearly marked with a sterility lot (control) number and date of sterilization as specified in 5.3.2.2. Each sterility lot shall be traceable to the pertinent manufacturing lot(s).

3.11.2 Certificate of freedom from pyrogens. A certificate of freedom from pyrogens, listing all lot or control numbers, shall state that samples from each lot or control have been tested for pyrogens, as required in 3.9, and have been found to comply with requirements. The certificate shall reference the method used in determining freedom from pyrogens.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the current version before use.

3.11.3 Certificate of safety. A certificate of safety, listing all lot or control numbers, shall state that samples from each lot or control have been tested for safety, as required in 3.10, and have been found to comply with requirements. The certificate shall reference the method used in determining safety.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, or auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificate of quality. Certificate of quality, supplied by the manufacturer of the steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I. For purposes of examination, unit of product shall be one needle in the immediate container.

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T11:49Z
Check the source to verify that this is the current version before use.

Table I. For examination

Defect	Inspection level	AQL(percent defective)
For visual examination		
Major A	S-3	1.0
Major B	S-3	1.0
Minor A	S-3	2.5
Minor B	S-3	2.5
Minor C	II	2.5
For dimensional examination	S-2	2.5

4.2.2 For test. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II. Acceptance number shall be zero. For purposes of testing, unit of product shall be one needle in the immediate container.

Table II. For tests

Characteristic	Requirement	Test Procedure	Inspection level
Adherence	3.3	4.4.1	S-1
Resistance to breakage	3.4	4.4.2	S-1
Stiffness	3.5	4.4.3	S-1
Corrosion resistance	3.6	4.4.4	S-1
Deformation	3.7	4.4.5	S-1
Sterility	3.8	4.4.6	*
Freedom from pyrogens	3.9	4.4.7	**
Safety	3.10	4.4.8	**

* Sampling for sterility test shall be as indicated for "Procedural Details for Sterility Tests" for Class B, Type II, Inoculated Product or Inoculated Carrier for Parenteral Devices (see 4.4.6).

** The number of samples required for the respective tests shall be taken from each sterility lot (see 4.4.7 and 4.4.8).

4.3 Examination. The needles shall be examined for defects including but not limited to those listed in table III.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

Table III - Classification of defects

Category	Defect
Major A	
101	Point not sharp.
102	Point edges not free of feathering.
103	Point not free of hooks and bends.
104	Point not symmetrical.
105	Lumen not free of constriction.
106	Cannula not straight (deviation from longitudinal axis exceeds 3°).
107	Cannula not free of cracks.
108	Cannula not free of scale and corrosion.
109	Cannula not free of slivers.
110	Cannula not free of foreign matter.
111	Cannula not free of burrs.
Major B	
151	Threading not free of breaks.
152	Hub not free of distortion.
153	Hub not free of cracks.
154	Sleeve not present (type II).
155	Sleeve not free of tears (type II).
Minor A	
201	Cannula not free of pits.
202	Cannula not free of tool marks.
Minor B	
231	Hub not free of fins.
232	Hub not free of foreign matter.
Minor C	
261	Immediate container not free of cracks.
262	Immediate container not free of deformation.
263	Needle size and manufacturer's identification not complete, correct, legible, or permanent.

4.3.1 Dimensional examination. The needles shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Adherence. A straight pull of 5 pounds shall be applied between the cannula and the hub for a period of 1 minute.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

4.4.2 Resistance to breakage. The needle hub shall be held in a fixed position, and a force shall be applied to the distal end of the cannula, 1 inch from the hub, in order to bend the cannula in a clockwise direction through an arc of 25° from the original or neutral position. The operations shall then be reversed (i.e., bent through an arc of 25° from the neutral position in a counterclockwise direction) and, finally, the cannula shall be returned to the neutral position. This complete operation (or cycle) shall be repeated 20 times.

4.4.3 Stiffness. The cannula shall be placed across two test edges (0.002-inch radius maximum) 0.750 inch ± 0.003 inch apart. For type II needles cannula shall be so placed that the side opening is in the test area between the test edges. A load of 50 ounces ± 1/4 ounce shall be applied to the center of the span, and the resulting maximum deflection of the cannula shall be measured using a gage whose minimum graduations are not greater than 0.001 inch. The force shall be applied through an edge with a maximum radius of 0.036 inch, and shall not be farther than 0.003 inch from the center.

4.4.4 Corrosion resistance. Corrosion resistance shall be tested in accordance with the "Boil test" of GG-I-526.

4.4.5 Deformation. The needle shall be placed in boiling water for a period of 5 minutes.

4.4.6 Sterility test. The needle, with cannual sheath or other covering removed, shall be tested for sterility in accordance with the method specified in the U.S.P. for Procedural Details for Sterility Tests of Class B, Type II Inoculated Product or Inoculated Carrier for Parenteral Divices using inoculated product, inoculated simulated product, or paper spore strip (carrier). Product containing a biological indicator shall be marked or labeled so that it clearly differentiates from product intended for distribution. The incubation medium and minimum time in each case shall be soybean casein digest for 7 days for inoculated product, inoculated simulated product, or paper spore strip (carrier). The incubation temperature shall be as indicated in paragraph 4.4.6.1. The minimum number of test units, regardless of lot size, shall be 10. except for inoculated carrier which shall be 20 for Type I Sterilization and 30 for Type II Sterilization including inoculated carrier and product test units. The inspection level shall be as indicated in Table II, For tests.

Note: Blood shut-off sleeve in type II needles shall be removed and cultured either separately or in the same culture tube with the needle.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

4.4.6.1 Inoculated product or simulated product. For each type of sterilization, the organism used shall be as listed below:

Type of Sterilization	Organism	Incubation Temperature
Steam	B. stearothermophilus	55° - 65°C
Dry Heat	B. stearothermophilus, or	55° - 65°C
	B. subtilis var. niger (or globigii)	30° - 35°C
Gas	B. subtilis var, niger (or globigii)	30° - 35°C
Radiation	B. pumilus	30° - 35°C

The number of viable cells shall be sufficient to provide assurance that the product has been sterilized.

4.4.6.2 Inoculated carrier. Inoculated carriers (paper spore strips) if used shall be in accordance with MIL-S-36586. Other paper carriers shall be inoculated to be of equivalent resistance. The method of incubation and number of test units shall be as indicated in 4.4.6 Sterility test and 4.4.6.1 Inoculated product or simulated product. The method of sterilization will control the organism in the spore strip to be tested for as shown in 4.4.6.1. NOTE: When an inoculated carrier is chosen, product samples must also be tested as required by the U.S.P.

4.4.6.3 Alternate method. Suppliers conducting sterility tests or designating lots in a manner other than that indicated herein shall submit proof that the alternate method provides equal assurance concerning the sterility of the product. However, all sterility tests shall be conducted using biological indicators. Requests for approval of any alternate method of testing for sterility shall be made to the Contracting Officer, and approval obtained before employment of the alternate method on a government contract.

4.4.6.4 Product testing. Testing for sterility of the product after receipt by the government shall be without a biological indicator and in accordance with the U.S.P.

4.4.7 Freedom from pyrogens. The following test shall be performed. Place 10 needles in a sterile, pyrogen-free flask, pour 250 milliliters (ml.) of sterile, pyrogen-free saline test solution (U.S.P.) into the flask, and then heat the contents of the flask at not less than 85° Centigrade (C.) for 1 hour. The resulting saline extract shall be subjected to the "Pyrogen Test" as described in the current edition of the U.S.P.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

4.4.8 Safety. The following test shall be performed. Cover 20 needles with 30 ml. of sterile, pyrogen-free saline test solution (U.S.P.) and warm at 37°C. for 24 hours. Decant the saline and test, undiluted, for both acute toxicity and tissue sensitivity. Determine acute toxicity by injecting 1.0 ml. of the eluate intravenously into each of 10 nonfasted, healthy, 28 - to 32-gram mice. Observe the animals at 4, 24 and 72 hours after injection for any deaths or discernible symptoms of toxicity. Determine tissue reaction by injecting 0.20 ml. of the eluate into each of 10 sites on the back of a rabbit; the injections shall be made in such a manner as to raise a distinct bleb. Observe the injection sites at 4, 24, and 48 hours after injections for any evidence of redness, swelling, or hardness. Sterile, pyrogen-free saline test solution (U.S.P.) shall be injected simultaneously, as controls, to eliminate rabbits irritated by trauma.

4.4.9 Examination of preparation for delivery requirements. An examination shall be made to determine compliance with the packaging, packing and marking requirements of Section 5. Defects shall be scored in accordance with the list below. The sample unit shall be on shipping container fully prepared for delivery. The lot size shall be the number of shipping containers in the end item inspection lot. The inspection level shall be S-2 and the AQL shall be 2.5 defects per hundred units.

Examination	Defects
Marking (exterior and interior)	Omitted, incorrect, illegible, of improper size, location, sequence, or method of application.
Material	Any component missing, damaged or not as specified.
Workmanship	Inadequate application of components such as incomplete closure of container flaps, loose strapping, inadequate stapling, open and non-continuous sealed seams and closure of the immediate container. Bulged or distorted container.
Weight or content	Number per container is more or less than required; gross/net weight exceeds requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the currentversion before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One package containing 100 needles, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	10 units	50 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Individual container. Each needle with protector shall be packaged in a sealed, peel-open type container of appropriate size. The container shall be so designed as to permit ready dispensing of the needle by sterile techniques. The container shall also be capable of maintaining sterility of contents unless the container is damaged or opened.

5.1.3.2 Unit package. One hundred individual containers shall be packaged in a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.3.3 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2-inch wide tape conforming to PPP-T-76. Closing of bottom flap with adhesive conforming to MMM-A-250 or metal stitches is permitted.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the currentversion before use.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. In addition to any marking specified in the contract or order, packages and shipping containers shall be marked in accordance with the requirements of Fed. Std. No. 123.

5.3.2 Military agencies.

5.3.2.1 Individual container. Each individual container shall be commercially identified.

5.3.2.2 Unit package. Each unit package shall be marked in accordance with MIL-STD-129 and the requirements of the Federal Food, Drug and Cosmetic Act. In addition, marking shall include the lot (control) number, contract or purchase order number, name of contractor and method of sterilization. The method of sterilization (G-Gas, S-Steam, D-Dry Heat sterilization) shall be shown following the level and date of packaging. (Example "A-9/70-G"). Final sterilization shall be on or after indicated packaging date. A legend indicating that the needles are sterile, disposable, and pyrogen-free shall also be shown. In addition, marking shall include the legend: "Contents of each unopened or undamaged package guaranteed sterile."

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

5.3.2.3 Intermediate package. Each intermediate package shall be marked in accordance with MIL-STD-129. Lot (control) number, name of contractor, contract or purchase order number and method of sterilization as specified in 5.3.2.2 shall be shown. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material.

5.3.2.4 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot (control) number and method of sterilization as specified in 5.3.2.2 shall be shown.

6.1 Intended use. Needles are intended for use with the following items:

Federal Stock No.	Item Identification
6630-404-2220	Holder, Blood Collecting Tube, Plastic, 12s
6630-145-1132	Tube, Blood Collecting, Vacuum, 5 ml., with Ammonium and Potassium Oxalate, 100s
6630-145-1137	Tube, Blood Collecting, Vacuum, 7 ml., without Anticoagulant, 100s
6630-145-1143	Tube, Blood Collecting, Vacuum, 15 ml., without Anticoagulant, 100s
6630-145-1525	Tube, Blood Collecting, Vacuum, 7 ml., without Anticoagulant, 100s
6630-145-1526	Tube, Blood Collecting, Vacuum, 5.5 ml., with Citric Acid and Dextrose Solution, without Anticoagulant, 100s
6630-145-1527	Tube, Blood Collecting, Vacuum, 15 ml., with Lithium Oxalate, 100s
6630-145-1533	Tube, Blood Collecting, Vacuum, 7 ml., with Disodium Edetate, 100s
6630-145-1534	Tube, Blood Collecting, Vacuum, 7 ml., with Sodium Fluoride, 100s
6630-145-1535	Tube, Blood Collecting, Vacuum, 7 ml., with Sodium Fluoride and Thymol, 100s
6630-250-4264	Tube, Blood Collecting, Vacuum, 5 ml., with Sodium Citrate 100s

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Procurement documents should specify the following:

a. Title, number and date of this specification.
b. Type of needle required (see 1.2).
c. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Military custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1671

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the current version before use.

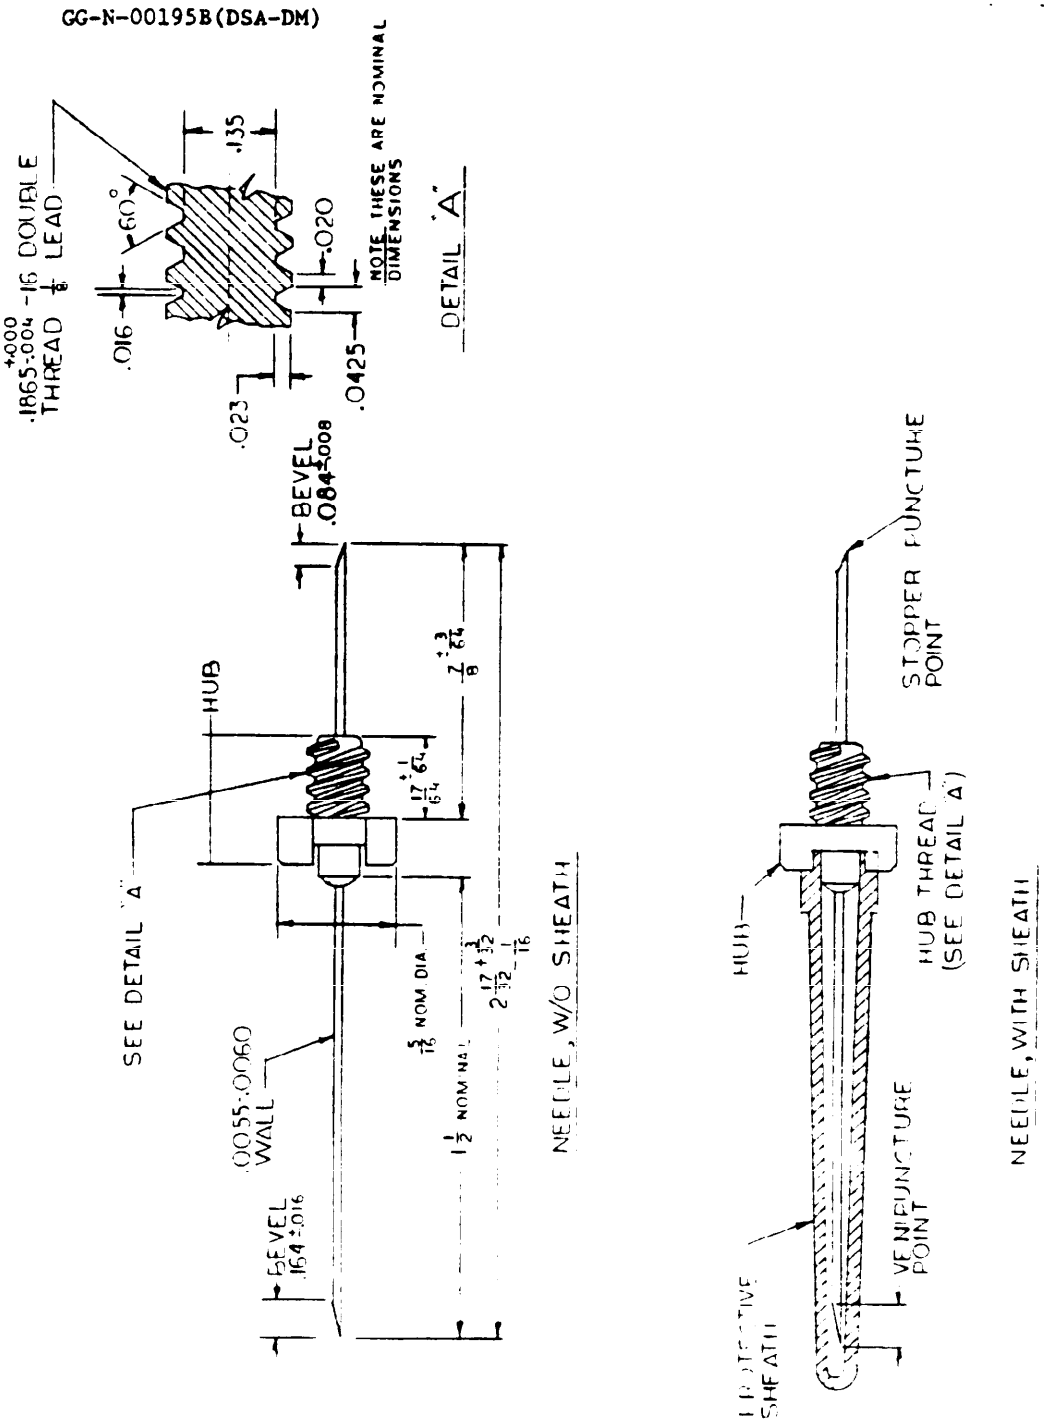


FIGURE 1 - NEEDLE, TYPE I
(WITHOUT SHUTOFF SLEEVE)

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the current version before use.

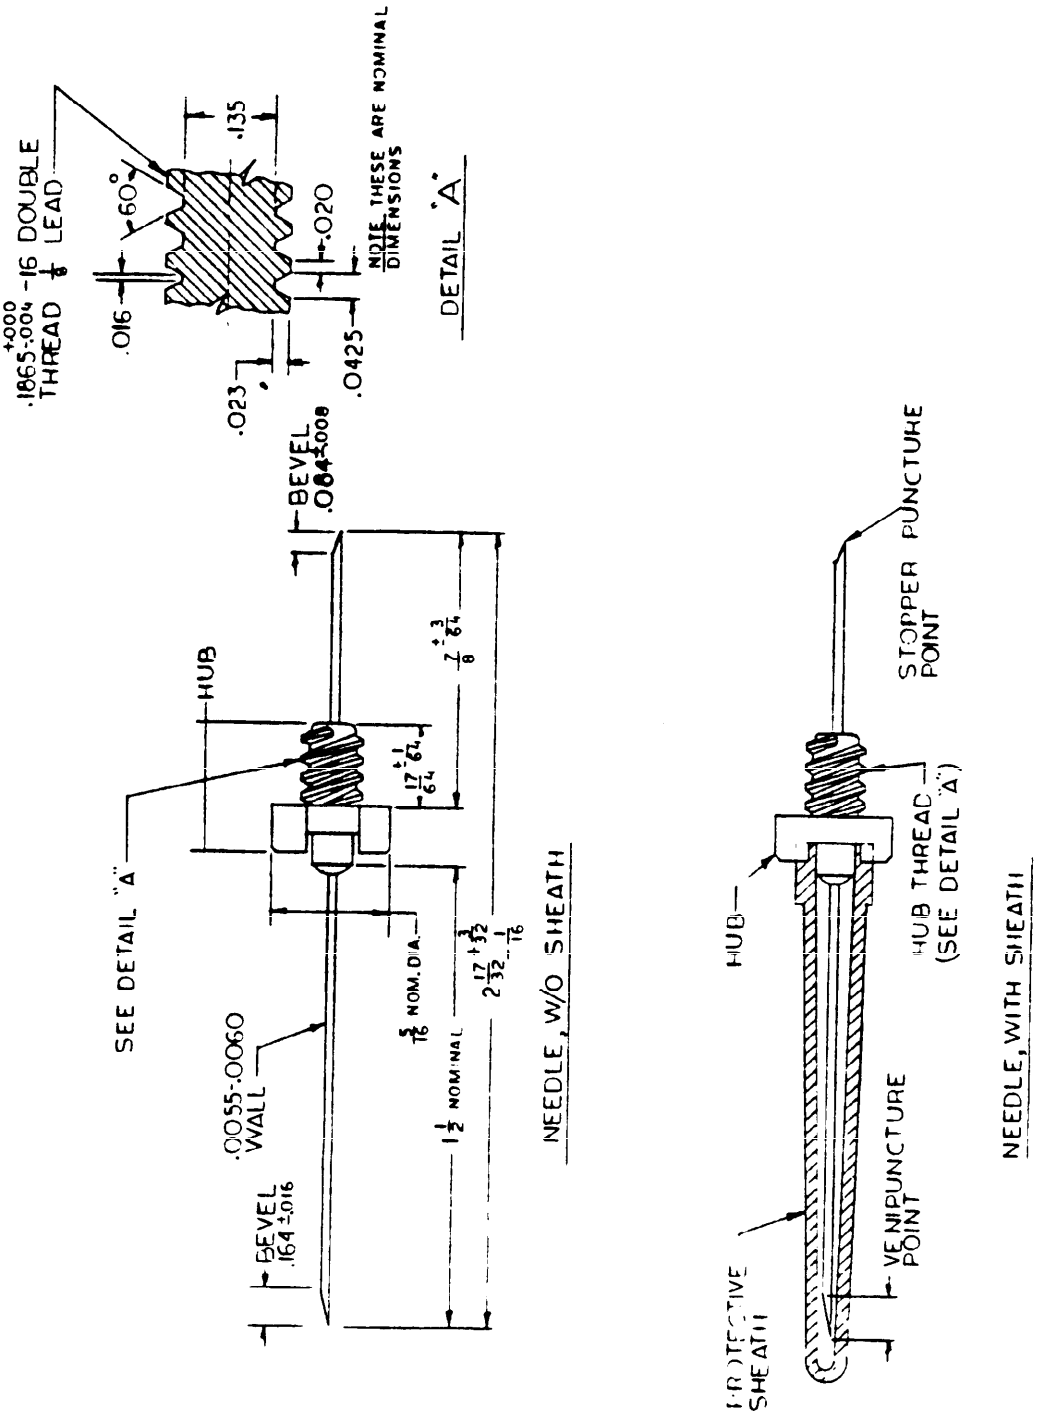
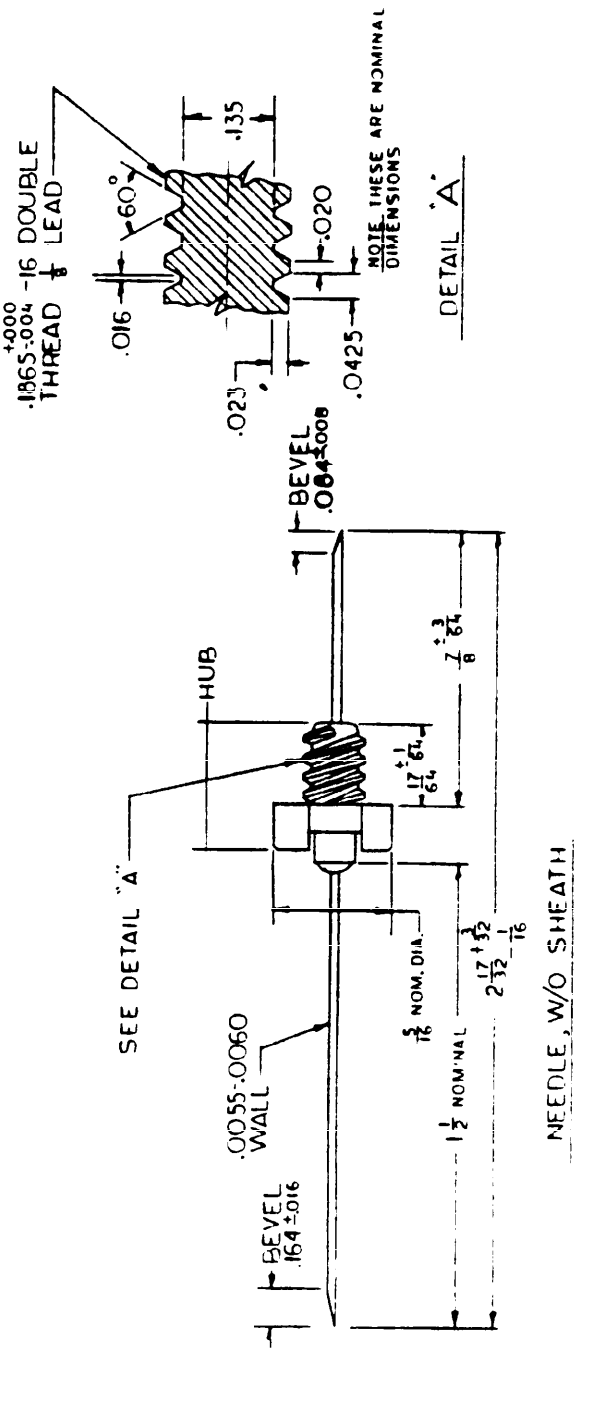


FIGURE 1 - NEEDLE, TYPE I
(WITHOUT SHUTOFF SLEEVE)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.



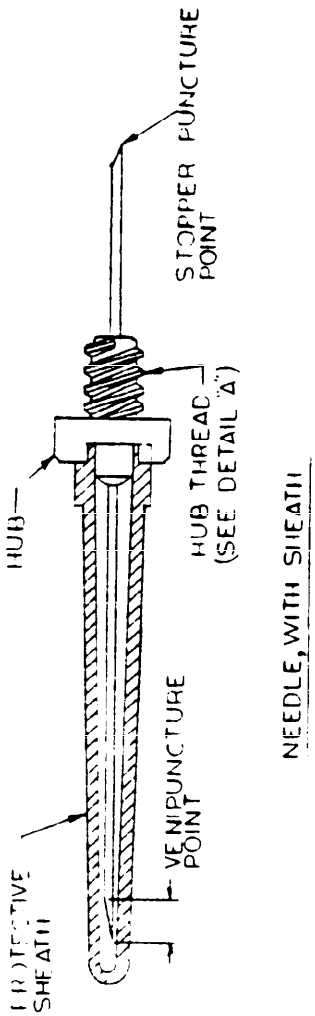


FIGURE 1 - NEEDLE, TYPE I
(WITHOUT SHUTOFF SLEEVE)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
GG-N-00195B(DSA-DM)

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.