GG-P-001428A (DSA-DM)
April 9, 1975
SUPERSEDING
Revision of Int. Fed. Spec.
GG-P-001428 (DSA-DM)
February 7, 1968
See Section 6

INTERIM FEDERAL SPECIFICATION

PREVENTIVE DENTISTRY KIT, PATIENT

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers preventive dentistry kits suitable for patient use in oral hygiene procedures as part of a complete preventive dentistry program.

1.2 Classification. Preventive dentistry kits shall be supplied in the following types as specified (see 6.1):

Type I. Adult

Type II. Child

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

H-S-951	General Specification for Synthetic Filament for Brushes.
L-P-394	Plastic Molding Material, Polypropylene, Injection and Extrusion.
PPP-B-585	Boxes, Wood, Wirebound.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

STANDARDS

Federal

FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).
FED-STD-140	Tablet (For Medicinal Purposes).
FED-STD-141	Paint, Varnish, Lacquer and Related Materials, Methods of Inspection, Sampling and Testing.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies).

SPECIFICATIONS

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

DRAWINGS

Defense Personnel Support Center (DPSC)

24340 Toothbrush, Dental, Patient, Adult.
24341 Toothbrush, Dental, Patient, Child

(Copies of specifications, standards, drawings and publications, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN PHARMACEUTICAL ASSOCIATION

National Formulary.

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pa. 18042).

U.S. DEPARTMENT OF HEALTH, EDUCATION, AND WELFARE
FOOD AND DRUG ADMINISTRATION

Federal Food, Drug, and Cosmetic Act and applicable regulations thereto.

(Application for copies should be addressed to the Division of Public Information, Food and Drug Administration, Washington, D. C. 20201).

THE UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The Pharmacopeia of the United States of America

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pa. 18042).

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

D 1562 Specification for Cellulose Propionate Molding and Extrusion Compounds.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Phila., Pa. 19103).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Materials. Materials shall be of high quality throughout, and suitable in all respects for the purpose intended. Any ingredients entering into the dentifrice and disclosing tablets which are not included in the Pharmacopeia of the United States of America (USP) or National Formulary (NF) shall be of quality suitable for pharmaceutical use.

3.1.1 Toothbrushes.

3.1.1.1 Synthetic filaments. Synthetic filaments, (bristles) shall be fabricated of natural (uncolored) nylon 610 or 612 filaments conforming to class N, type II (Polyamide, level) of H-S-951.

3.1.1.2 Brush block. The brush block shall be molded of one of the following materials at the manufacturer's option:

(a) Polypropylene in conformance with type I of L-P-394, except that the requirement and test for deformation under load shall not apply.
(b) Cellulose acetate propionate in conformance with grade H-3 of ASTM D 1562.

Materials and dyes used shall be nontoxic and suitable in all respects for the purpose intended. Acceptable evidence of non toxicity shall consist of Food and Drug Administration (F.D.A.) approval of use of the plastics or dyes in food contact, drug, or cosmetic applications involving contact with oral mucosa. As an alternate, a dye shall be considered acceptable for use in toothbrushes provided its concentration is less than 0.3%, and the dye has been used for this application for a minimum of 3 years without toxic effects.

3.1.2 Erythrosine disclosing tablets. Erythrosine disclosing tablets shall be in accordance with the applicable requirements of FED-STD-140 for type XIII, class 1 tablets, together with the options, additions, and deletions stated hereinafter. Whenever the requirements of this specification for erythrosine tablets are in conflict with FED-STD-140, this specification shall govern. The following ingredients shall enter into the manufacture of the tablet:

Erythrosine (Food, Drug and Cosmetic, (F.D. & C.), Red #3—— 2.0 ± 0.2 percent and sufficient quantities of the following flavoring, binding, and excipient agents:

Sodium chloride (USP)
Saccharin (USP)
Ethyl vanillin (NF)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

Suitable raspberry flavoring agents
Peppermint oil (USP)
Magnesium stearate
Sorbitol (USP)
Mineral oil (Light) (NF)
Stearic acid (USP)

The erythrosine, used in the manufacture of the tablets, shall meet all applicable requirements of the F.D.A. for the certification of F. D. & C. Red #3. Each lot of the F. D. & C. Red #3 used shall be certified by the F. D. A. The sodium chloride, sorbitol, saccharin, stearic acid, and peppermint oil shall be in accordance with the tests, standards, and requirements of the USP including any supplements or revisions thereto. The ethyl vanillin and mineral oil (light) shall be in accordance with the tests, standards, and requirements of the NF, including any supplements or revisions thereto. Assay of the erythrosine shall be made in accordance with the test method of 4.4.1. The dye (erythrosine) shall be dispersed throughout the tablet. As an alternate to the above listed formulation, the elimination of sodium chloride and mineral oil, and the substitution of spray dried peppermint powder in place of peppermint oil are permissible for dry mix processing.

3.1.3 Dentifrice. The following ingredients shall enter into the manufacture of the dentifrice:

Stannous fluroide ----------0.40 percent
Stannous pyrophosphate----------1.0 percent
Calcium pyrophosphate---------- 39.0 percent

and sufficient quantities of the following:

Suitable flavoring and coloring agents
Carboxymethyl cellulose
Veegum
Humectants (Glycerine, USP and Sorbitol, USP)
Sodium monoglyceride sulfonate
Sodium alkyl sulfate
Distilled water

Assay of the fluorine shall be 0.090 to 0.112 percent, when determined as specified in 4.4.2. Stannous and calcium pyrophosphate content shall be determined by reference to the manufacturer's formulation sheet.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

3.1.4 Floss. Floss shall be waxed, or unwaxed (bonded or natural) filament, white dental floss made of bright, high tenacity continuous multi-filament nylon (synthetic polyamide) of chemical species and physical form suitable for the use intended and having no objectionable odor or taste.

3.2 Description. Type I Kit shall consist of a tube of dentifrice, dental floss, 6 disclosing tablets and 1 adult toothbrush. Type II kit shall consist of a tube of dentifrice, 6 disclosing tablets and 1 child toothbrush. Immediate container shall be a suitable cardboard box, securely holding the components. Each box shall have adequate and accurate instructions on dental health rules printed on the outside of the container, including dental health rules and use of disclosing tablets.

3.2.1 Toothbrushes. Style, design, and dimensions of the adult toothbrush shall be in accordance with Defense Personnel Support Center (DPSC) Drawing 24340. Style, design, and dimensions of the child toothbrush shall be in accordance with DPSC Drawing 24341. Brush block of both size toothbrushes shall consist of a head, neck, and a handle gripping section. Toothbrush (block) shall be of straight line design and shall have at least one flat surface to facilitate through tactile sense, the orienting of the bristles in the desired direction and the maintenance of the proper position. Tufts shall be firmly secured in holes by means of a corrosion-resisting, nickel-silver slug flattened strip of metal. Adult toothbrush shall be furnished in any one of the styles shown in DPSC Drawing 24340. Child toothbrush shall be furnished in any one of the styles shown in DPSC Drawing 24341. Color of toothbrush block shall be red, blue, yellow, ivory, rose, clear (colorless), or green. Any one color or assortment of colors shall be acceptable, provided that each handle is one solid color. Block shall have a polished finish, free from flash, rough mold marks and sharp projections. Filaments shall have a bright, smooth finish.

3.2.1.1 Filament ends per tuft. The number of filament ends per tuft shall be as specified in the applicable drawing (see 3.2.1) when tested as specified in 4.4.5.

3.2.1.2 Tuft angle. Filament ends shall be splayed no more than 15 degrees from the perpendicular to the axis (handle) of the toothbrush when tested as specified in 4.4.6.

3.2.1.3 Filament shaping. Filaments shall be free from sharp points and rough edges and shall be straight, flat, even-trimmed, and end-rounded to approximate hemispheric shape to preclude trauma to the hard and soft tissues of the mouth. No more than 30 percent of the filaments shall be classified as unacceptable when tested as specified in 4.4.7.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

3.2.2 Erythrosine disclosing tablets. The erythrosine disclosing tablets shall be suitably flavored, uncoated red tablets, which dissolve readily in the mouth fluids upon chewing to form a palatable, nontoxic solution of the erythrosine dye. This dye shall be capable of staining food deposits and other areas not cleaned in brushing the teeth. The appearance of the tablets may be mottled or spotted or slightly grainy (striated) in appearance; all tablets shall have a dust-free surface. Tablets shall not liquefy, soften, or disintegrate at temperatures up to 140 degrees Fahrenheit (°F.). Weight of 20 tablets shall be 7.80 ± 0.78 grams (g).

3.2.2.1 Immediate container. Six of the erythrosine tablets shall be packaged in a hermetically sealed, 0.0007 inch (in.) thick strip of either cellophane or laminate material containing aluminum foil or plastic coated cellophane. Each tablet shall be hermetically heat-sealed within its own enclosed pocket or cell. The tablets may be furnished in individual or multiple tablet strips, or a combination thereof. If multiple tablet strips are used, each such pocket shall be separated from the adjacent pocket by perforations that enable one pocket to be removed easily from the strip without disturbing the heat seal of the adjoining pocket.

3.2.3 Dentifrice. Dentifrice tube shall contain 1-1/2 ounces (oz.) of the dentifrice listed in 3.1.3. The side wall of the tube shall be a paper-aluminum foil-polyolefin laminate structure which shall be side seamed and sealed (to prevent leakage) to form a tube. The high density polyethylene head and neck shall be injection molded on the sidewall sleeve and shall hold a urea disk. The disk shall provide rigidity and favorable barrier properties. Polypropylene screwcap shall be properly threaded to insure adequate closure of the dentifrice tube. Dentifrice shall be free from foreign matter and shall have a pleasant taste and odor.

3.2.3.1 pH of dentifrice. The pH of the dentifrice shall be 4.6 to 5.1, when tested as specified in 4.4.3.

3.2.3.2 Consistency of dentifrice. Consistency of the dentifrice shall be 18 ± 6 Brookfield units, when tested as specified in 4.4.4.

3.2.4 Floss. (Type I, Adult kit only). A minimum of 10 yards of dental floss specified in 3.1.4 shall be furnished in a dispenser in each adult kit. Dispenser shall be made of suitable metal or plastic or a combination of the two. Floss shall be firmly and evenly wound and shall dispense properly. Floss shall be free from tangles, snarls, knots, or other imperfections which would affect its use or ease of unwinding. Floss shall be clean (free from foreign matter).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

3.3 Marking. Carton shall be marked with the contents, dental health rules, and directions for use of the disclosing tablets to check brushing technique. Tootbrushes shall be marked with the name or trademark of the contractor or manufacturer and the name of the country or origin. The use of an identification code for marking is permissible provided approval is obtained from the contracting officer prior to award. The exterior of the cellophane or laminate material containing the erythrosine tablets shall be marked with the contents and lot or batch number. Marking of the exterior of the dentifrice tube shall include the brand identification, net weight of contents, and name and address of manufacturer. Each dentifrice tube shall be marked with the lot or batch number, or suitably code dated to relate to the lot or batch number.

3.4 Workmanship. Workmanship shall be first class throughout. Kits shall be free from defects which may detract from their appearance or impair their serviceability. Kits and all components therein shall be furnished clean and ready for use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of compliance. Certificates of compliance, supplied by the manufacturer of the toothbrushes and floss, may be furnished in lieu of actual performance of such testing by the contractor. When certificates of compliance are submitted, the Government reserves the right to check test such items to determine the validity of the certification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

4.1.4 Inspection of materials and components. In accordance with 4.1, the supplier is responsible for insuring that materials and components used were manufactured, tested, and inspected in accordance with the requirements of referenced subsidiary specifications to the extent specified, or if none, in accordance with this specification. In the event of conflict, this specification shall govern.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables I, III, and IV (see 4.2.1, 4.3.1 and 4.3.2) and table II (see 4.2.2).

4.2.1 Sampling for visual examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in table I. Unit of product for examination purposes shall be one kit.

Table I. Inspection and acceptable quality levels (AQL's)

Type defect	Inspection level	AQL (Percent defective)
Major	S-2	2.5
Minor	S-2	6.5

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II, except that the acceptance number shall be zero for all sample sizes. Unit of product for test purposes shall be one kit.

Table II. Tests

Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Dentifrice				
Fluoride Assay	3.1.3. 1/	4.4.2	2/	3/
pH	3.2.3.1 1/	4.4.3	2/	3/
Consistency	3.2.3.2 1/	4.4.4	2/	3/
Disclosing tables				
Erythrosine Assay	3.1.2	4.4.1	2/	3/
Toothbrush				
Microscopic testing	3.2.1.3	4.4.7	S-2	6.5
Filament Count per tuft	3.2.1.1	4.4.5	S-2	4/
Tuft angle	3.2.1.2	4.4.6	S-2	2.5
All Components in kit, Dimensional and weight testing	3.2.1, 3.2.1.1, 3.2.2, 3.2.3 and 3.2.4	4.4.8	S-2	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

. components.		
hed	X	
e container.	X	
ther than		X
nted on		X
ner not		X
ly crimped	X	
stripped	X	
	X	
	X	
aste or		X

1/ Analysis performed at
2/ One determination sh
3/ Noncompliance will ca
4/ AQL is not applicable
tested (see 4.4.5)

4.3 Examination. Vis
performed as shown below.
it shall be considered de
exceeds the acceptance nu
be considered as having f

4.3.1 Visual examinat
but not limited to, those

Table III.

Examine	
Assembled Kit	Any of in kit Immedia causin damage Immedia but no Wrong s for ap Presenc Presenc dirt i Instruc immedi Printin legibl
Dentifrice	Dentifr at sea Tube no thread Cap loo Foreign Dentifr odor.

; results will change with aging.
r batch number.
based on average of samples

for delivery examination shall be
ls any examination requirement,
of defective samples examined
L-STD-105, the entire lot shall
quirements of the specification.

examined for defects including,

fects for Visual Defects

	Classification	
	Major	Minor
ıot included	X	
damaged	X	
its to be		

of
ained
ne
th
ifrice
ame
e
number.

hall
ir

con-
f
-

c-
es
n
r-

the
Gov-

ed
use
by

ed by
f
f

Source: https://assist.dla.mil -- Downloaded: 2026-02-26T11:54Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects for Visual Defects (cont'd)

Examine	Defect	Classification	
		Major	Minor
Disclosing tablets	Two to six tablets damaged to the extent to prevent normal usage.	X	
	One tablet damaged to the extent to prevent normal usage.		X
	Disclosing tablets not of pleasant odor or taste.		X
	Die not fully dispersed in tablets.		X
	Less than six tablets furnished.		X
	Tear off strip for disclosing tablets (when provided) does not dispense one tablet at a time.		X
	Marking of disclosing packets not as specified.		X
	Packets not properly sealed, closure inadequate.		X
Toothbrush	Toothbrush not in accordance with one of styles specified.	X	
	Tufts not firmly anchored; can be easily removed.	X	
	Filaments crimped.	X	
	Filaments embedded with dirt.	X	
	Brush head not smooth; edges and corners sharp; flash present.	X	
	Tootbrush not wrapped in cellophane.	X	
	Identification marking missing.		X
	Brush handle not smooth; edges, and corners sharp; flash present.		X
Floss 1/	Floss not evenly or not firmly wound; cannot be dispensed properly from container.	X	
	Cutting device missing on dispenser.	X	
	Floss not clean; contains foreign matter.	X	
	Floss tangled, knotted, or snarled.		X

1/ Listed defects applicable to Type I kit only.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:54Z
Check the source to verify that this is the current version before use.

4.3.2 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

Table IV. Examination for Preparation for Delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging, packing materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

4.4 Tests.

4.4.1 Erythrosine content of disclosing tablet.

4.4.1.1 Apparatus. The following apparatus shall be utilized to determine the erythrosine content of the disclosing tablets:

(a) Spectrophotometer for use at 510 to 540 millimicrons, providing a light path of 1 centimeter (cm) or longer

or

Filter photometer providing a light path of 1 cm or longer equipped with a green filter having maximum transmittance at 510 to 540 millimicrons.

(b) Volumetric flasks of 100-milliliter (ml) and 50-ml capacity.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

4.4.1.2 Reagent. Methanol (Reagent Grade) shall be used for dilution of samples and as the reference solvent in the spectrophotometer or filter photometer.

4.4.1.3 Preparation of standard solution. Sufficient quantity of P. D. & C. Red #3 dye equivalent to 50 milligrams (mg) of 100 percent pure dye shall be weighed and transferred to a dry 100 ml volumetric flask. The correct weight of dye may be calculated as follows:

$$\frac{50 \text{ mg}}{\text{percent pure dye}} = \text{mg of dye to weigh for standard solution.}$$

Fifty milliliters of methanol shall be added to the dye and the flask shall be shaken well until all the dye is dissolved, the sample further diluted to the 100-milliliter mark on the flask, and mixed well. The following dilution shall be made from the above solution:

10 ml to 100 ml, equal to 50 micrograms (mcg) of pure dye/ml
(Label this: Standard Solution No. 1)

Make the following dilutions from Standard Solution No. 1:

10 ml to 100 ml, equal to 5 mcg of pure dye/ml
(Label this: Standard Solution No. 2)

4 ml to 50 ml, equal to 4 mcg of pure dye/ml

8 ml to 50 ml, equal to 8 mcg of pure dye/ml

Make the following dilutions from Standard Solution No. 2:

10 ml to 50 ml, equal to 1 mcg of pure dye/ml

20 ml to 50 ml, equal to 2 mcg of pure dye/ml

The optical density of each of the above standards shall be read in a 1 cm cell against methanol as a reference, using monochromatic light of 530-millimicron wavelength. Readings shall be made shortly after the standard solutions have been prepared since dye color is not stable. Readings shall be plotted on linear graph paper as optical density or absorbance (ordinate) verus concentration in mcg/ml (abscissa). The best straight line to fit the series of these points shall be drawn, and the slope of this line shall be calculated by dividing the absorbance of any point on this line by the concentration at this point. The resulting slope is defined as the absorptivity of the dye in units of milliliters per microgram.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

4.4.1.4 Preparation of sample. Twenty erythrosine tablets shall be finely powdered with a clean, dry mortar and pestel. One hundred milligrams of the combined powdered tablets shall be weighed accurately and transferred quantitatively to a dry 100-ml volumetric flask. Fifty milliliters of methanol shall be added, and the flask shall be stoppered and shaken for 5 minutes. The sample shall be further diluted to the 100-milliliter mark on the flask with methanol and mixed well. Insoluble particles shall then be allowed to settle in the flask. Twenty milliliters of the above solution shall be transferred carefully by means of a pipet to another dry 100-milliliter volumetric flask, diluted further with methanol to the 100-milliliter mark and mixed. The absorbance of this solution shall be measured in a 1-centimeter cell using monochromatic light of 530-millimicron wavelength, and using methanol as the reference solvent. The absorbance of the diluted sample should be recorded within 2 hours, since the optical density of the dye decreases with time. The percent pure dye in the tablets shall be calculated as follows:

$$\frac{\text{Absorbance of sample}}{\text{Absorptivity of pure dye}} \quad \frac{(\text{ml})}{(\text{mcg})} \times \frac{100\ \text{ml}}{20\ \text{ml}} \times \frac{100\ \text{ml}}{100\ \text{mg}} \times \frac{1}{10} =$$

$$\frac{\text{Absorbance of sample}}{\text{Absorptivity of pure dye}} \quad \frac{(\text{ml})}{(\text{mcg})} \times 2 = \text{percent pure dye in tablets}$$

4.4.2 Fluorine content in dentifrice. Total fluorine content of the dentifrice shall be determined by direct potentiometric measurement using a fluoride specific ion electrode.

4.4.3 pH. pH of the dentifrice shall be determined on an accurate and precise pH meter. A 3 to 1 water to dentifrice slurry shall be used.

4.4.4 Consistency. Consistency of the dentifrice shall be measured using the "E" spindle on a Brookfield viscosimeter. Consistency shall be determined in accordance with Method 4287 of FED-STD-141, at 85 °F ± 1°F and at 2 revolutions per minute (r.p.m.).

4.4.5 Filament count per tuft. Filament ends shall be counted in fifteen representative tufts. The average value for the fifteen counts shall be considered the result.

4.4.6 Tuft angle. The toothbrush shall be placed on a level surface with the head resting on the surface. By means of a bevel protractor, determine the angularity of the tufts at the end and side rows.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

4.4.7 Microscopic testing of filaments. Microscopic testing of the toothbrush filaments shall be conducted on any combination of two of the tufts in the middle rows excluding the end tufts. Filaments shall be "ideal" or "acceptable" as shown in figure 1, when tested with a binocular microscope with a 10 power (10X) lens and a setting of 1.5 (15X magnification). The number of defective ("unacceptable" as shown in figure 1) filaments shall be noted. The sum of the defective filaments in the two tufts shall be divided by the total number of filaments in two tufts and the percentage of defective filaments calculated by multiplying by 100. If the percentage is over 30 percent, the brush shall be classified defective.

4.4.8 Dimensional and weight testing. Standard measuring instruments shall be used to determine the following dimensions and weight:

Dimensions

a. Dimensions of toothbrush.

b. Number and arrangement of tufts in toothbrush.

c. Length of floss present in dispenser (for Adult kit only).

Weight

a. Weight of erythrosine disclosing tablets.

b. Weight of dentifrice in tube.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.1).

5.1.1 Unit of issue. One package, containing thirty six (36) kits as specified constitutes one unit of issue.

5.1.1.1 Level A.


5.1.1.1.1 Unit package. One unit of issue shall be packaged in a box of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening.

5.1.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.1).

5.2.1 Level A. Four (4) units of issue shall be packed in an exterior container designed for a type 2 load and constructed in accordance with

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:54Z
Check the source to verify that this is the current version before use.

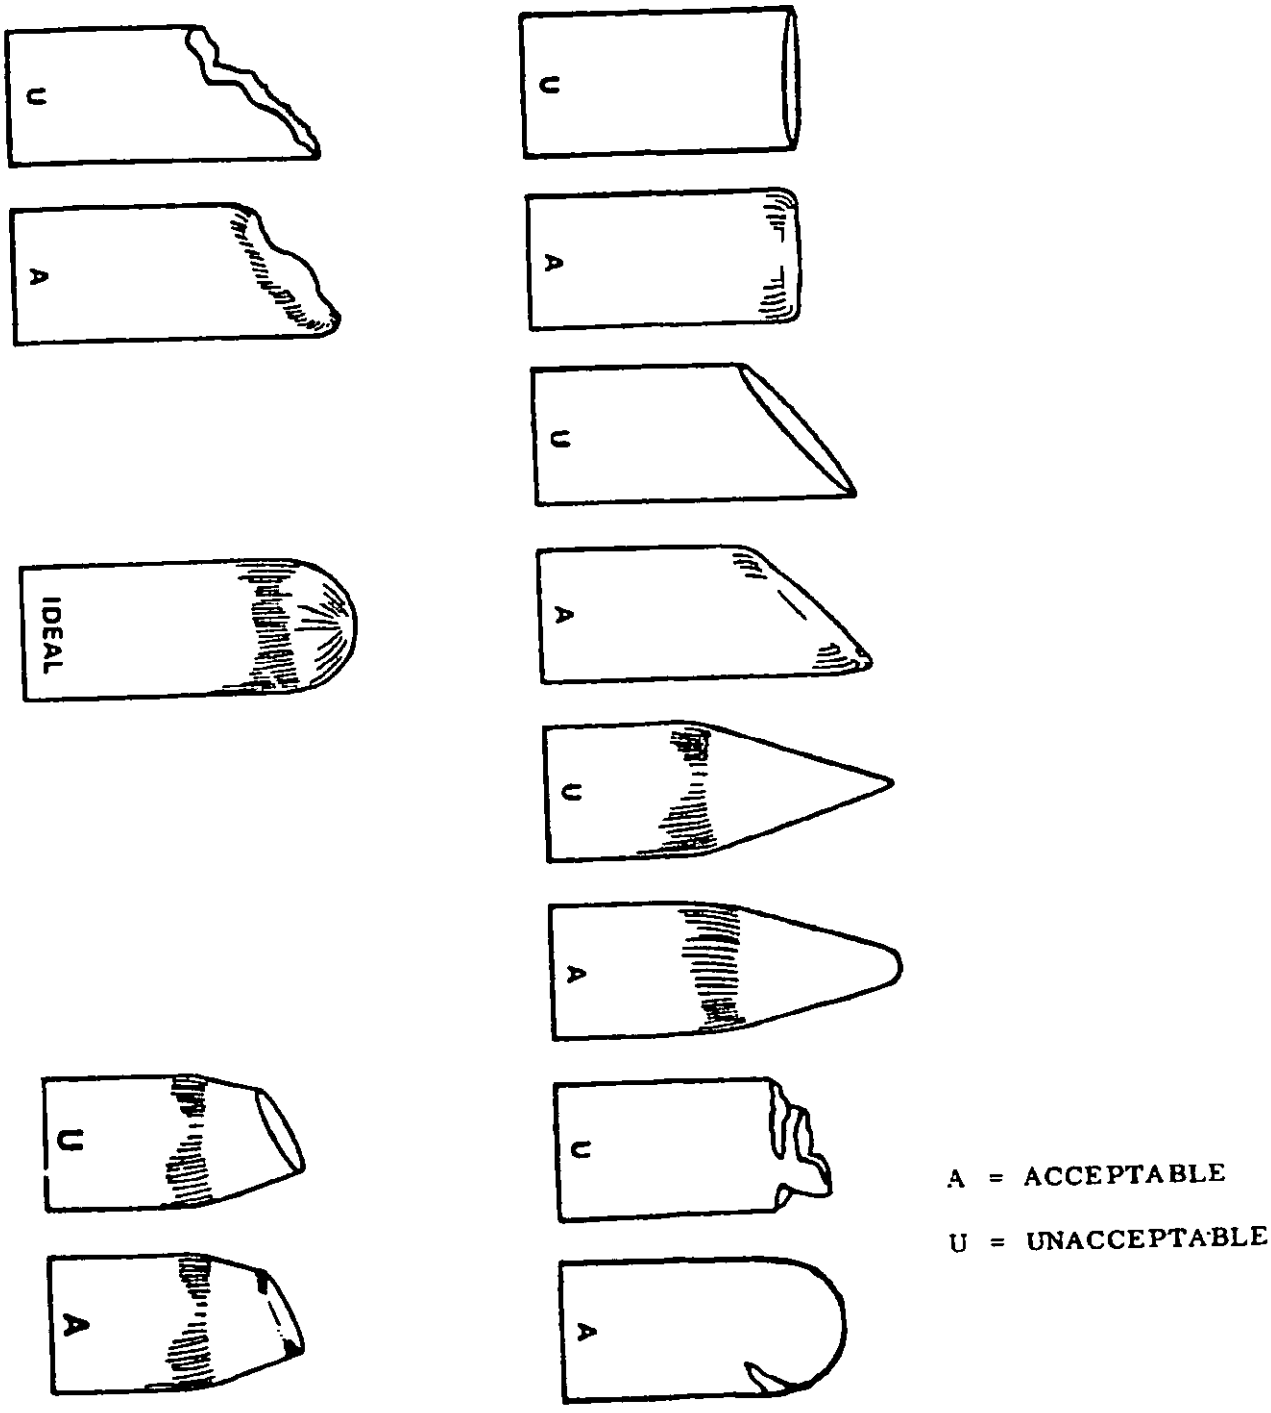

A = ACCEPTABLE

U = UNACCEPTABLE

FIGURE 1. TOOTHBRUSH BRISTLE ACCEPTABILITY

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:54Z
Check the source to verify that this is the current version before use.

PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof as specified in the appendix of PPP-B-636.

5.2.2 Level B. No further packing is required. Unit package as specified in 5.1.1.1.1 shall be shipped as the exterior container.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, constructed so as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipments shall be in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number, lot (control) number and name of contractor shall be shown. Date of manufacture shall be shown in lieu of date packed. Marking shall include the legend:

"STORE AT CONTROLLED ROOM TEMPERATURE (59° - 86°F)".

Note: When level B packing is specified, the unit package shall be marked as required for the exterior container in accordance with MIL-STD-129. Unit package shall be marked "B" in lieu of "A/B".

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Date of manufacture shall be shown in lieu of date packed. Marking shall include the lot (control) number and the legend:

"STORE AT CONTROLLED ROOM TEMPERATURE (59° - 86°F)".

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:54Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Type required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Supersession data. Type I, adult preventive dentistry kit corresponds to the preventive dentistry kit specified in MIL-P-36529; however, some characteristics have been changed.

6.3 National Stock Number (NSN) coverage. This specification covers the following items appearing in the Federal Supply Catalog:

NSN	Item Identification
6520-00-086-6554	PREVENTIVE DENTISTRY KIT, PATIENT, Child, 36s
6520-00-890-2080	PREVENTIVE DENTISTRY KIT, PATIENT, Adult, 36s.

6.4 Specification changes. Because of the extensiveness of changes to this document, the margins have not been marked with an asterisk to indicate where changes from the previous issue have been made.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1390
is

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:54Z
Check the source to verify that this is the currentversion before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
CG-P-001428A (DSA-DM) PREVENTIVE DENTISTRY KIT, PATIENT

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO (If "Yes", in what way?)

4. REMARKS

SUBMITTED BY (Printed or typed name and address - Optional)

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

© GPO 1974—603-680/6136 2-1

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:54Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
D-D - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:54Z
Check the source to verify that this is the current version before use.