GG-R-001171(DSA-DM)
21 April 1966
INTERIM REVISION OF
Fed. Spec. GG-R-50,
25 August 1960 and
Fed. Spec. GG-R-35
10 March 1953

# INTERIM FEDERAL SPECIFICATION

## RACKS, DRYING, HOSPITAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-R-50, dated 25 August 1960.

### 1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers two types of corrosion-resisting steel drying racks suitable for use in military medical services.

1.2 Classification. Racks covered by this specification shall be of the following types:

| | |
|---|---|
| Type I | RACK, DRYING, GLOVE, Corrosion-resisting Steel. |
| Type II | RACK, GAUZE PAD, Corrosion-resisting Steel. |

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

2. APPLICABLE SPECIFICATIONS, STANDARDS AND OTHER PUBLICATIONS.

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

FF-C-82 Casters, Swivel, Chair.
PPP-B-640 Box, Fiberboard, Corrugated, Triple Wall.

STANDARDS

Federal

FED-STD-66 Steel Chemical Composition and Hardenability.
Fed. Test Method Std. No. 151 Metals; Test Methods.

Military

MIL-STD-105 Sampling Procedure and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

National Fire Protection Association (NFPA):

NFPA No. 56 Code For The Use Of Flammable Anesthetics 1965.

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch Street, Boston, Mass. 02110).

3. REQUIREMENTS

3.1 Preproduction sample. Unless otherwise specified (see 6.1), prior to the start of production of the contract quantity, one preproduction sample of the drying rack shall be assembled, completely finished, and tested by the contractor. The sample shall be submitted, together with the contractor's inspection and test reports, to the contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the contracting officer, or his authorized representative, prior to the manufacture and assembly of the remaining quantity to be manufactured. Further production of the item by the contractor, prior to this approval, shall be at the contractor's risk. Accepted preproduction sample shall become the property of the procuring activity and shall be included in the quantity called for in the contract or order. In the event that the preproduction sample is not approved, the contractor shall submit a new sample for approval, or modify the existent sample so as to remove the deficiencies cited.

3.2 Material.

3.2.1 Steel. Steel shall be corrosion-resisting, conforming to class 302 or 304 of FED-STD-66 and shall meet the chemical requirements specified therein, when tested as specified in 4.4.1. Commercial tolerances on gage size and diameters shall apply.

3.2.2 Casters. Casters shall be in accordance with FF-C-82 for type I, size B, except that casters shall have rubber wheels with metal stems. Rubber wheels shall be fabricated of electrically conductive rubber. Conductivity shall be such that the resistance between a metallic object placed on any part of the rack and a metallic plate placed under any one supporting member, but insulated from the floor, shall be not more than 250,000 ohms.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

3.3 Construction. All tubing used in the fabrication of the drying racks shall be 1 inch diameter steel tubing having 0.065 inch (No. 16, Birmingham Wire gage) thick walls. The drip pans shall be fabricated from 0.050 inch (No. 18, United States Standard gage) thick corrosion-resisting steel. Drain holes shall be provided in the bottom of the tubular cross members to provide escape for water entering around the pins. The pins shall be rounded at both ends to prevent damage to the item supported by the pin and to provide a rounded surface for welding to the bottom of the cross member. The inverted C-braces at the base of the rack shall be heavily weighted and fitted with casters as specified in 3.2.2.

3.3.1 Type I construction. The type I drying rack shall be constructed in accordance with figure 1. The drip pan shall be fully hemmed at the top edge, welded at all corners, and welded to the tubular upright. The bottom of the drip pan shall be pitched down to the front center so that the drainage shall flow to this point. A chromium plated brass drain cock shall be provided at the front center of the drip pan for removing the drainage.

3.3.2 Type II construction. The type II drying rack shall be constructed in accordance with figure 2. The drip pan shall be removable for emptying. The drip pan, when centered in the angle frame holder, shall have a maximum of 1/2 inch clearance between the tubular uprights and the ends of the pan.

3.3.3 Welding. All welds, except pins, shall be fillet welds finished to give the appearance of a continuous piece. Welds shall be sound, well-fused, and free from blisters or blowholes, developing strength equal to the part welded. Welding rod shall be of similar chemical composition to part welded. All welds shall be cleaned and free from twists or strains. Exposed welds shall be ground smooth to eliminate pit marks and seams, and shall be polished to blend with the finish of the adjacent surfaces.

3.4 Finish. All parts shall be finished in a No. 4 commercial finish.

3.5 Identification marking. Each rack shall be permanently and legibly marked with the following information:

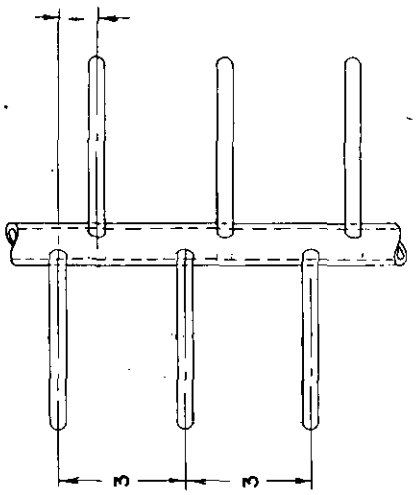
Manufacturer's name or registered trademark.
Contract or purchase order number.
Federal stock number.
The letters U.S.

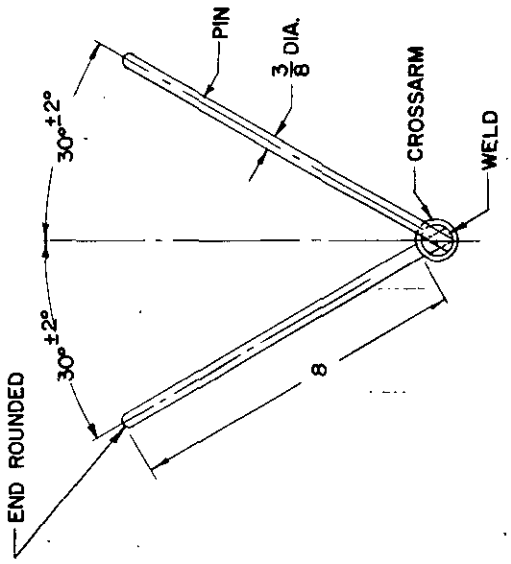
Markings secured by adhesives shall not be used.

3.6 Workmanship. Shall be first class throughout. The finished units shall be clean, well-made, and free from defects which detract from its appearance or may impair its serviceability.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.



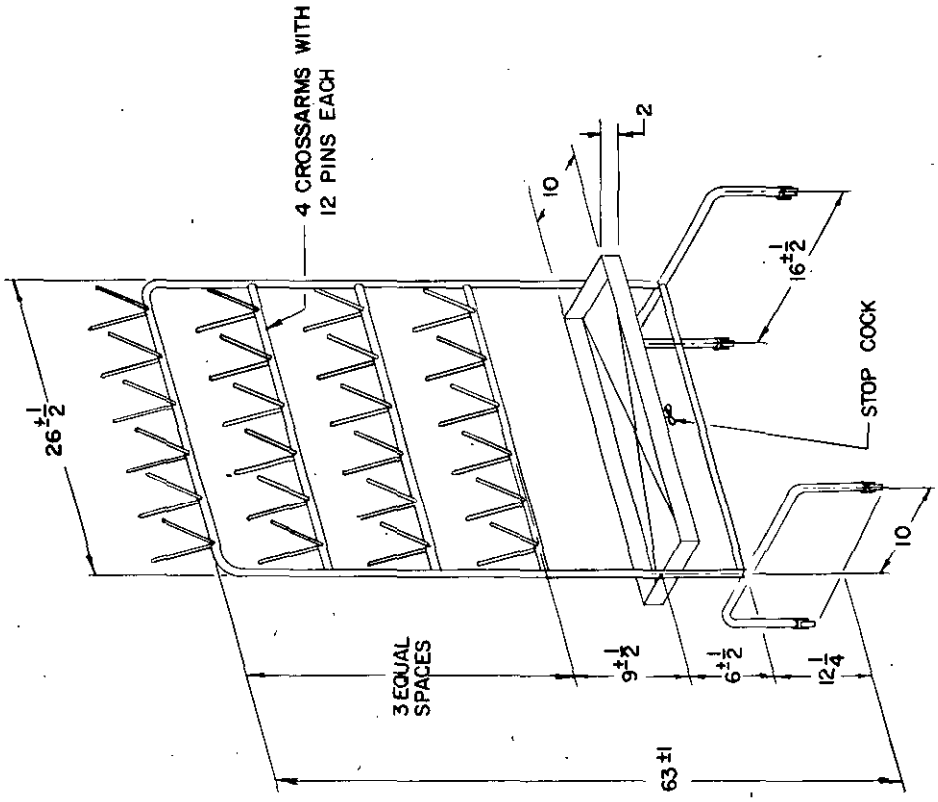



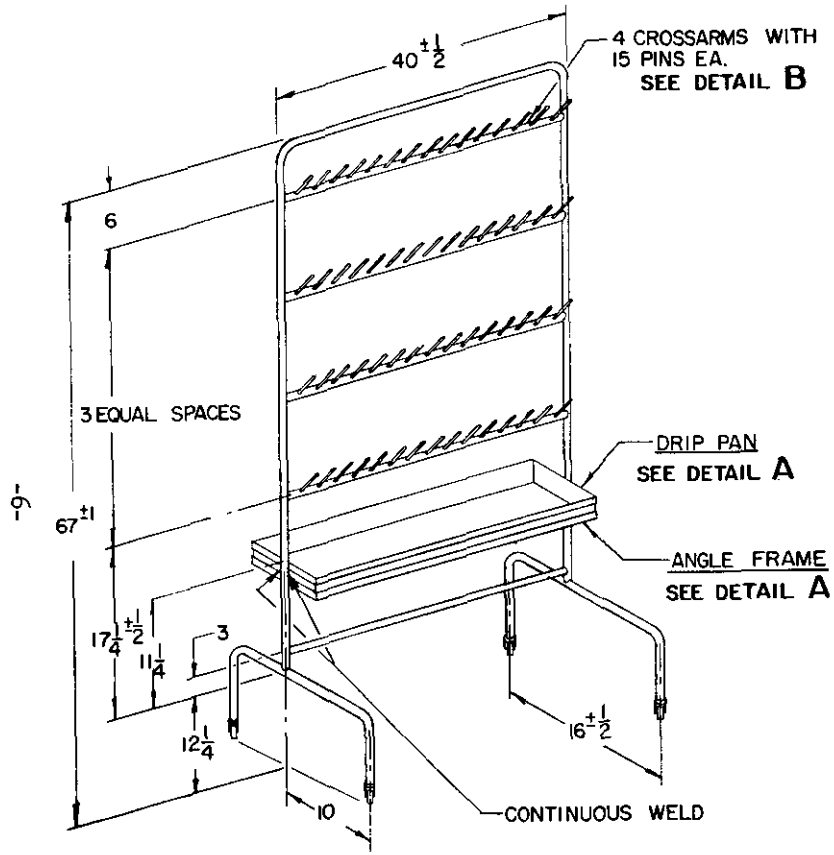

FIGURE 1

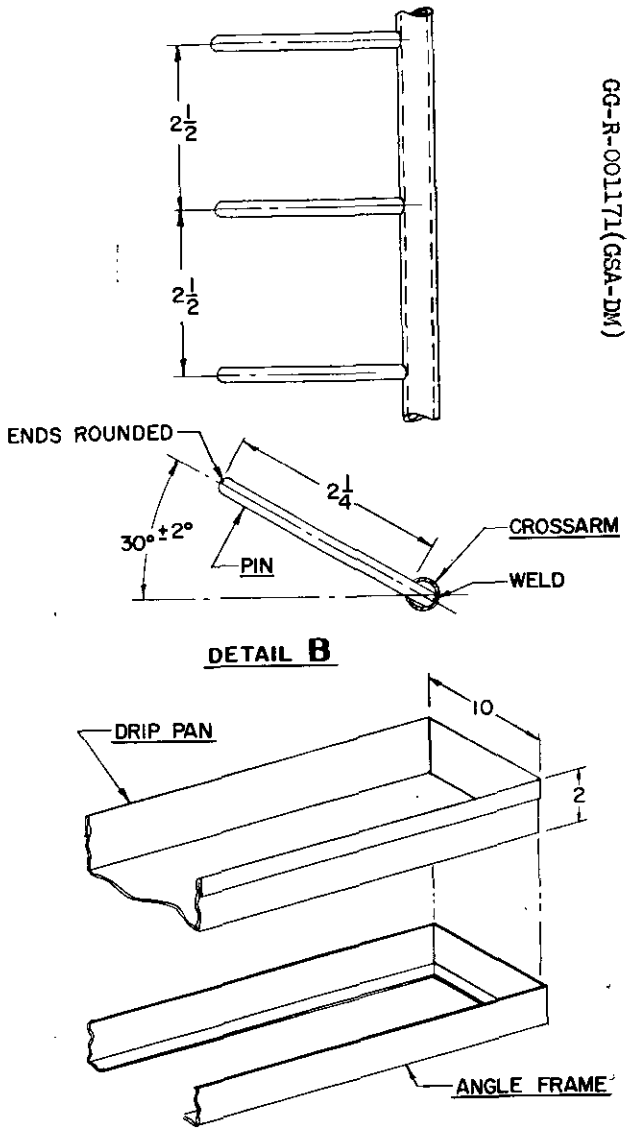
RACK, GLOVE, DRYING

UNLESS OTHERWISE SPECIFIED
TOLERANCES ON FRACTIONS ±1/8



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.




UNLESS OTHERWISE SPECIFIED
TOLERANCES ON FRACTIONS ± 1/8

FIGURE 2
RACK, GAUGE PAD



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

## 4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

| | Inspection level | AQL (defects per 100 units) |
|---|---|---|
| For visual examination | | |
| Major defects | II | 1.0 |
| Total (major and minor combined) defects | II | 4.0 |
| For dimensional examination | S-3 | 2.5 |

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105.

4.2.3 Raw materials. Four ounces of each lot of metal used in the construction of the drying racks shall be selected for chemical analysis.

4.3 Examination. The racks shall be examined to determine compliance with all requirements contained in this specification.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects *

Major

| | |
|---|---|
| 101 | Rack not free of cracks, tears, ruptures, or deformed surfaces. |
| 102 | Component parts improperly aligned or fitted. |
| 103 | Exposed edges, corners, or surfaces not free of burs or sharpness. |
| 104 | Seam and fillet welds not sound, continuous, or ground smooth to blend with adjacent surfaces. |
| 105 | Seam and fillet welds not free of blowholes, flux, splatter, or discoloration. |
| 106 | Braces not weighted. |
| 107 | Any component part missing, damaged or otherwise unusable. |

Minor

| | |
|---|---|
| 201 | Unexposed welds not cleaned or free of slag and spatter. |
| 202 | Fillet welds undercut. |
| 203 | Finish not uniform |
| 204 | Finish not free of coarse grind marks or scratched areas. |
| 205 | Pin ends not rounded. |
| 206 | Pins not uniformly aligned. |
| 207 | Identification marking not complete, legible, correct, or permanent. |

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The racks shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with requirements contained in this specification.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard 151.

4.4.2 Conductivity. Test for electrical conductivity shall be in accordance with Article 253 of the National Fire Protection Association's publication No. 56.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One rack, as specified, constitutes one unit of issue.

5.1.2 Level A. Casters shall be removed, packaged in a cloth bag or other suitable container and secured to the rack. Pan, if removable, shall be secured into position. All exterior finished surfaces shall be protected by wrapping, and wrapping secured by typing with cord or sealing with tape.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A. Each unit shall be overpacked in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-640, class 2, Grade A, style E. Container shall be designed with interior fittings to insure against shifting of or damage to the item. Adequate cushioning shall be utilized to insure against marring of surfaces. Fittings shall also be adequate to distribute weight of the item over entire base of container. Closure and sealing of container shall be as specified in the appendix, except that the use of steel strapping is not authorized.

5.2.2 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).
(c) Where preproduction sample shall be sent.
(d) When preproduction sample is not required.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types, which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

# SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. *Fold on lines on reverse side, staple in corner, and send to preparing activity.* Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426

REPLACES EDITION OF 1 OCT 64 WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

FOLD

DEFENSE SUPPLY AGENCY
DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20th ST.
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER

ATTN: DIRECTORATE MEDICAL MATERIEL

2800 SOUTH 20TH STREET

PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.