GG-S-001015a(DSA-DM)
September 25, 1969
Revision of Interim
Federal Specification
GG-S-001015 (DSA-DM)
June 15, 1965

INTERIM FEDERAL SPECIFICATION
SYRINGE, FOUNTAIN

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-S-1015.

1. SCOPE

1.1 This specification covers one type of completely assembled enema fountain syringe

2. APPLICABLE DOCUMENTS

2.1 Specifications, standards and drawings. The following specifications, standards and drawing of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive Water Resistant (For Sealing Waterproofed Paper)
PPP-B-566	Boxes, Folding Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.
PPP-T-76	Tape Pressure Sensitive Adhesive Paper, Water Resistant (For Carton Sealing)

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:53Z
Check the source to verify that this is the current version before use.

Military

MIL-L-1054 Liners Case and Sheet Overwrap; Water-Vaporproof, or Waterproof, Flexible

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index The Index which includes cumulative monthly supplements as issued is for sale on a subscription basis by the Superintendent of Documents U. S. Government Printing Office, Washington, D C., 20402.)

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo , Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D C)

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies)

(Copies of Military specifications standards and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer)

2 2 Other publications. The following documents form a part of this specification to the extent specified herein Unless otherwise indicated the issue in effect on date of invitation for bids or request for proposal shall apply.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the currentversion before use.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

822 Test for Tensile Properties of Thin Plastic Sheeting

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa 19103.)

U.S. PHARMACOPEIAL CONVENTION, INC. (U.S.P.)

Pharmacopeia of the United States

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pa)

3. REQUIREMENTS

3.1 Materials.

3 1.1 Plastic. The plastic sheeting and tubing shall be medical grade polyvinylchloride The plastic shall be transparent flexible and nonfrangible. The sheeting and tubing shall contain not more than 5 parts per million of lead when tested as specified In addition, the plastic shall pass the toxicity test specified The plastic sheeting shall have a minimum tensile strength of 300 p.s.i and a minimum elongation of 200 percent

3.1 2 Lubricant. The lubricant employed for the rectal tip section shall conform to the requirements of the current edition of the Pharmacopeia of the U.S.P. for white petrolatum

3 2 Construction. The enema fountain syringe shall be as shown in Figure 1 and as hereinafter specified. The fountain syringe shall be comprised of a plastic bag, plastic tubing, and a shut-off clamp Comprehensive instructions for filling and use shall accompany each unit

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

3 2 1 Plastic bag The plastic shall be heat-sealed to for a leakproof plastic bag and shall include a filling spout and outlet The bag shall have a minimum capacity of 1800 milliliters (1.). The plastic material shall be 0.009 ± 0.003 inches thick. One side of the bag shall have graduation markings at not less than 3 points 500, 1000, and 1500 ml. Markings shall be accurate to ± 25 ml. The opening at the top shall have a suitable leakproof mechanical or self sealing type closure The top outer edge of the bag (outside of the sealed edge and immediately adjacent to the filling opening) shall be provided with a reinforced opening to permit suspension of the filled bag from an intravenous stand or other support.

3 2 2 Plastic tubing The tubing shall have a minimum inside diameter of 0 2 inch, a minimum wall thickness of 0.030 inch, a maximum outside diameter of 0.324 inch and shall be 60 ± .1 inches long The tubing shall be permanently attached at one end to the bottom opening of the bag and there shall be no constriction of the opening as the result of the attachment of the tubing The other end of the tubing shall have as an integral part a smooth, rounded tip Not less than one opening 3/16 inch ± 1/32 inch in diameter shall be located 3/4 inch ± 1/8 inch from the end of the tip A plastic vial containing the petrolatum lubricant shall be securely fastened to the end of the tubing by a white plastic cap. The cap shall be movable on the tubing, enabling the person administering the enema to set the cap for the desired depth of insertion. The side of the carton enclosing the individual syringe shall be marked in one inch increments from one to six inches as a guide for measuring depth of penetration The plastic vial shall be so designed to serve as a guide in measuring depth of penetration. When the vial is removed by rotation or the tip of the tube the tip shall be adequately lubricated.

3 2 3 Shut-off clamp. The syringe shall be provided with a positive acting shut-off clamp, attached to the tubing, which by compression of the tubing shall be capable of accomplishing complete shut-off. The bags shall show no leakage nor danger rupture when tested as specified in 4.4.4 and 4 4.5. The shut-off clamp shall be of suitable corrosion-resistant material

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T11:53Z
Check the source to verify that this is the current version before use.

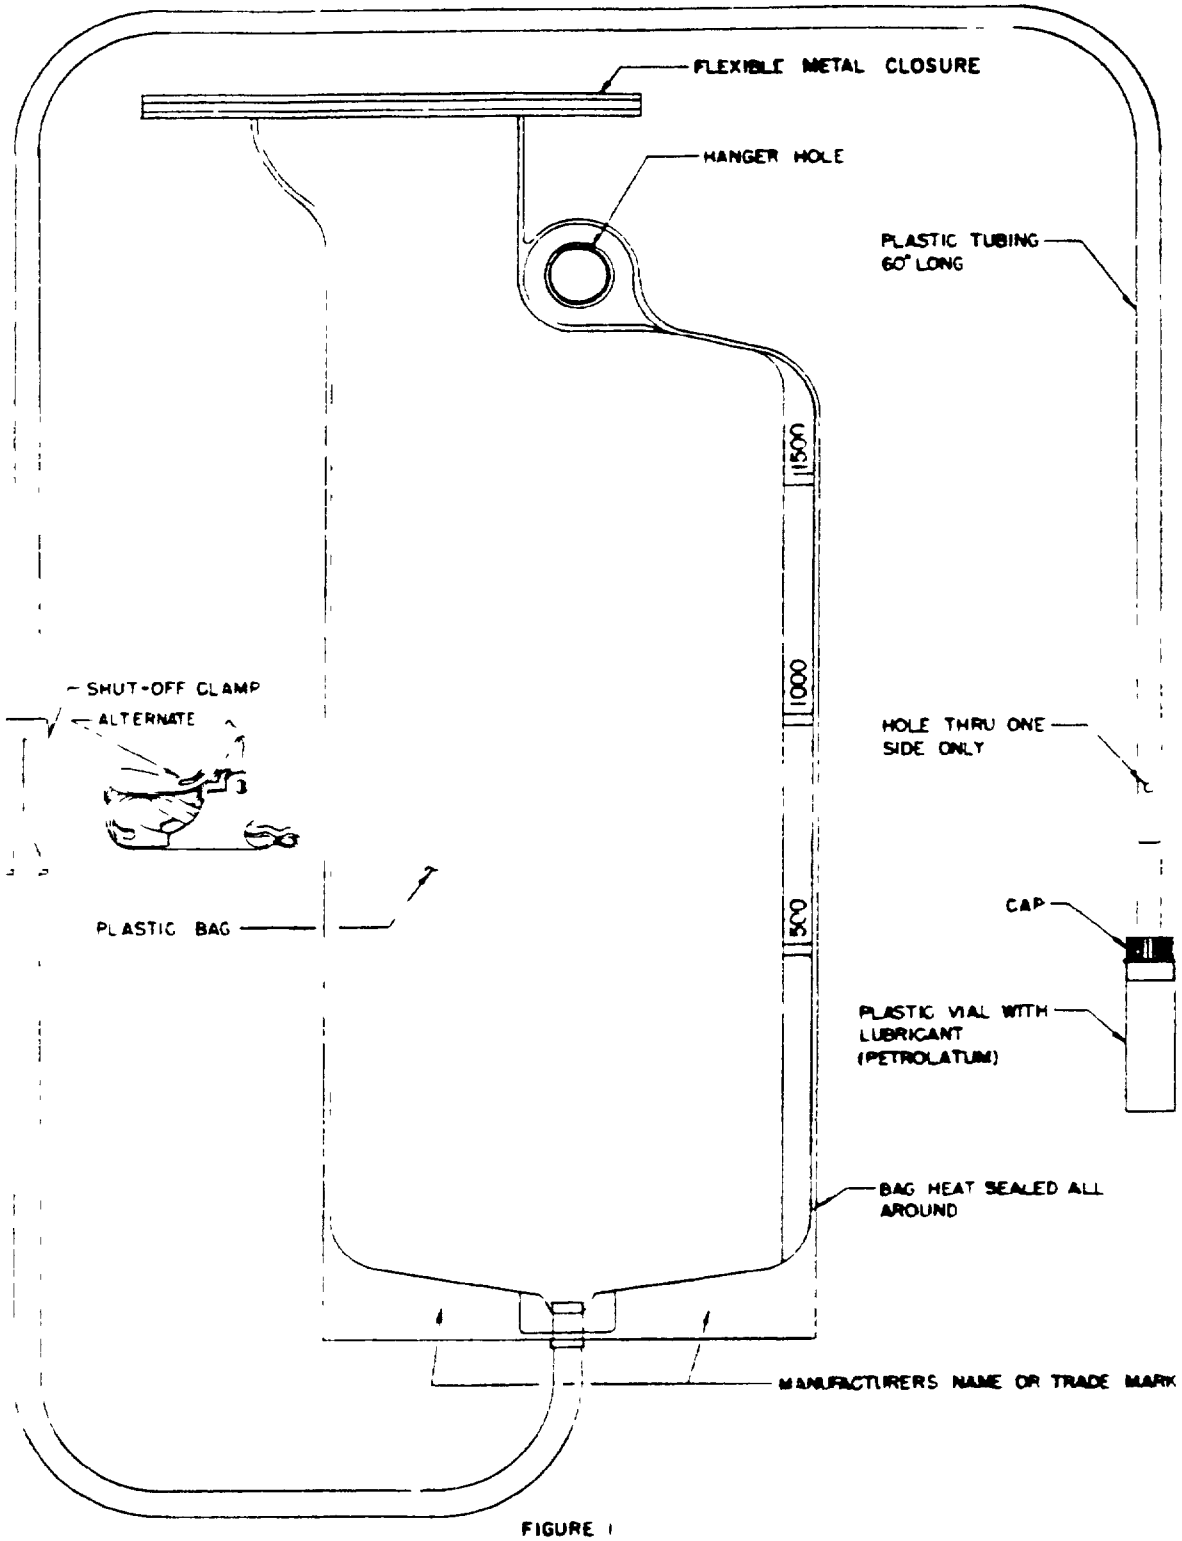


FIGURE 1
DISPOSABLE ENEMA FOUNTAIN SYRINGE

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:53Z
Check the source to verify that this is the currentversion before use.

3.3 Identification marking. The manufacturer's name or registered trademark shall be legibly impressed on the bag as shown on the figure. Identification secured by adhesive shall not be accepted

3 4 Workmanship. Workmanship shall be first class throughout The syringes shall be free from defects which detract from their appearance or may impair their serviceability.

4 QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements

4.1.1 Inspection Inspection as used in this specification, is defined as both examination (such as visual, or auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality When available, certificates of quality supplied by the manufacturer of the component or material listing the specified test method and test results obtained may be furnished in lieu of actual performance of such testing by the contractor.

4 2 Sampling.

4.2 1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and Table I.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the currentversion before use.

Table I

Type defects	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total defects (Major and minor combined)	II	4.0
For dimensional examination	S-1	2 5

* 4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table II.

Table II.

Characteristics	Requirement	Test procedure	Inspection level	AQL
Tensile and Elongation test	3.1.1	4.4.6	**	*
Clamp test	3 2 3	4 4 4	S-2	*
Drop test	3 2 3	4 4.5	S-2	*
Lead test	3 1.1	4 4 2	S-1	*
Toxicity	3.1.1	4 4 3	S-1	*

* The acceptance number shall be zero and not less than three samples shall be taken regardless of lot size
** Each lot or batch of sheeting shall be tested.

4 3 Examination. The enema syringes shall be examined to determine compliance with all requirements contained in this specification

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

* 4 3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects as shown in Table III.

Table III.

Categories	Defects*
Major	
101	Any component missing or incomplete.
102	Sealing device at filler does not function properly.
103	Opening for hanging bag not sufficiently reinforced.
104	Tubing not permanently attached to bag.
105	Tubing not reasonably round· not free from obstruction throughout its length.
106	Tubing does not have smooth rounded tip integral.
107	Lubricant missing or not of proper consistency.
108	Opening in tip not in proper place, proper diameter or missing.
Minor	
201	Graduations missing or illegible.
202	Manufacturers name or registered trademark missing or illegible.

* 4 3.2 Dimensional examination. The enema syringes shall be examined for defects in dimensions Any dimension not within the tolerances specified herein shall be classified as a defect.

4 4 Tests. Tests shall be conducted to determine compliance with all requirements contained in this specification

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the currentversion before use.

4.4.1 Component materials. Sufficient sample of plastic material shall be selected from each lot used in the manufacture of the syringe to perform the tests specified in 4 4 2 and 4 4 3. A lot of plastic tubing or sheeting shall be defined as one continuous production run using the same batch of ingredients

4.4 2 Lead test. Ten grams of sample shall be ignited to char then further ignited in a muffle furnace at 700° centigrade (C.) to a white ash. The ash shall be boiled in 15 ml of 10 percent nitric acid filtered into a volumetric flask and made up to 100 ml. An aliquot portion equivalent to one gram of sample shall be placed in a separator The dithizone method for lead as described in the current edition of the Pharmacopeia of the United States using 5 parts per million of lead solution as a control, shall be applied

4 4.3 Toxicity. Two 2-inch squares of plastic sheeting and two 2-inch lengths of plastic tubing shall be placed in separate containers containing 100 ml of Sodium Chloride Injections U.S.P. The solution shall be autoclaved for 35 minutes at 235 degrees Fahrenheit 0 5 ml. of the solution so prepared shall be cooled and injected intravenously into each of five healthy mice weighing between 17 and 23 grams At the end of 4, 24, and 48 hours the animals shall show no discernable symptoms of toxicity If any of the animals show gross signs of toxicity or die, the test shall be repeated with five unused mice weight 20 ± 1 gram each All of the animals shall survive for 48 hours.

4 4 4 Clamp test. Sample syringes with clamps closed shall be filled to the 1500 ml. mark with water at 120° F and suspended by the hangers for 60 minutes. The syringes shall be examined for evidence of leakage and hanger rupture

4 4 5 Drop test. Sample syringes with clamps and spouts closed and filled with 1500 ml of warm water, 120° F, shall be dropped from a height of four feet onto a hard regular surface If any sample ruptures or leaks the lot shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

4 4 6 Tensile strength and elongation test. The plastic sheeting shall be tested for tensile strength and elongation in accordance with ASTM-D-882 Method of "Test for Tensile Properties of Thin Plastic Sheeting."

5 PREPARATION FOR DELIVERY

5 1 Packaging. Packaging shall be level A or C, as specified (see 6 1).

5.1 1 Unit of issue. One syringe, as specified, constitutes one unit of issue.

5 1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container as applicable for the required level of protection specified in the procurement document

Table IV Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	48 units	144 units

5 1 2 1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container such units may be packed in an exterior container of suitable size and design acceptable to a common carrier which shall insure safe delivery to destination

5 1 3 Level A.

5 1 3 1 Unit package. The tubing of each unit shall be coiled in such a manner as to prevent kinking or taking to permanent set The unit shall be further packaged in a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable Closure shall be adequate to prevent spilling of contents under normal handling

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636 type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76 Closing of bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted

5.1 4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used which will afford the degree of protection required for shipment and use of the product for its intended purpose

5 2 Packing. Packing shall be level A, B, or C, as specified. (see 6.1).

5 2 1 Level A.

5 2 1 1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3, PPP-B-601 overseas type; PPP B-621 class 2 or PPP-B-636, class weather-resistant, grade V3 Closure and strapping shall be as specified in appendix of the applicable box specification

5 2 2 Level B.

5 2 2 1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601 domestic type, PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2 3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Civil agencies. Interior and exterior containers shall be marked in accordance with FED-STD-123.

5.3.2 Military agencies.

5 3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material Contract or purchase order number, name of contractor and lot (control)number shall be shown.

5 3 2 2 Exterior container Exterior container shall be marked in accordarce with MIL-STD-129. Lot (control) number shall be shown.

6 NOTES

6 1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification
(b) Selection of applicable level of packing (see 5 1) and (5 2)

6 2 This specification covers the following item appearing in the Federal Supply Catalog

Stock No	Item Identification
6530-073-6264	Syringe, Fountain, Disposable Enema Unit

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:53Z
Check the source to verify that this is the current version before use.

6.3 This specification does not include all types, classes, grades, sizes, of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, which are normally procured to meet Federal Government requirements.

6.4 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Military custodians
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities.
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION
QQ-S-001015a(DSA-DM) PSN

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1 HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A GIVE PARAGRAPH NUMBER AND WORDING

B RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2 COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3 IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO (If "yes" in what way?)

4 REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.)

SUBMITTED BY (Printed or typed name and activity - Optional)

DATE

DD FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 64 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA PA 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS DEFENSE PERSONNEL SUPPORT CENTER
ATTN DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA PA 19101

Fold

DPSC FORM 2418
MAR 68

EDITION AUG 66 WILL BE USED UNTIL EXHAUSTED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.