GG-S-757a
AUGUST 6, 1958
SUPERSEDING
Fed. Spec. GG-S-757
July 7, 1947
(See section 6.)

FEDERAL SPECIFICATION

STETHOSCOPES

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers stethoscopes used to convey to the ear sounds produced by the body.

1.2 Classification.

1.2.1 *Types.*—Stethoscopes shall be of the following types as specified (see 6.1).

Type I.—Blood pressure, bracelet type.
Type II.—Combination type.

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND OTHER PUBLICATIONS

2.1 Specifications and standards.—The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

GG-I-526 — Instruments, Dental and Surgical; General Specifications.
QQ-B-626 — Brass, Leaded and Non-Leaded; Rods, Shapes, Forgings and Flat Products with Finished Edges Bars, Flat Wire and Strips).
ZZ-T-831—Tubing; Rubber and Plastic.
PPP-B-566 — Boxes, Folding, Paperboard.
PPP-B-585—Boxes; Wood, Wirebound.
PPP-B-601—Boxes, Wood, Cleated-Plywood.
PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636—Boxes, Fiber.
PPP-B-676 — Boxes, Set-Up, Paperboard.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging and Packing Levels.
Fed. Test Method Standard No. 151—Metals; Test Methods.
Fed. Test Method Standard No. 601—Rubber; Sampling and Testing.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL-P-116—Preservation, Methods of.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

MIL–W–530—Webbing, Textile, Cotton, General Purpose, Natural or in Colors.

MIL–B–10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

MIL–L–10547 — Liners, Case, Waterproof.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL–STD–129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publication.—The following document forms a part of this specification. Unless otherwise indicated, the issue in effect on date of invitation for bids shall apply.

American Standards Association, Standard:

ASA Z70.1–1955 (UDC615.47)—American Standard Dimensions of Glass and Metal Luer Tapers for Medical Applications.

(Application for copies should be addressed to the American Standards Association, Incorporated, 70 East Forty-Fifth Street, New York 17, N. Y.).

3. REQUIREMENTS

3.1 Material.

3.1.1 *Brass.*—Brass shall conform to the requirements of Federal Specification GG–I–526 for class 4, composition N material. As an alternate, all machinable brass shall comply with requirements of Federal Specification QQ–B–626 for composition 22 brass; and shall comply with plating and corrosion tests of Federal Specification GG–I–526 for class 4, composition N material.

3.1.2 *Carbon steel.*—Carbon steel shall be tool-steel quality, heat-treated to spring temper.

3.1.3 *Rubber tubing.*—Rubber tubing shall be commercial gum rubber tubing conforming to the applicable requirements of Federal Specification ZZ–T–831 for grade A tubing except that the specific gravity shall be a maximum of 1.40.

3.1.4 *Plastic.*—Plastic shall be black, nonshattering and shall be suitable for the purpose intended. Plastic shall be nontoxic when used for the purpose intended, and shall be free from objectionable odor.

3.1.5 All other materials hereinafter specified shall be of the best quality and suitable for the purpose intended.

3.1.6 *Webbing.*—Webbing shall be in accordance with Military Specification MIL–W–530 for type I, lightweight, ¾-inch webbing.

3.2 Construction.

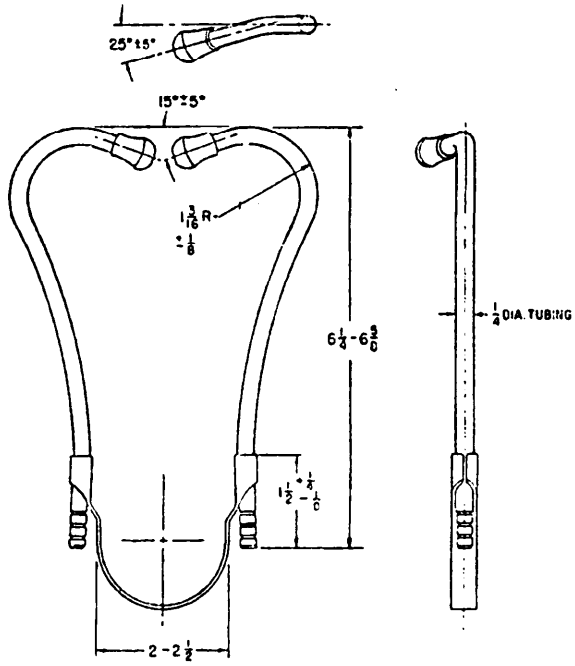


FIGURE 1.

3.2.1 *Type I.*—Type I stethoscope shall be of the conventional design and shall consist essentially of a binaural section. Y-piece adapter, chest piece, and rubber tubing.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

3.2.1.1 *Binaural section.*– Binaural section shall consist of two aural tubes, a steel spring, and two ear tips.

3.2.1.1.1 *Aural tubes.*—Aural tubes shall be fabricated from brass tubing having an outside diameter of ¼ inch and not less than 0.032-inch wall thickness (No. 21 S.G.). After shaping, each tube shall have an over-all linear length of not less than 6¼ inches. The aural end of each tube shall be threaded with 32 threads per inch for not less than ¼ inch to receive and securely hold the female threaded ear tips specified in 3.2.1.1.3. The distal ends shall be grooved or otherwise provided with suitable means for securely retaining the rubber tubing specified in 3.2.1.2. The aural tubes shall be shaped as shown in figure 1 and when assembled with the steel spring, specified in 3.2.1.1.2, the assembled tubes shall be comfortable in use. The shape of the tubes shall be such that there shall be no sharp bends or constructions of the lumens of the tubes.

3.2.1.1.2 *Steel spring.* — The aural tubes shall be permanently connected by soldering or brazing to a U-shaped steel spring approximately 6 inches in over-all length, not less than 0.028 inch thick and approximately ⅜ inch wide at the center, tapering to approximately ¼ inch at the ends. Each end of the spring shall be properly shaped to facilitate a secure connection to the aural tubes with approximately ¾-inch clearance at the end of each aural tube for securing the rubber tubing.

3.2.1.1.3 *Ear tips.*—Ear tips shall be fabricated of plastic, bulbular in shape and ⅝ inch ± ⅛ inch in length, and provided with a lumen the entire length. The lumen shall be properly threaded to securely fit the thread of the aural tubes.

3.2.1.2 *Rubber tubing.*—The rubber tubing shall be $\frac{3}{16}$-inch-inside diameter by $\frac{3}{32}$-inch wall thickness. The breaking strength and elongation of the tubing shall not decrease more than 25 percent nor shall the tubing crack, or become tacky or brittle, when subjected to the accelerated aging test specified in 4.3.1. Two 6-inch lengths and one 3-foot length of rubber tubing shall be supplied with each stethoscope.

3.2.1.3 *Y-piece.*—Y-piece shall be fabricated of brass or die-cast zinc aluminum alloy, and shall have an approximate overall length of 2¾ inches. The two upper ends of the Y-piece shall be approximately 1½ inches long and ¼ inch in outside diameter. The lower end shall be approximately 1¼ inches long and ¼ inch in outside diameter. The ends of the Y-piece shall be provided with suitable means for securely holding the rubber tubing.

3.2.1.4 *Adapter.*—The distal end of the 3-foot length of rubber tubing shall be fitted with a female Luer lock connection in accordance with figure 3 of ASA Standard Z70.1–1955. This connection shall make a leakproof fit with the connection on the chest piece specified in 3.2.1.5.1.

3.2.1.5 *Chest-piece assembly.*—Chest-piece assembly shall consist of the chest-piece body, retaining ring, diaphragm, and bracelet.

3.2.1.5.1 *Chest-piece body.* — Chest-piece body shall be fabricated of plastic. The chest piece shall be circular in shape and shall be suitably threaded to receive the diaphragm retaining ring specified in 3.2.1.5.2. As an alternate, the outer edge of the chest-piece body shall be grooved to receive a snap-on type retaining ring as an alternate specified in 3.2.1.5.2. The chest-piece body shall be supplied with a male Luer lock connection in accordance with figure 4 of ASA Standard Z70.1–1955, except that the 0.085-inch by 0.070-inch slot may be omitted. This connection shall make a leakproof fit with the adapter specified in 3.2.1.4. The chest piece body shall be provided with guides for the bracelet specified in 3.2.1.5.4.

3.2.1.5.2 *Retaining ring.*—Retaining ring shall be made of plastic threaded on the inner surface to mate with the threaded outer edge

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

of the chest piece body specified in 3.2.1.5.1. As an alternate, a snap-on type ring may be used which shall properly engage in the groove on the outer edge of the chest piece body in such a manner as not to become accidentally disengaged from chest piece specified in 3.2.1.5.1. In either case, the diaphragm as specified in 3.2.1.5.3 shall be securely held in place. The retaining ring shall be so designed that the unsupported diameter of the outside surface of the diaphragm on the assembled chest piece shall be 1 13/32 inches ± 3/32 inch.

3.2.1.5.3 *Diaphragm.* — The diaphragm shall be made of a suitable plastic, circular in shape, and shall have a diameter of suitable size to fit the retaining ring specified in 3.2.1.5.2. The thickness of the diaphragm shall be 0.013 inch ± 0.003 inch.

3.2.1.5.4 *Bracelet.*—Bracelet shall be made of webbing as specified in 3.1.6, and shall be not less than 15 inches in length. It shall be supplied with a chromium-plated metal buckle and hook.

3.2.2 *Type II.*—Type II stethoscope shall be a combination type. It shall consist essentially of a binaural section, Y-piece, and chest piece in which shall be integrally fabricated the selector valve, the bell chest piece, the diaphragm chest piece, and rubber tubing. The stethoscope shall be either the Sprague Bowles, Rieger Bowles, or Fleisher dual style.

3.2.2.1 *Binaural section.*—Binaural section shall consist of two aural tubes, a steel spring, and two ear tips.

3.2.2.1.1 *Aural tubes.*—Aural tubes shall be as specified in 3.2.1.1.1.

3.2.2.1.2 *Steel spring.*—Steel spring shall be as specified in 3.2.1.1.2.

3.2.2.1.3 *Ear tips.* —Ear tips shall be as specified in 3.2.1.1.3.

3.2.2.2 *Rubber tubing.* — Rubber tubing shall be as specified in 3.2.1.2, except that two 15-inch lengths of rubber tubing shall be supplied for the Sprague Bowles and Rieger Bowles style stethoscopes, and two 6-inch lengths and one 10-inch length of rubber tubing shall be supplied with the Fleisher dual-style stethoscope.

3.2.2.3 *Y-piece.*

3.2.2.3.1 *Sprague Bowles and Rieger Bowles styles.*—The Y-piece body shall be fabricated of brass or die-cast zinc aluminum alloy. The two upper ends of the Y-piece shall be approximately 1 inch in length and ¼ inch in diameter, and shall be provided with suitable means for securely holding the rubber tubing specified in 3.2.1.2. The Y-piece body shall widen at its central portion to provide a housing for the selector valve specified in 3.2.2.5. This portion shall also be provided with an opening to receive the Bowles chest piece specified in 3.2.2.4.1.1. The Y-piece body shall flare at the distal end. The flared end shall be threaded to receive the male threaded end of the plastic bell specified in 3.2.2.4.1.2.

3.2.2.3.2 *Fleisher dual style.*—The Y-piece shall be as specified in 3.2.1.3.

3.2.2.4 *Chest pieces.*

3.2.2.4.1 *Sprague Bowles and Rieger Bowles styles.* — The Sprague Bowles and Rieger Bowles chest pieces shall both have a Bowles diaphragm chest piece and a Sprague or Rieger bell chest piece.

3.2.2.4.1.1 *Bowles diaphragm chest piece.*—The Bowles chest piece shall consist of a chest piece body, a retaining ring, and a diaphragm. The construction of this chest piece shall be such as to accurately register high pitched sounds.

3.2.2.4.1.1.1 *Chest piece body.*—The Bowles chest piece body shall be fabricated of brass or die-cast zinc aluminum alloy and shall be permanently secured to the Y-piece body, at the selector valve, as specified in 3.2.2.3.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

The body shall be circular in shape and suitably threaded, to receive the diaphragm retaining ring specified in 3.2.2.4.1.1.2. As an alternate, the outer edge of the chest piece shall be grooved to receive a snap-on retaining ring specified as an alternate in 3.2.2.4.1.1.2.

3.2.2.4.1.1.2 *Retaining ring.* — Retaining ring shall be fabricated of brass or plastic and shall be threaded on the inner surface to mate with the threaded outer edge of the chest piece body specified in 3.2.2.4.1.1.1. As as alternate, a snap-on type ring may be used which shall properly engage in the groove on the outer edge of the chest piece in such a manner as not to become accidentally disengaged from chest piece body specified in 3.2.2.4.1.1.1. In either case the diaphragm, as specified in 3.2.2.4.1.1.3 shall be securely held in place. The retaining ring shall be so designed that the unsupported diameter of the outside surface of the diaphragm on the assembled chest piece shall be $1\frac{13}{32}$ inches $\pm$ $\frac{3}{32}$ inch,

3.2.2.4.1.1.3 *Diaphragm.*—The diaphragm shall be made of a suitable plastic, shall be circular in shape and shall have a diameter of suitable size to fit the retaining ring specified in 3.2.2.4.1.1.2. The thickness of the diaphragm shall be 0.013 inch $\pm$ 0.003 inch.

3.2.2.4.1.2 *Sprague and Rieger bell chest pieces.*—The Rieger or Sprague style bell shall be made of molded plastic and shall be threaded on the smaller end to mate with the threads on the Y-piece body. The outside surface of the bell shall be uniformly tapered from the union with the Y-piece body on the bell opening. The length of the bell and the depth of the concavity of the bell shall be consistent with either the Sprague or Rieger design, and shall be suitable for registering low pitched sounds.

3.2.2.4.2 *Fleisher dual type.*—The body of the Fleisher dual style chest piece shall be fabricated of brass or die-cast zinc aluminum alloy and shall incorporate the diaphragm chest piece body, the bell chest piece body, and the housing for the selector valve specified in 3.2.2.5. The proximal end of the body shall be provided with suitable means for making a secure attachment with the 10-inch length rubber tubing specified in 3.2.2.2.

3.2.2.4.2.1 *Diaphragm chest piece.*—The diaphragm chest piece shall consist of a diaphragm and a retaining ring. The diaphragm chest piece shall be so constructed as to accurately register high pitched sounds. The diaphragm chest piece body shall be circular in shape and shall be suitably threaded to receive the diaphragm retaining ring specified in 3.2.2.4.2.1.1. As an alternate, the outer edge of the chest piece shall be grooved to receive a snap-on retaining ring specified as an alternate in 3.2.2.4.2.1.1.

3.2.2.4.2.1.1 *Retaining ring.*—The retaining ring shall be fabricated of brass or plastic and shall be threaded on the inner surface to mate the threaded edge of the chest piece body specified in 3.2.2.4.2.1. As an alternate, a snap-on type ring may be used which shall properly engage in the groove on the outer edge of the chest piece body in such a manner as not to become accidentally disengaged from the chest piece body specified in 3.2.2.4.2.1. In either case, the diaphragm as specified in 3.2.2.4.2.1.2 shall be securely held in place. The retaining ring shall be so designed that the unsupported diameter of the outside surface of the diaphragm on the assembled chest piece shall be $1\frac{13}{32}$ inches $\pm$ $\frac{3}{32}$ inch.

3.2.2.4.2.1.2 *Diaphragm.*—The diaphragm shall be made of a suitable plastic, shall be circular in shape, and shall have a diameter of suitable size to fit the retaining ring specified in 3.2.2.4.2.1.1. The thickness of the diaphragm shall be 0.013 inch $\pm$ 0.003 inch.

3.2.2.4.2.2 *Bell chest piece.*—The bell shall be fabricated of plastic and shall be threaded on the smaller end to mate with the thread on the chest piece body. The outside surface of the bell shall be uniformly tapered for the union with the chest piece body to the bell

Source: https://assist.dla.mil -- Downloaded: 20260-26T11:53Z
Check the source to verify that this is the currentversion before use.

opening, and shall be properly designed to accurately register low pitched sounds.

3.2.2.5 *Selector valve.*—A selector valve shall be incorporated in the Y-piece body of the Sprague Bowles and Rieger Bowles styles and in the combination chest piece of the Fleisher dual style which shall serve to connect to the binaural section the desired chest piece and to completely eliminate sounds from the chest piece not in use. The selector valve shall be a tapered and ground valve to assure a perfect and soundproof fit. The Y-piece body of the Sprague Bowles and Rieger Bowles styles and the Fleisher dual combination chest piece shall be suitably marked to indicate the position of the valve for selection of a desired chest piece.

3.3 Finish. — All brass and carbon-steel components shall be chromium plated over nickel. Where die cast alloys are used, these components shall be given a black lacquered finish.

3.4 Identification marking. — The chest piece of the stethoscope shall be permanently and legibly marked with the manufacturer's name or registered trade-mark.

3.5 Corrosion-resistance.—All metal parts (other than those given a lacquered finish) shall not show evidence of corrosion exceeding 2 percent, when tested as specified in 4.3.2.

3.6 Workmanship.—Workmanship shall be first class throughout. Stethoscopes shall be free from defects which detract from their appearance or may impair their serviceability. All parts which are joined by soldering shall be silver soldered.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.*—Sampling procedures for visual examination shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

4.1.2 *For tests.*

4.1.2.1 *Raw material.*—Four ounces of each metal, representative of each lot used in the manufacture of the end item, shall be selected for determining chemical composition.

4.1.2.2 *End item.*—Sample size for each test shall be as indicated for inspection level L2 in Appendix to Military Standard MIL–STD–105, except that the acceptance number shall be zero (0) for all sample sizes, and a minimum of three (3) samples shall be taken regardless of lot size.

4.1.2.3 *Components.*—Except as otherwise indicated herein, components in the end items selected in accordance with 4.1.2.2 above, shall be subjected to specified tests.

4.2 Inspection.—The inspector shall ascertain that the stethoscopes have been examined and tested in accordance with specification requirements.

4.3 Tests.

4.3.1 *Accelerated aging test.*—The rubber tubing shall be subjected to the air heat test in accordance with Method 7221 of Federal Test Method Standard No. 601. Straight specimens shall be used for testing the tubing, and dumbell specimens shall be used for testing the arm bag.

4.3.2 *Corrosion-resistance.* — All metal parts (other than those given a lacquered finish) shall, before testing, be scrubbed with soap and water, rinsed thoroughly, and dried. After cleaning, they shall be boiled in distilled water in a glass beaker for 30 minutes and allowed to remain submerged for 24 hours. Samples of only the same components shall be boiled in the same vessel. The parts shall then be inspected for evidence of corrosion.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:53Z
Check the source to verify that this is the current version before use.

4.3.3 *Chemical composition of metals.*—Tests for determination of chemical composition of metal parts shall be conducted in accordance with method 111 or 112 of Federal Test Method Standard No. 151.

4.4 **Supplier responsibilities for inspection.**—The supplier shall perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government, upon the Government's request, at any time, or from time to time, for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

5. PREPARATION FOR DELIVERY

Levels of preservation, packaging, and packing protection used are defined in Fed. Std. No. 102 (for civil agencies only).

5.1 **Packaging.**

5.1.1 *Unit of issue.*—One stethoscope, as specified, constitutes one unit.

5.1.2 *Quantities.*—Packaging and packing quantities shall be as specified in table I.

5.1.2.1 *Packing variation permitted.*—If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676. Carton shall be adequately secured to prevent accidental opening. Each unit shall be further packaged in accordance with Method IA-2 or IA-8 of Military Specification MIL-P-116.

5.1.3.2 *Intermediate package.*—The number of units specified in table I shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566, PPP-B-636, or PPP-B-676. Carton shall be adequately secured to prevent accidental opening.

5.1.4 *Level B.*

5.1.4.1 *Unit package.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676. Carton shall be adequately secured to prevent accidental opening.

5.1.4.2 *Intermediate package.*—The number of units specified in table I shall be packaged in a carton of appropriate size and design, or shall be completely wrapped with kraft paper of suitable weight. Carton or wrapping shall be adequately secured to prevent accidental opening.

TABLE I.—*Packaging and packing quantities*

Federal Stock Number	Unit Pack	Intermediate pack	Shipping container
6515-374-2200	1 unit	Not required	48 units
6515-374-2220	1 unit	6 units	96 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

5.1.5 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used for the purpose, which will afford the degree of protection required for shipment and use of the end product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—The number of units specified in table I shall be overpacked in an exterior container designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; PPP–B–621, table III; or Military Specification MIL–B–10377, table II.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.*—Strapping (when required) shall be in accordance with the applicable box specification.

Note—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—The number of units specified in table I shall be overpacked in an exterior container conforming to Federal Specification PPP–B–601, table I, using class 1 plywood; or an exterior container designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 2 use; PPP–B–621, table I; or Military Specification MIL–B–10377, table I.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *Interior packages.*—Each unit carton and barrier, and each intermediate carton shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 Ordering data. — Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title number and date of this specification.

(*b*) Type required (see 1.2).

(*c*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

(1) Level B packaging is intended to provide economical but limited protection, and should be specified only when it is determined the stethoscopes will be held in covered storage approximately twelve (12) months from date of initial packaging.

6.2 Storage surveillance.—Items packaged in accordance with level B requirements must be inspected to determine condition when not used within the time period indicated in 6.1(c)(1). Items not used within the time

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

period specified must be repackaged in accordance with level B requirements in this specification or with level A requirements if storage beyond an additional year is anticipated.

6.3 This specification covers the following items appearing in the Armed Services Medical Stock List:

6515-374-2200 STETHOSCOPE, Blood Pressure, Bracelet Type.

6515-374-2220 STETHOSCOPE, Combination Type.

6515-374-2325 CHEST PIECE, STETHOSCOPE.

6515-374-2330 TIP, EAR, STETHOSCOPE.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.5 **Transportation description.**—The transportation description applicable to these items is:

Type I

Surgical instruments, not otherwise indexed by name.

Carload minimum weight 10,000 pounds, subject to Rule 34, Uniform Freight Classification.

Motor volume minimum weight 10,000 pounds.

Type II

Rubber goods, not otherwise indexed by name.

Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Motor volume minimum weight 20,000 pounds.

6.6 **Supersession data.**—This specification supersedes Military Specification MIL-S-16530 (BuMed), dated 15 August 1951.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:

Army—M
Navy—Md
Air Force.

Copies of this specification may be purchased for 10 cents each.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:53Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION

ORGANIZATION *(Of submitter)* | CITY AND STATE

CONTRACT NO. | QUANTITY OF ITEM PROCURED | DOLLAR AMOUNT
$

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)* | DATE

DD FORM 1 APR 63 1426 REPLACES NAVSHIPS FORM 4863, WHICH IS OBSOLETE PLATE NO. 15419

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:53Z
Check the source to verify that this is the current version before use.

FOLD

)EPARTMENT OF THE NAVY

POSTAGE AND FEES PAID
NAVY DEPARTMENT

OFFICIAL BUSINESS

COMMANDER
DEFENSE PERSONNEL SUPPORT CENTER (MED.)
2800 S. 20TH ST.
PHILA., PA. 19101

FOLD

PLATE NO. 15419 (B

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

5098 .N1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

NOTICE OF CANCELLATION

GG-S-757A
NOTICE 1
7 October 1991

FEDERAL SPECIFICATION

STETHOSCOPE

GG-S-757A, dated August 6, 1958, is hereby cancelled without replacement.

Preparing Activity:
DoD-MB
(Project No. 6515-5301)

AMSC N\A FSC 6515

DISTRIBUTION STATEMENT A. Approval for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:53Z
Check the source to verify that this is the current version before use.