A-A-54024
13 November 1989

COMMERCIAL ITEM DESCRIPTION

FILES AND REAMERS, PULP CANAL, DENTAL, STANDARDIZED

The General Services Administration has authorized the use of this Commercial Item Description as a replacement to Federal Specification GG-F-00336G which is cancelled.

This commercial item description covers standardized pulp canal files and reamers for use in endodontic procedures.

Salient characteristics:

Except as noted below, the files and reamers shall be in accordance with ANSI (American National Standards Institute)/ADA (American Dental Association) Specification No. 28. In case of a conflict, this document shall govern.

Classification. Files and reamers shall be classified in the following types, classes and sizes.

Type I - Reamers
Type II - Files
Type III - File set

Class 1 - 21 millimeter (mm) operative end
Class 2 - 25 mm operative end
Class 3 - 30 mm operative end

Sizes - 8, 10, 15, 20, 25, 30, 35, 40, 45, 50, 55, 60, 70, 80, 90, 100, 110, 120, 130, 140

Material.

Operative end. The operative end of the files and reamers shall be fabricated from stainless steel type 302 (maximum silicon content shall be 1.40%), type 304 vacuum melted or type 631 in accordance with ASTM Designation F899 for composition. Composition shall be tested as specified herein.

AMSC N/A FSC 6520
DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Handles. Handles shall be fabricated of plastic material which is rigid and of a quality suitable to withstand normal operative procedures. Handles shall be capable of being autoclaved and dry heat sterilized without losing the shape of the handle or bleaching out the color when sterilized as specified in ADA Specification No. 28.

Tensile strength. The tensile strength of the operative ends of the files and reamers shall conform to the requirements below for the respective material and file or reamer size listed. Files and reamers shall be tested for tensile strength as specified herein.

Tensile strength

Material	File sizes	Reamer sizes	Tensile strength (pounds per square inch)
302 (Si,1.4% max)	8,10,15 and 20	10,15 and 20	310,000 minimum
	25 through 80	25 through 80	270,000 to 380,000
	90 through 140	90 through 100	240,000 to 380,000
304	8 through 20	10 through 20	290,000 minimum
	25 through 55	25 through 55	270,000 minimum
	60 through 80	60 through 80	267,000 minimum
	90 through 140	90 through 100	258,000 minimum
361	8		310,000 minimum
	10 through 55	10 through 55	260,000 to 330,000

Design and dimensions. Files and reamers shall be of the standardized system conforming to the dimensions specified herein and in ADA Specification No. 28. Files and reamers shall be of two-piece construction consisting of an operative end and a handle.

File set. Unless otherwise specified, the file assortment set shall consist of 15 files, 1 each of sizes 10 through 100 of the files listed under classification. The file sets shall be furnished with class 3 operative ends.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Operative ends. Operative ends of instruments shall be made of stainless steel wire conforming to the requirements specified under materials. The operative ends shall be smoothly finished, uniformly twisted in spirals to form the cutting edges, and shall taper to a fine point. The twisted operative lengths shall form a sharp cutting instrument and shall have triangular or square cross-sectional configurations. Operative ends of class 1 instruments shall be 21 ± 1 mm in length. Class 2 instruments shall have operative ends 25 ± 1 mm in length and class 3 instruments shall have operative ends 30 ± 1 mm in length.

Handles. Operative ends of files and reamers shall be securely and permanently affixed in the handles with no movement of operative ends permitted. The entire handle shall be longitudinally serrated or shall have cross cut serrations. As an alternate, only the finger gripping portion shall be serrated. The handle shall be in accordance with Figure 1 of this description.

Finish. The spiral section of the operative end of the file shall have a bright and smooth finish. The instrument shall be uniform and free from burrs, scales, rough areas and grind marks.

Identification marking. The handle shall be color coded and numbered with the respective size. Size and color shall be in accordance with ANSI/ADA specification No. 28.

Workmanship. Files and reamers shall be properly constructed and finished and shall be free from defects which may detract from their appearance or impair their serviceability.

Certification. Suppliers shall furnish at time of award a dated certificate and data showing that the dental file or reamer they propose to furnish is the same in quality and brand as that appearing on the list of certified materials for American Dental Association Specification No. 28 for endodontic files and reamers, type K. Type I of this specification shall be certified for type I of ADA specification No. 28 and types II and II of this specification shall be certified for type II of ADA specification No. 28. Compliance with this certification requirement does not absolve the contractor from complete compliance with the requirements of this specification.

Unit. Package (PG). One package containing six pulp canal files or reamers of the type, class and size specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Unit package. One package containing six files or reamers of the type class and size specified or one set containing fifteen files of one class shall be packaged in a plastic tray with a clear plastic slip-over or hinged cover. The tray shall be designed with six or fifteen cavities or inserts as applicable to hold each file or reamer in such a manner so as to prevent movement and damage to the operative ends. The cover shall be secured with tape.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (with visual inspection at 2x magnification or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an inspection level of S-2. The unit of product for examination purposes shall be one unit of issue as specified in this description.

Examination. Examination shall be as specified herein. Examination shall include, but shall not be limited to the following:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Defects

Type, class, and size not as specified.
Assortment not as specified.
Design not as specified.
Quantity (unit of issue) not as specified.
Files and reamers not of two-piece construction.
Cutting edge not sharp.
Spiral section of operative end does not have a bright, smooth finish.
Operative ends not firmly affixed in the handles.
Laminations or cracks, bends, deformed portions, gouges, chips, or broken areas present in any part of file or reamer.
Handle not rigid.
Finish of handle not as specified.
Color coding and size number marking not present on handle or incorrect.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as specified below. The unit product for test purposes shall be one unit of issue.

Test criteria

Component	Characteristic	Inspection level
Steel stock	Composition	*
	Tensile strength	*
Operative ends	Resistance to fracture by twisting	S-2
	Stiffness	S-2
	Corrosion resistance	S-2
	Dimensions	S-2
Handles	Sterilization tests	**
	Dimensions	S-2

*A sufficient quantity of each lot of raw material used in the fabrication of the files shall be selected for testing.

**Separate S-2 level quantities for both autoclave and dry heat tests.

Tests. Tests, as specified herein or in ADA specification No. 28, shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Chemical analysis. In the absence of certificates of quality, chemical analysis of the raw material shall be determined in accordance with Method 111 of FED-STD-151.

Tensile strength. Tensile strength shall be performed in a tension tester on an 8-inch sample of steel stock used to produce the file or reamer.

Dimensions. All file and reamer dimensions listed in this description or in ADA specification No. 28 shall be measured using a shadowgraph, measuring microscope, or other suitable device capable of measuring these dimensions with the accuracy specified.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pounds units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

National Stock Number	Item Identification	Specification Designation			Unit of Issue
		Type	Class	Size	
6520-00-133-1905	FILE, PULP CANAL, DENTAL, Standardized, 1-7/16 inch, set of 15	III	3		Set
6520-00-850-4919	REAMER, PULP CANAL, DENTAL, Standardized, Size 10, 6s	I	2	10	Pkg
6520-00-850-4920	REAMER, PULP CANAL, DENTAL, Standardized, Size 15, 6s	I	2	15	Pkg
6520-00-850-4921	REAMER, PULP CANAL, DENTAL, Standardized, Size 20, 6s	I	2	20	Pkg
6520-00-850-4922	REAMER, PULP CANAL, DENTAL, Standardized, Size 25, 6s	I	2	25	Pkg
6520-00-850-4923	REAMER, PULP CANAL, DENTAL, Standardized, Size 30, 6s	I	2	30	Pkg

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

6520-00-890-4924	REAMER, PULP CANAL, DENTAL, Standardized, Size 35, 6s	I	2	35	Pkg
6520-00-890-4925	REAMER, PULP CANAL, DENTAL, Standardized, Size 40, 6s	I	2	40	Pkg
6520-00-890-4926	REAMER, PULP CANAL, DENTAL, Standardized, Size 45, 6s	I	2	45	Pkg
6520-00-890-4927	REAMER, PULP CANAL, DENTAL, Standardized, Size 50, 6s	I	2	50	Pkg
6520-00-890-4928	REAMER, PULP CANAL, DENTAL, Standardized, Size 55, 6s	I	2	55	Pkg
6520-00-890-4929	REAMER, PULP CANAL, DENTAL, Standardized, Size 60, 6s	I	2	60	Pkg
6520-00-890-4930	REAMER, PULP CANAL, DENTAL, Standardized, Size 70, 6s	I	2	70	Pkg
6520-00-890-4931	REAMER, PULP CANAL, DENTAL, Standardized, Size 80, 6s	I	2	80	Pkg
6520-00-890-4932	REAMER, PULP CANAL, DENTAL, Standardized, Size 90, 6s	I	2	90	Pkg
6520-00-890-4933	REAMER, PULP CANAL, DENTAL, Standardized, Size 100, 6s	I	2	100	Pkg
6520-00-850-5119	FILE, PULP CANAL, DENTAL, Standardized, Size 10, 6s	II	2	10	Pkg
6520-00-850-5120	FILE, PULP CANAL, DENTAL, Standardized, Size 15, 6s	II	2	15	Pkg

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

6520-00-850-5121	FILE, PULP CANAL, DENTAL, Standardized, Size 20, 6s	II	2	20	Pkg
6520-00-850-5122	FILE, PULP CANAL, DENTAL, Standardized, Size 25, 6s	II	2	25	Pkg
6520-00-850-5123	FILE, PULP CANAL, DENTAL, Standardized, Size 30, 6s	II	2	30	Pkg
6520-00-850-5124	FILE, PULP CANAL, DENTAL, Standardized, Size 35, 6s	II	2	35	Pkg
6520-00-850-5125	FILE, PULP CANAL, DENTAL, Standardized, Size 40, 6s	II	2	40	Pkg
6520-00-850-5126	FILE, PULP CANAL, DENTAL, Standardized, Size 45, 6s	II	2	45	Pkg
6520-00-850-5127	FILE, PULP CANAL, DENTAL, Standardized, Size 50, 6s	II	2	50	Pkg
6520-00-850-5128	FILE, PULP CANAL, DENTAL, Standardized, Size 55, 6s	II	2	55	Pkg
6520-00-850-5129	FILE, PULP CANAL, DENTAL, Standardized, Size 60, 6s	II	2	60	Pkg
6520-00-850-5130	FILE, PULP CANAL, DENTAL, Standardized, Size 70, 6s	II	2	70	Pkg
6520-00-850-5131	FILE, PULP CANAL, DENTAL, Standardized, Size 80, 6s	II	2	80	Pkg
6520-00-850-5132	FILE, PULP CANAL, DENTAL, Standardized, Size 90, 6s	II	2	90	Pkg

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

6520-00-850-5133	FILE, PULP CANAL, DENTAL, Standardized, Size 100, 6s	II	2	100	Pkg
6520-01-018-8990	FILE, PULP CANAL, DENTAL, Standardized, Size 10, 6s	II	1	10	Pkg
6520-01-018-8991	FILE, PULP CANAL, DENTAL, Standardized, Size 15, 6s	II	1	15	Pkg
6520-01-019-0859	FILE, PULP CANAL, DENTAL, Standardized, Size 20, 6s	II	1	20	Pkg
6520-01-019-0860	FILE, PULP CANAL, DENTAL, Standardized, Size 25, 6s	II	1	25	Pkg
6520-01-019-0861	FILE, PULP CANAL, DENTAL, Standardized, Size 30, 6s	II	1	30	Pkg
6520-01-019-0862	FILE, PULP CANAL, DENTAL, Standardized, Size 35, 6s	II	1	35	Pkg
6520-01-019-0863	FILE, PULP CANAL, DENTAL, Standardized, Size 40, 6s	II	1	40	Pkg
6520-01-019-0864	FILE, PULP CANAL, DENTAL, Standardized, Size 45, 6s	II	1	45	Pkg
6520-01-019-0865	FILE, PULP CANAL, DENTAL, Standardized, Size 50, 6s	II	1	50	Pkg
6520-01-019-0866	FILE, PULP CANAL, DENTAL, Standardized, Size 55, 6s	II	1	55	Pkg
6520-01-019-0867	FILE, PULP CANAL, DENTAL, Standardized, Size 60, 6s	II	1	60	Pkg

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

6520-01-019-0868	FILE, PULP CANAL, DENTAL, Standardized, Size 70, 6s	II	1	70	Pkg
6520-01-067-1229	FILE, PULP CANAL, DENTAL, Standardized, Size 130, 6s	II	2	130	Pkg
6520-01-067-1230	FILE, PULP CANAL, DENTAL, Standardized, Size 130, 6s	II	3	130	Pkg
6520-01-067-1231	FILE, PULP CANAL, DENTAL, Standardized, Size 140, 6s	II	2	140	Pkg
6520-01-067-1232	FILE, PULP CANAL, DENTAL, Standardized, Size 140, 6s	II	3	140	Pkg
6520-01-067-1233	FILE, PULP CANAL, DENTAL, Standardized, Size 8, 6s	II	1	8	Pkg
6520-01-067-1234	FILE, PULP CANAL, DENTAL, Standardized, Size 120, 6s	II	2	120	Pkg
6520-01-067-1235	FILE, PULP CANAL, DENTAL, Standardized, Size 120, 6s	II	3	120	Pkg
6520-01-067-3086	FILE, PULP CANAL, DENTAL, Standardized, Size 110, 6s	II	2	110	Pkg
6520-01-070-1515	FILE, PULP CANAL, DENTAL, Standardized, Size 110, 6s	II	3	110	Pkg

Ordering data. Intermediate/exterior package quantities, labeling and marking must be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

A-A-54024

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
PHS
FDA-MPQAS

PROJECT NO. 6520-2295
LOCATION: NCR DISK 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.

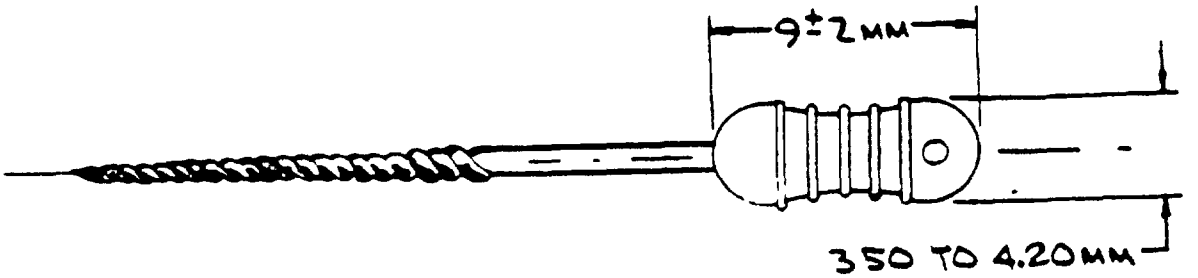

HANDLE
(PLASTIC)

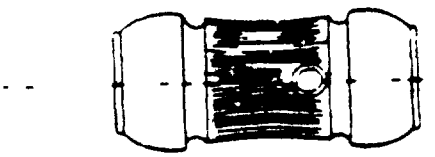

ALTERNATE HANDLE

NOTES:
Handles shall be in strict accordance with this figure for dimensional requirements. The style and design of the handles shown above are typical and are not intended to restrict or preclude the purchase of files and reamers which are otherwise in accordance with the requirements of this commercial item description.

FIGURE 1 : HANDLE, FILES AND REAMERS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:28Z
Check the source to verify that this is the current version before use.